

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
 Data File : FF010181.D
 Signal(s) : FID2B.ch
 Acq On : 27 Mar 2022 05:42
 Operator : AJ\MA
 Sample : N2119-05 10X
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 27 06:09:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
 Quant Title :
 QLast Update : Sat Mar 26 09:58:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

4)	N-TETRADECANE	8.198	485072	3.462 ug/ml
5)	N-HEXADECANE	9.798	4541926	32.230 ug/ml
6)	N-OCTADECANE	11.212	22624722	156.978 ug/ml
7)	N-EICOSANE	12.554	9359563	66.938 ug/ml
15)	N-TETRATRIACONTANE	19.353	344339	3.188 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010181.D
Signal(s) : FID2B.ch
Acq On : 27 Mar 2022 05:42
Operator : AJ\MA
Sample : N2119-05 10X
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 27 06:09:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

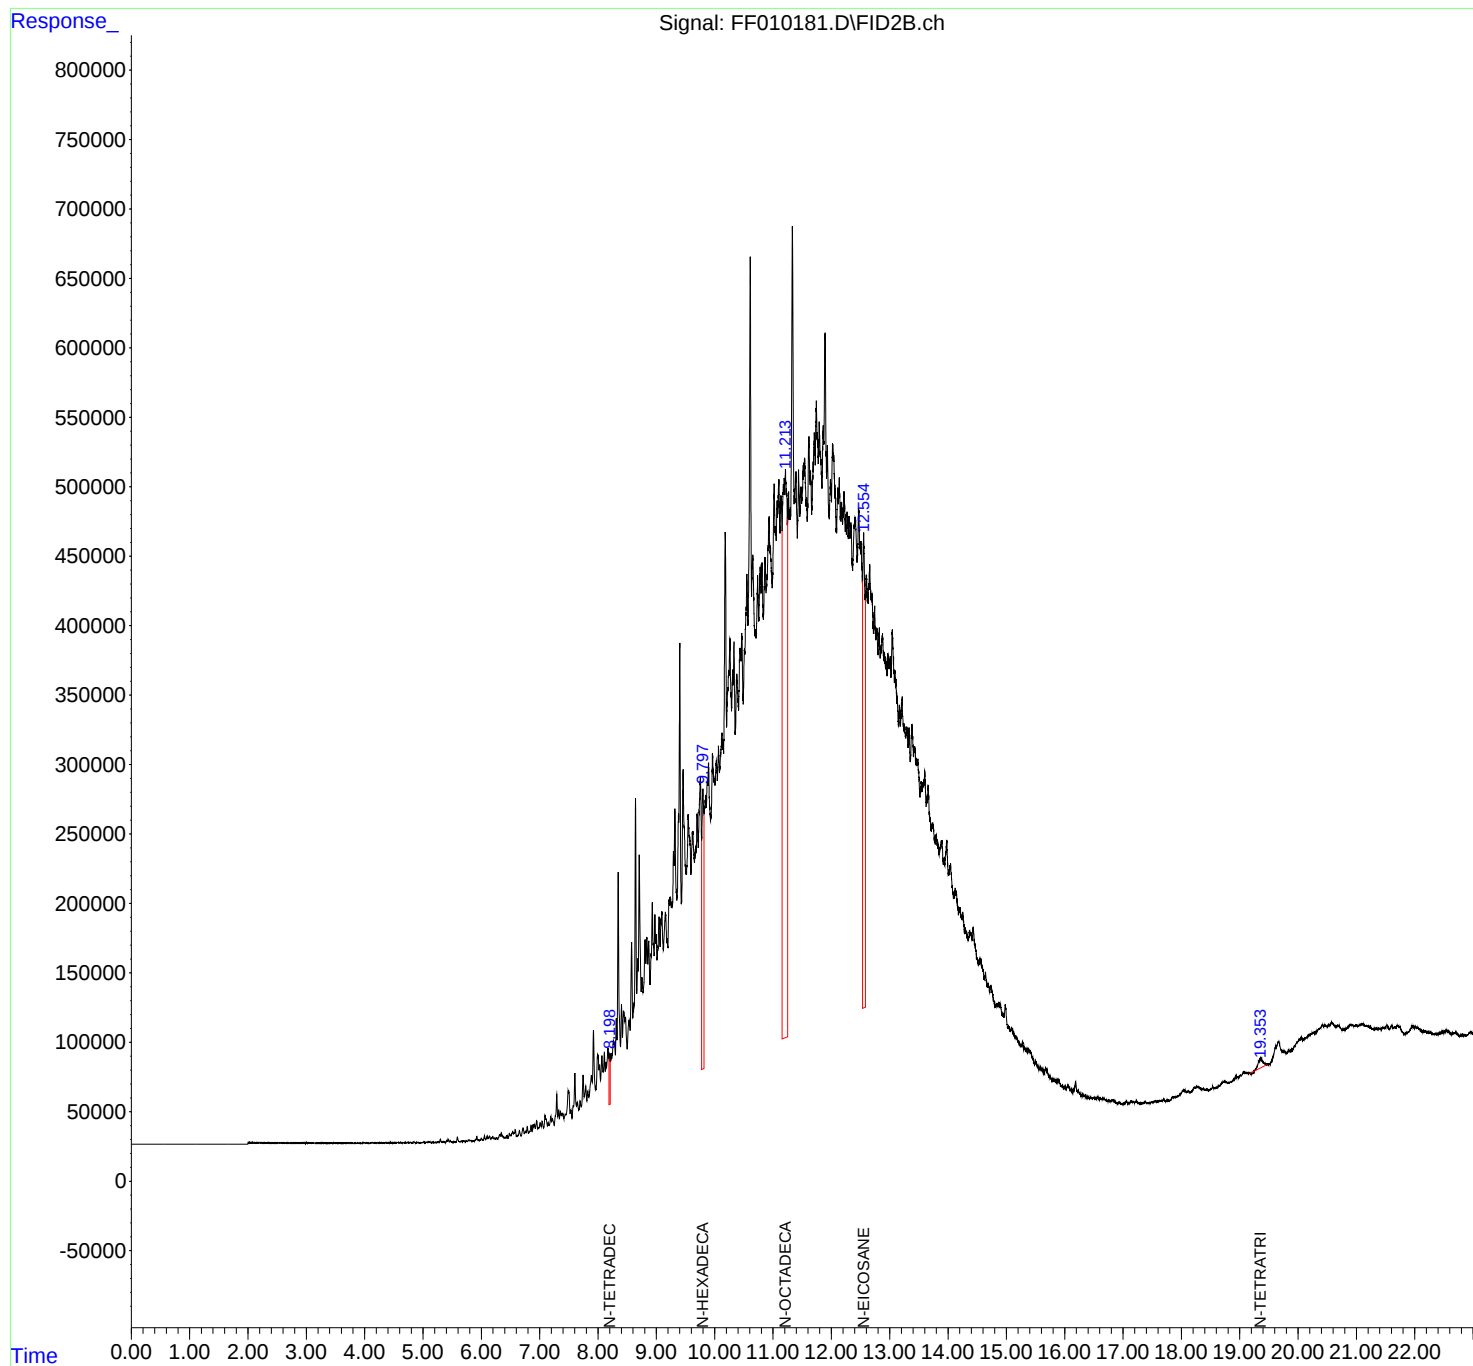


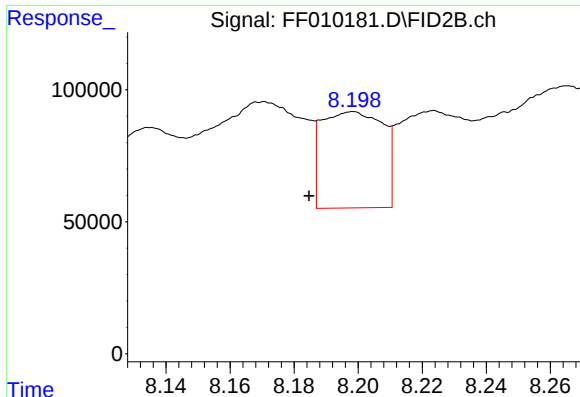

#4 N-TETRADECANE


R.T.: 8.198 min
Delta R.T.: 0.013 min
Response: 485072
Conc: 3.46 ug/ml

Instrument :
FID_F
ClientSampleId :

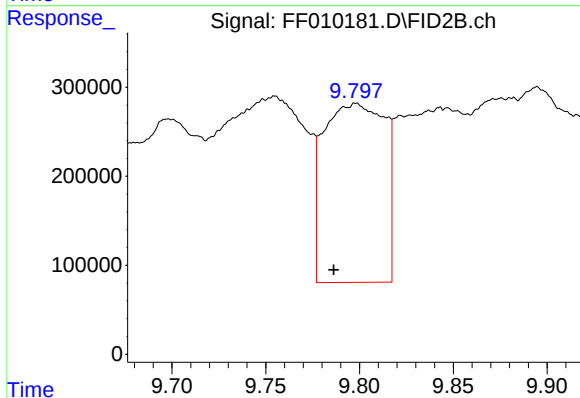


#5 N-HEXADECANE

R.T.: 9.798 min
Delta R.T.: 0.011 min
Response: 4541926
Conc: 32.23 ug/ml

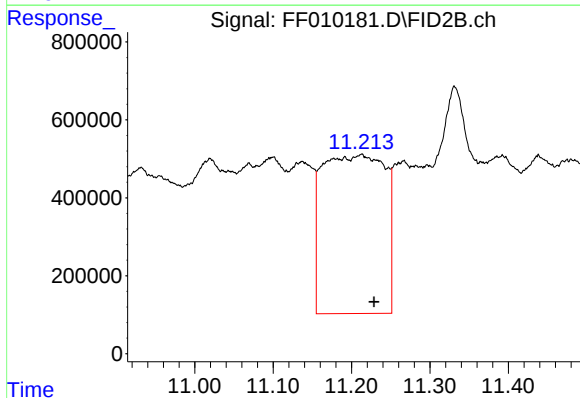


#6 N-OCTADECANE

R.T.: 11.212 min
Delta R.T.: -0.016 min
Response: 22624722
Conc: 156.98 ug/ml

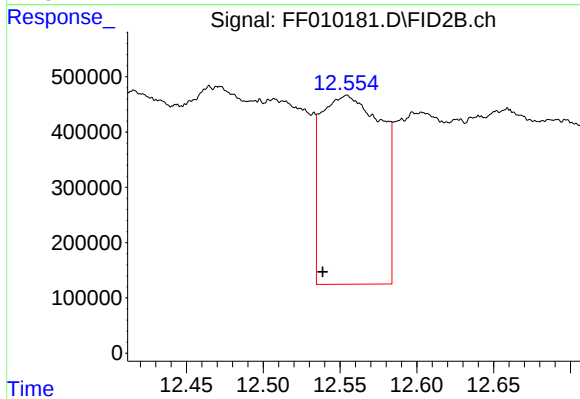

#7 N-EICOSANE


R.T.: 12.554 min
Delta R.T.: 0.015 min
Response: 9359563
Conc: 66.94 ug/ml

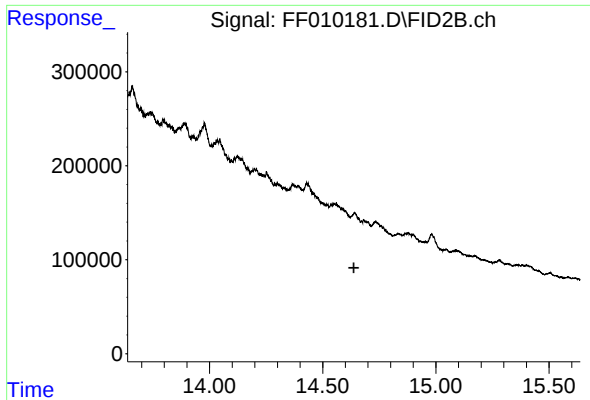

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.638 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

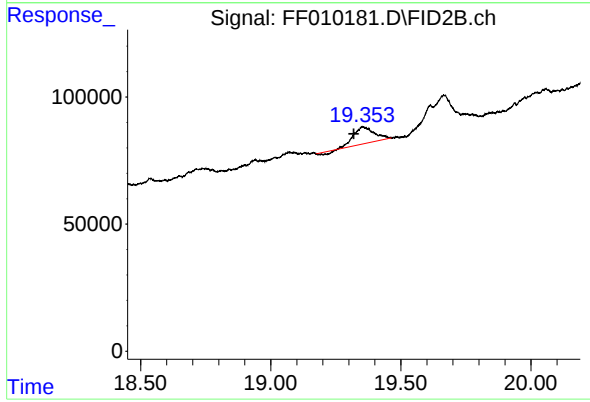

#15 N-TETRATRIACONTANE

R.T.: 19.353 min
Delta R.T.: 0.034 min
Response: 344339
Conc: 3.19 ug/ml