

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010170.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2022 23:39
Operator : AJ\MA
Sample : N1958-07 20X
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
C-7-6-7

Integration File: autoint1.e
Quant Time: Mar 27 01:04:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010170.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2022 23:39
Operator : AJ\MA
Sample : N1958-07 20X
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
C-7-6-7

Integration File: autoint1.e
Quant Time: Mar 27 01:04:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

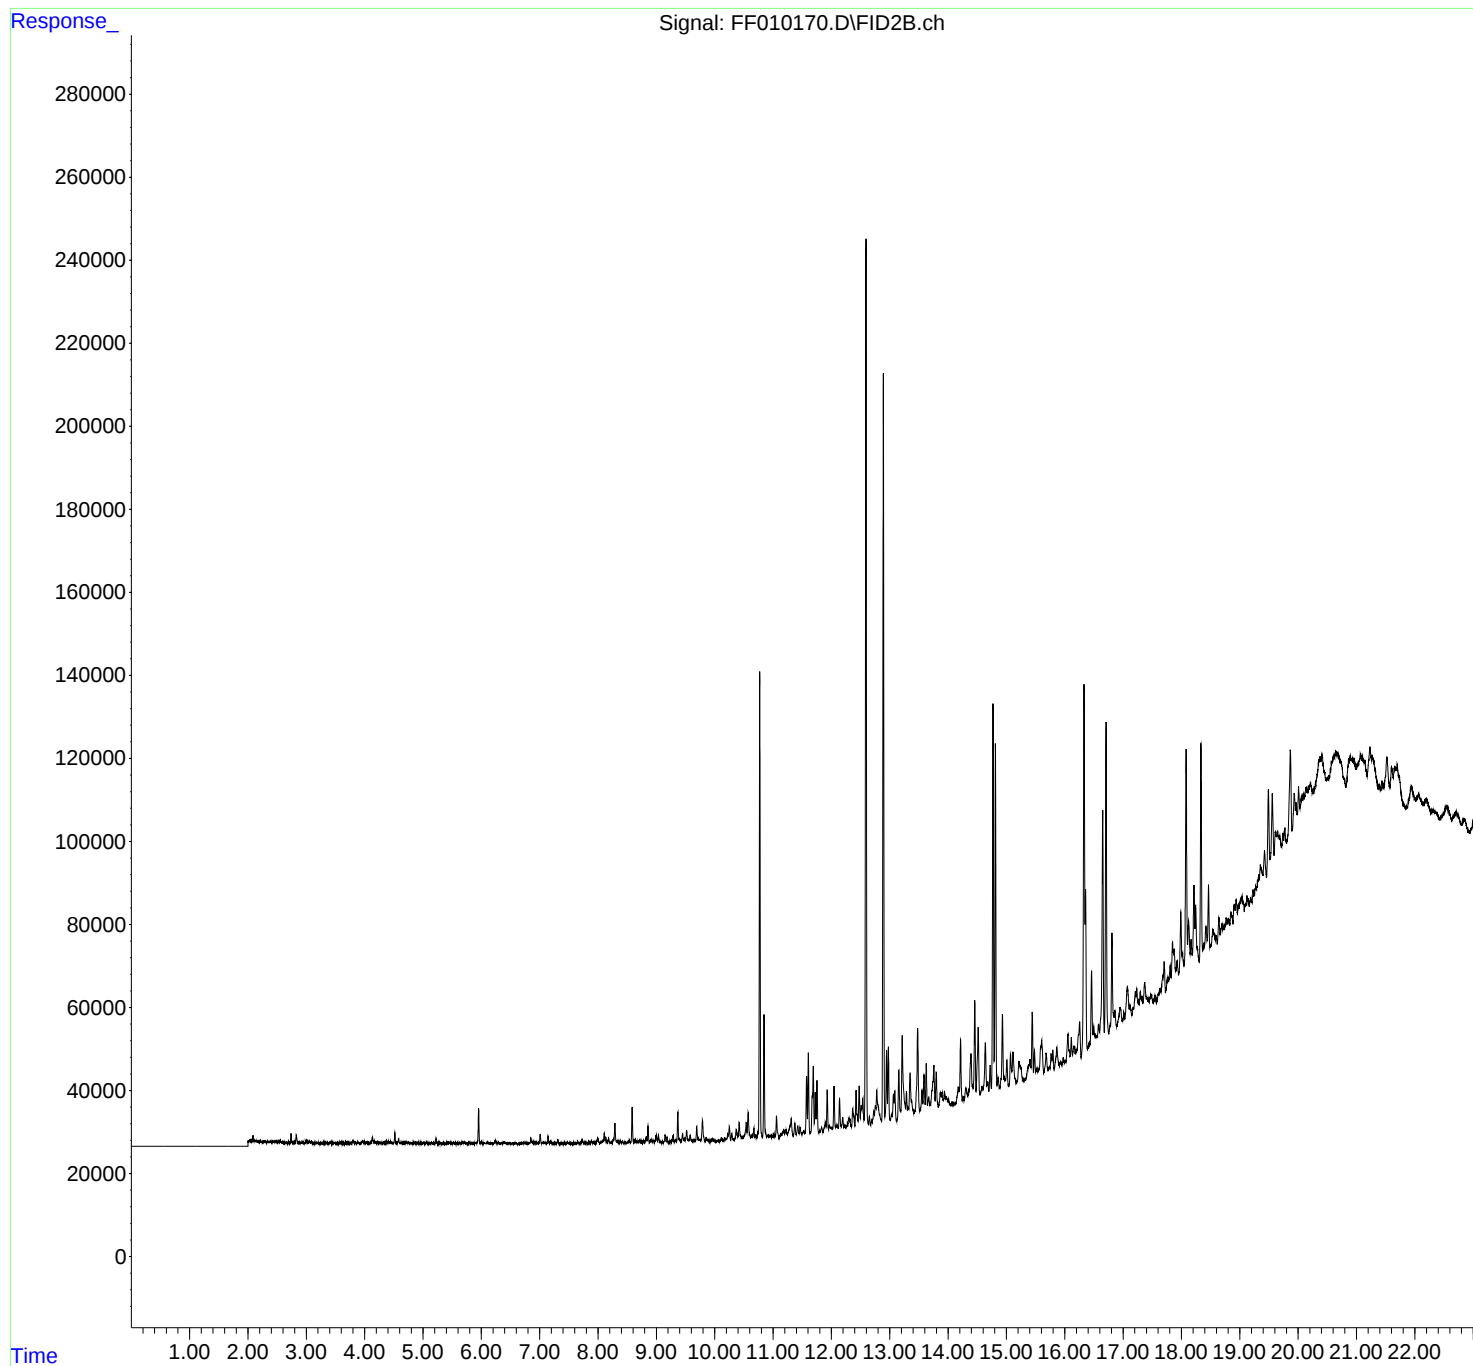

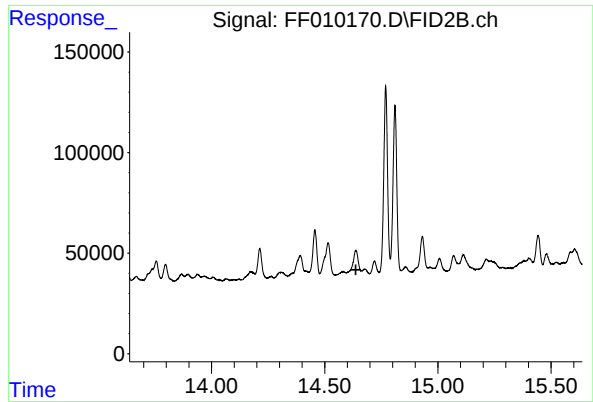

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.638 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
C-7-6-7