

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032625\
Data File : FF015729.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2025 09:27
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Mar 26 15:14:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032625.M
Quant Title :
QLast Update : Wed Mar 26 13:03:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13)	N-TRIACONTANE	18.094	46986	0.381 ug/ml
14)	N-DOTRIACONTANE	18.929	66240	0.561 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032625\
Data File : FF015729.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2025 09:27
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Mar 26 15:14:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032625.M
Quant Title :
QLast Update : Wed Mar 26 13:03:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

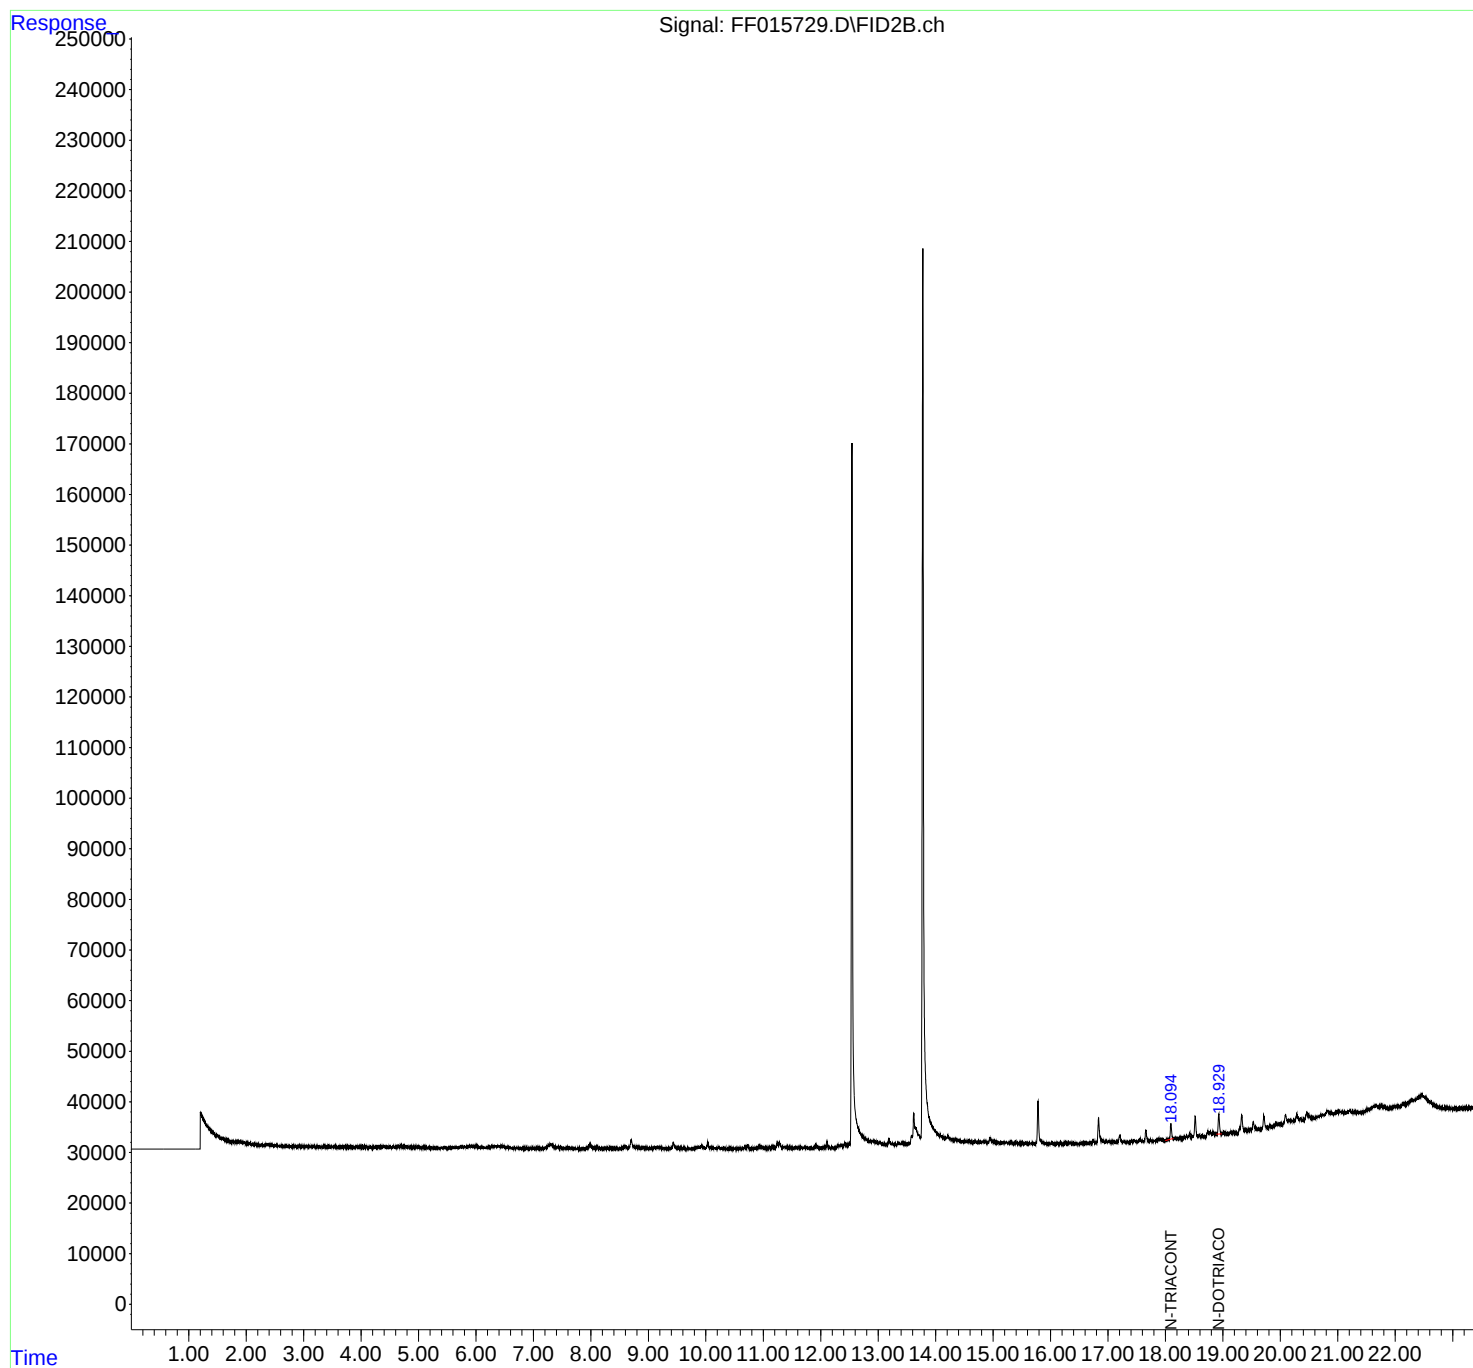


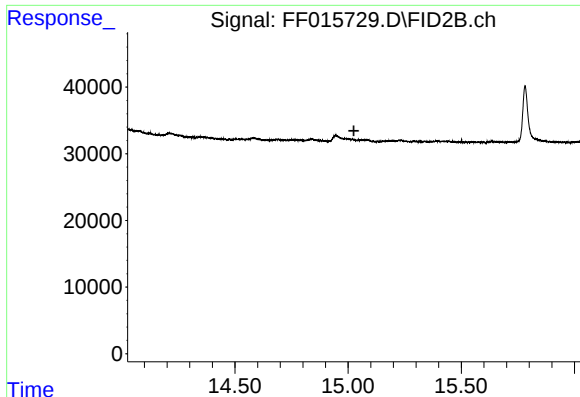

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.025 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
MECL2

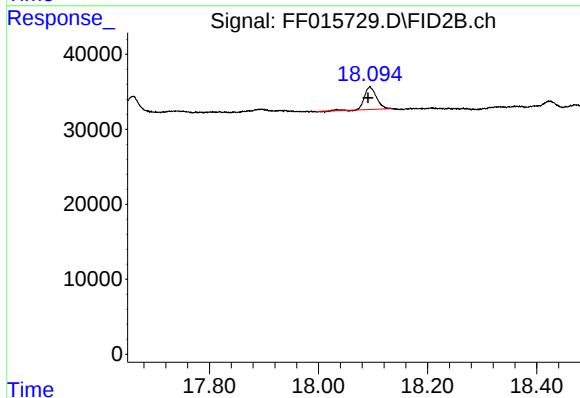

#13 N-TRIACONTANE

R.T.: 18.094 min
Delta R.T.: 0.004 min
Response: 46986
Conc: 0.38 ug/ml

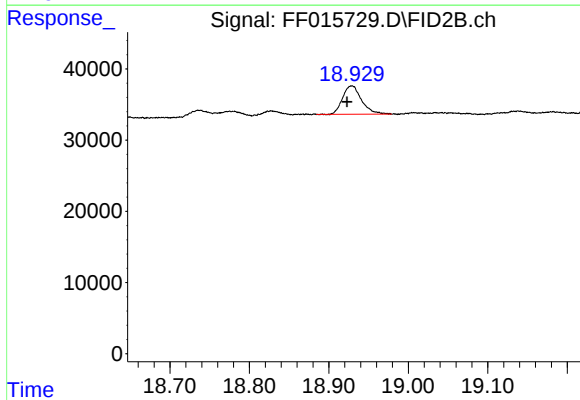

#14 N-DOTRIACONTANE

R.T.: 18.929 min
Delta R.T.: 0.006 min
Response: 66240
Conc: 0.56 ug/ml