

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032625\
Data File : FF015730.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2025 09:56
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 26 15:13:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032625.M
Quant Title :
QLast Update : Wed Mar 26 13:03:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.023	2155881	19.674 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.932	57889	0.490 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032625\
Data File : FF015730.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2025 09:56
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 26 15:13:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032625.M
Quant Title :
QLast Update : Wed Mar 26 13:03:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

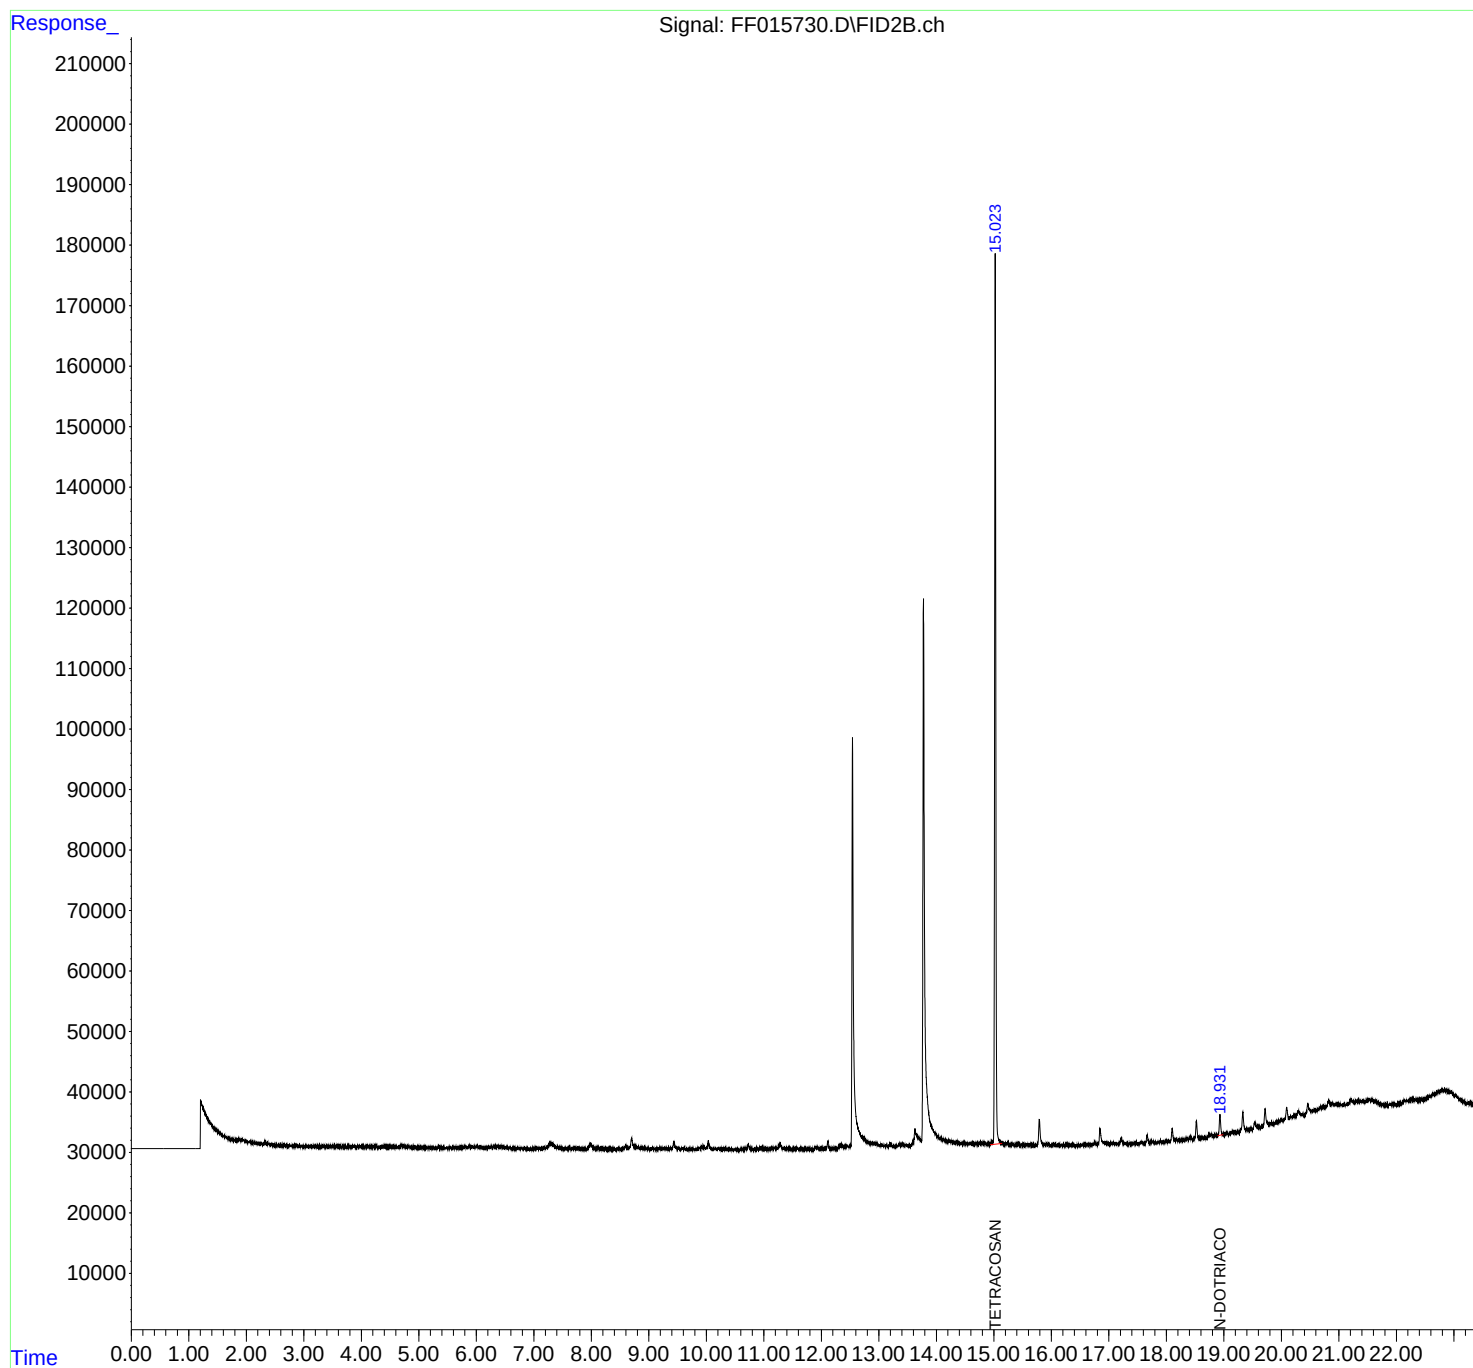


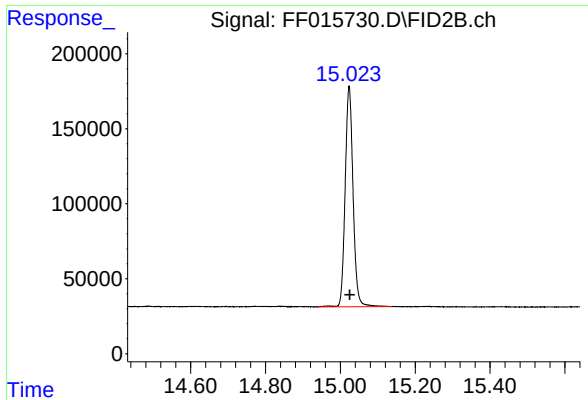

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.023 min
Delta R.T.: -0.002 min
Response: 2155881
Conc: 19.67 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

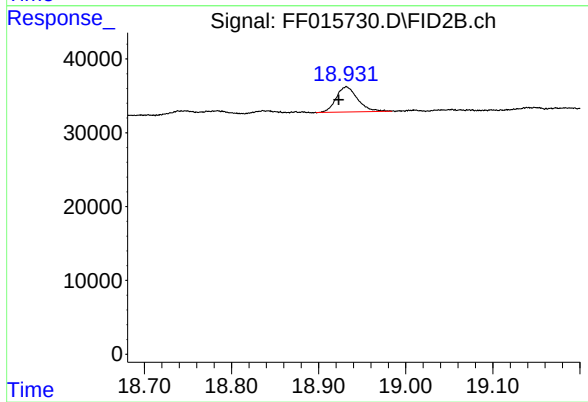

#14 N-DOTRIACONTANE

R.T.: 18.932 min
Delta R.T.: 0.009 min
Response: 57889
Conc: 0.49 ug/ml