

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032720\
 Data File : FF006701.D
 Signal(s) : FID2B.ch
 Acq On : 27 Mar 2020 17:47
 Operator : DD\AJ
 Sample : L2053-07
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 28 00:45:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.582	1913902	14.871 ug/ml
Target Compounds			
4) N-TETRADECANE	8.217f	718819	5.026 ug/ml
11) N-HEXACOSANE	15.802	182871	1.262 ug/ml
12) N-OCTACOSANE	16.746	314120	2.193 ug/ml
13) N-TRIACONTANE	17.629	347168	2.453 ug/ml
14) N-DOTRIACONTANE	18.456	237968	1.765 ug/ml
16) N-HEXATRIACONTANE	19.976	128382	1.398 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032720\
Data File : FF006701.D
Signal(s) : FID2B.ch
Acq On : 27 Mar 2020 17:47
Operator : DD\AJ
Sample : L2053-07
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 28 00:45:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

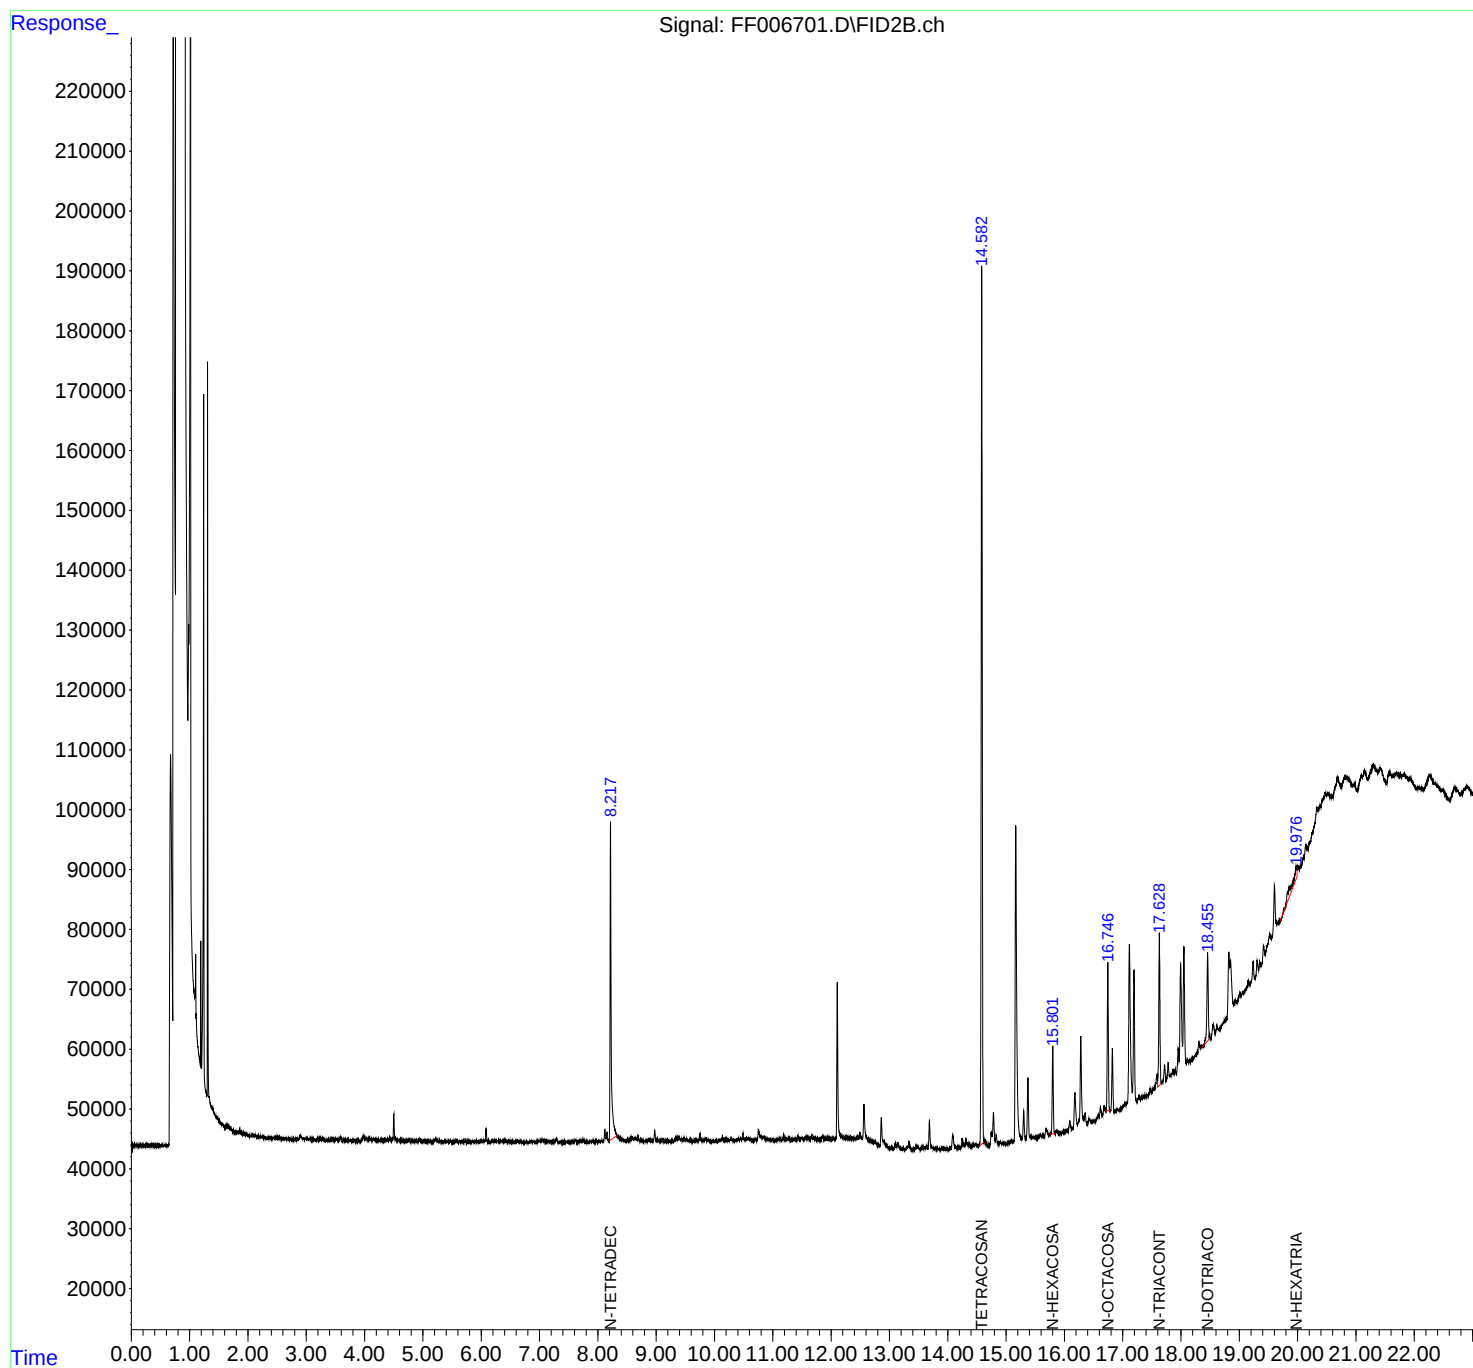


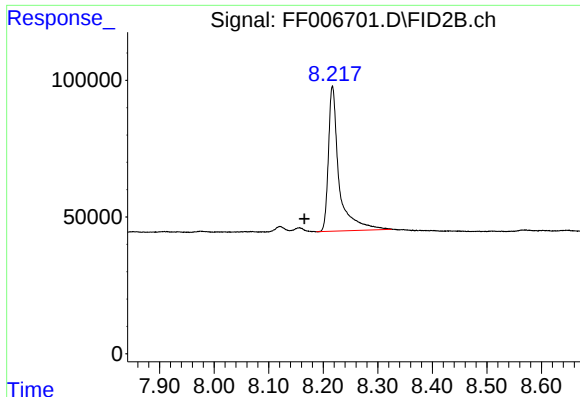

#4 N-TETRADECANE


R.T.: 8.217 min
Delta R.T.: 0.051 min
Response: 718819
Conc: 5.03 ug/ml

Instrument :
FID_F
ClientSampleId :

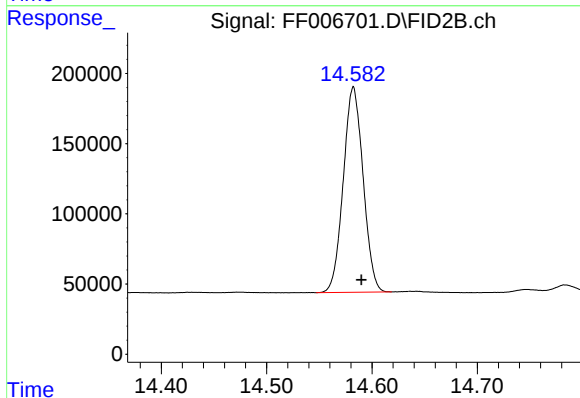


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.582 min
Delta R.T.: -0.007 min
Response: 1913902
Conc: 14.87 ug/ml

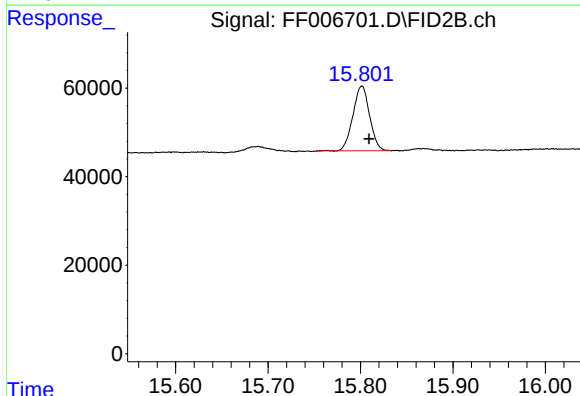


#11 N-HEXACOSANE

R.T.: 15.802 min
Delta R.T.: -0.008 min
Response: 182871
Conc: 1.26 ug/ml

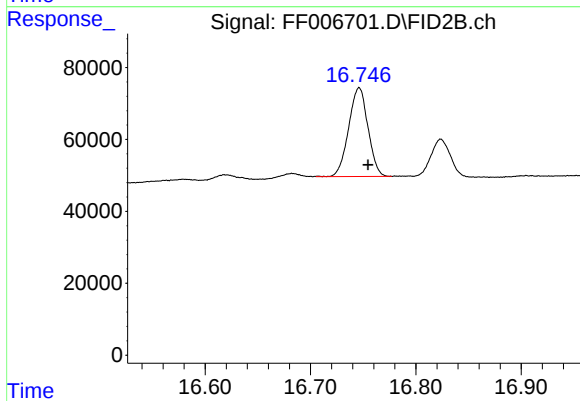

#12 N-OCTACOSANE


R.T.: 16.746 min
Delta R.T.: -0.008 min
Response: 314120
Conc: 2.19 ug/ml

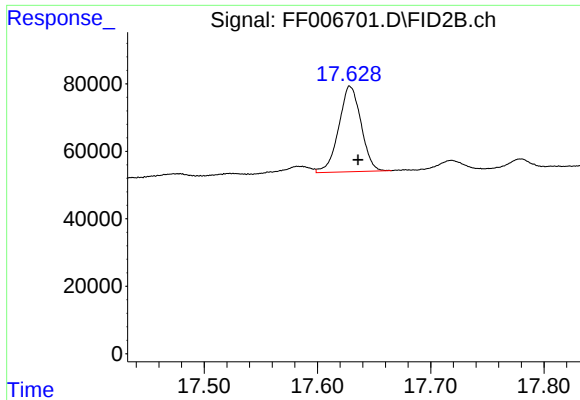

#13 N-TRIACONTANE


R.T.: 17.629 min
Delta R.T.: -0.007 min
Response: 347168
Conc: 2.45 ug/ml

Instrument :
FID_F
ClientSampleId :

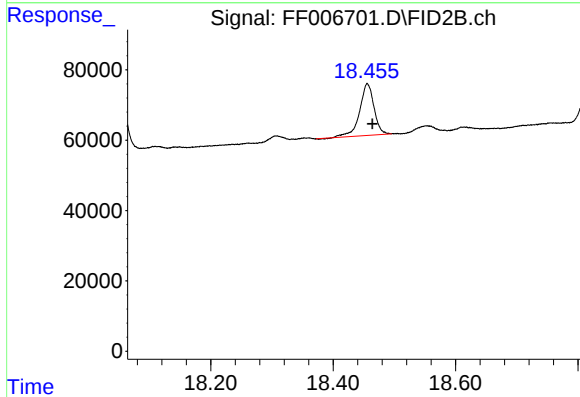

#14 N-DOTRIACONTANE

R.T.: 18.456 min
Delta R.T.: -0.008 min
Response: 237968
Conc: 1.77 ug/ml

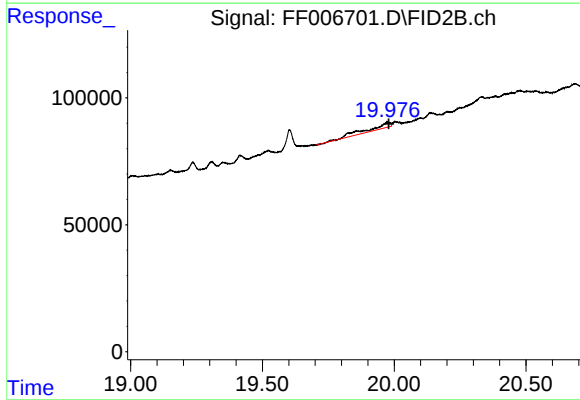

#16 N-HEXATRIACONTANE

R.T.: 19.976 min
Delta R.T.: -0.002 min
Response: 128382
Conc: 1.40 ug/ml