

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032720\
 Data File : FF006702.D
 Signal(s) : FID2B.ch
 Acq On : 27 Mar 2020 18:17
 Operator : DD\AJ
 Sample : L2053-06
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 28 00:45:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.583	2141714	16.641 ug/ml
Target Compounds			
4) N-TETRADECANE	8.217f	823666	5.759 ug/ml
7) N-EICOSANE	12.560f	420858	2.832 ug/ml
10) N-TETRACOSANE	14.778	224482	1.519 ug/ml
11) N-HEXACOSANE	15.801	108157	0.746 ug/ml
12) N-OCTACOSANE	16.748	369455	2.580 ug/ml
13) N-TRIACONTANE	17.630	381334	2.694 ug/ml
14) N-DOTRIACONTANE	18.455	371110	2.753 ug/ml
15) N-TETRATRIACONTANE	19.237	104787	0.928 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032720\
Data File : FF006702.D
Signal(s) : FID2B.ch
Acq On : 27 Mar 2020 18:17
Operator : DD\AJ
Sample : L2053-06
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 28 00:45:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

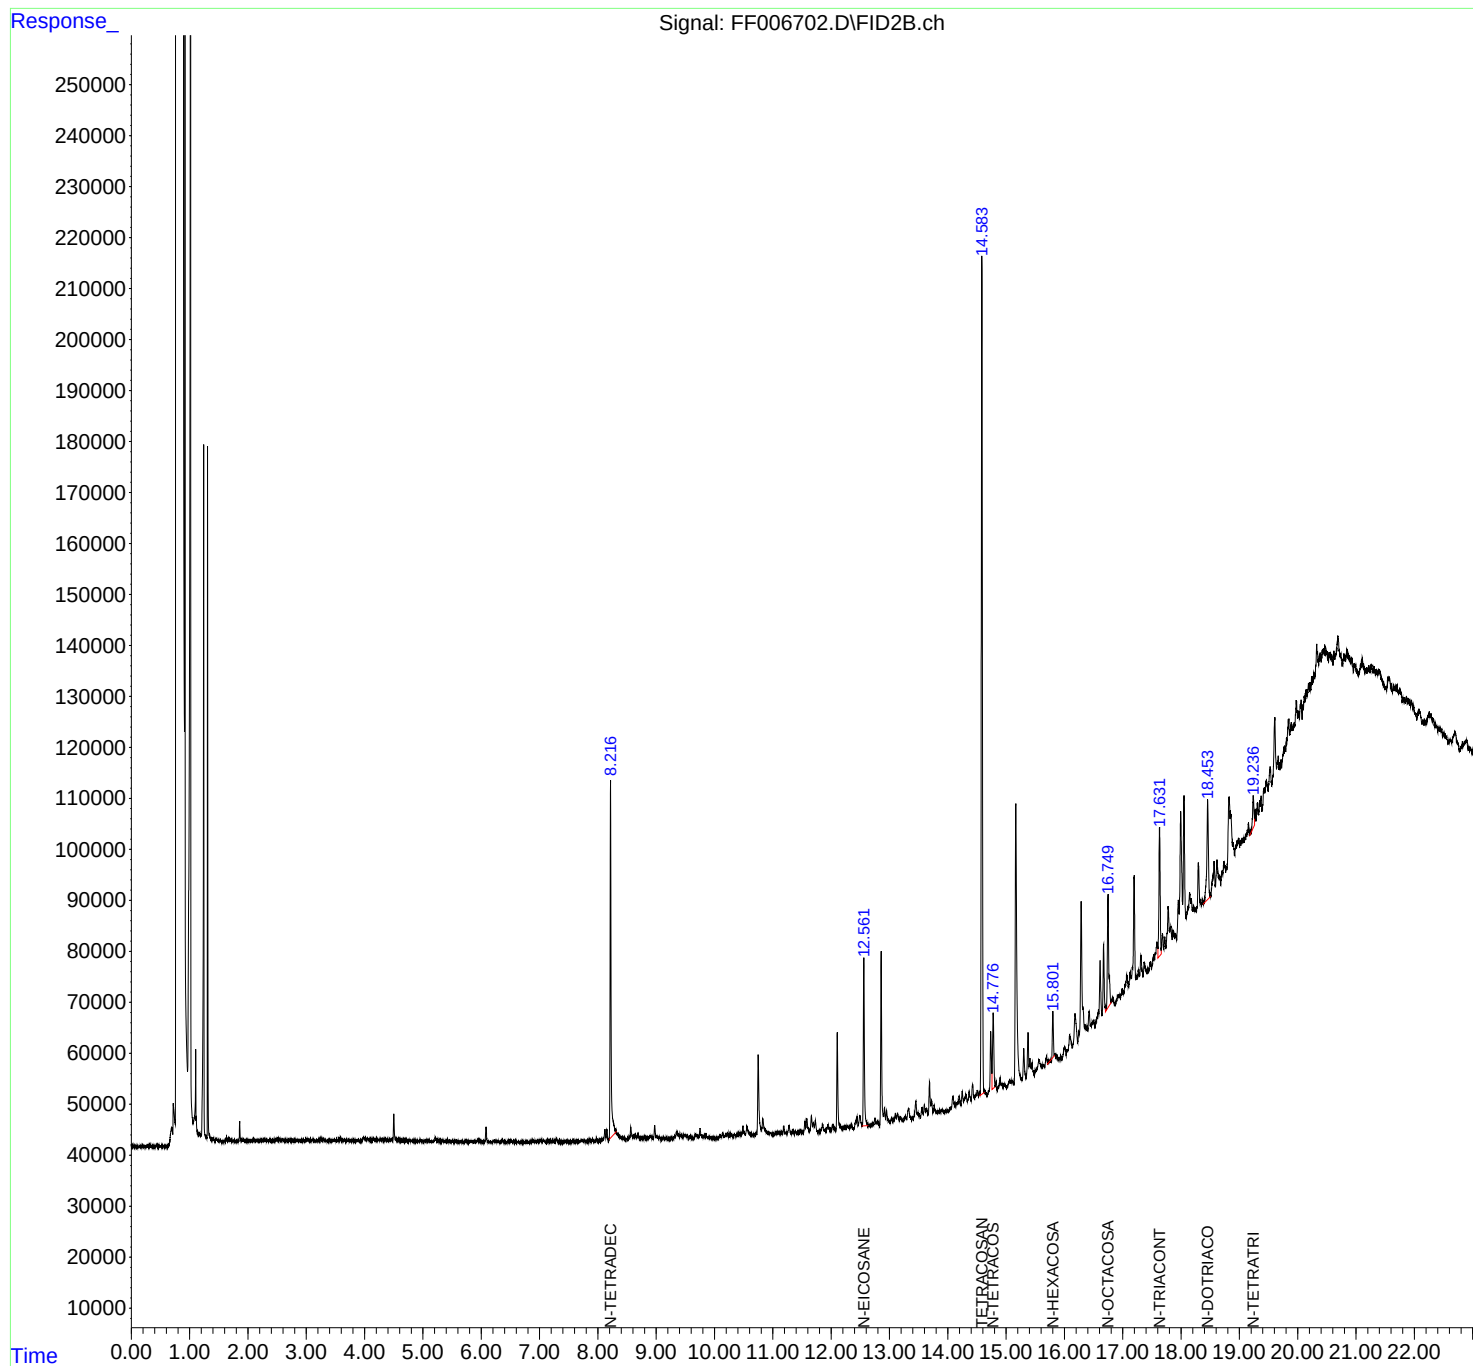


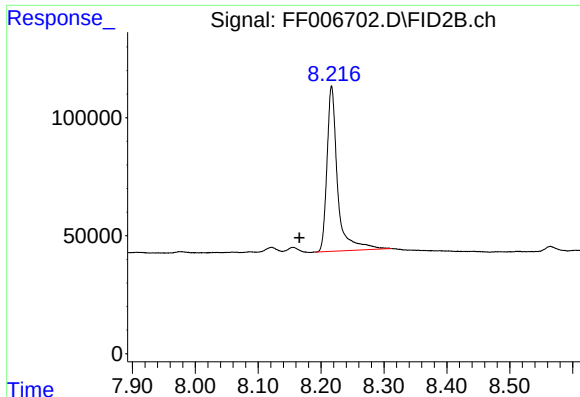

#4 N-TETRADECANE


R.T.: 8.217 min
Delta R.T.: 0.051 min
Response: 823666
Conc: 5.76 ug/ml

Instrument :
FID_F
ClientSampleId :

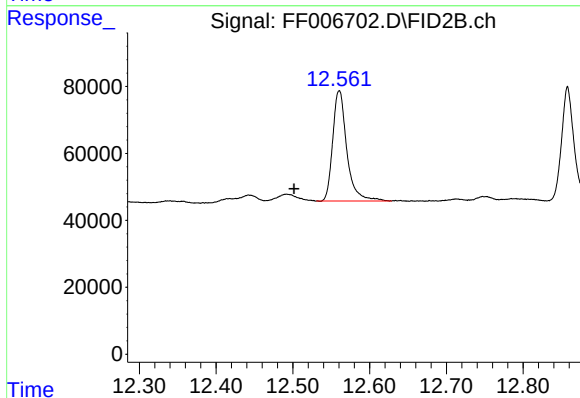


#7 N-EICOSANE

R.T.: 12.560 min
Delta R.T.: 0.059 min
Response: 420858
Conc: 2.83 ug/ml

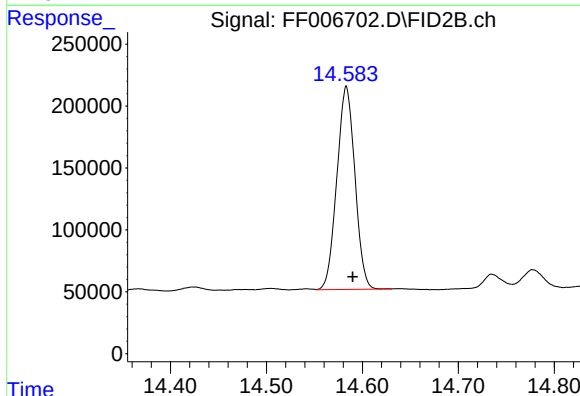


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.583 min
Delta R.T.: -0.007 min
Response: 2141714
Conc: 16.64 ug/ml

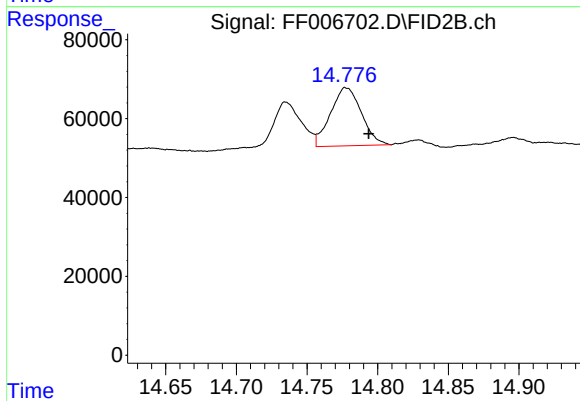

#10 N-TETRACOSANE


R.T.: 14.778 min
Delta R.T.: -0.016 min
Response: 224482
Conc: 1.52 ug/ml

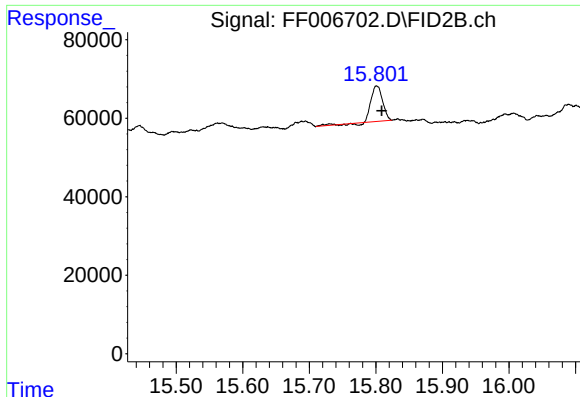

#11 N-HEXACOSANE


R.T.: 15.801 min
Delta R.T.: -0.008 min
Response: 108157
Conc: 0.75 ug/ml

Instrument :
FID_F
ClientSampleId :

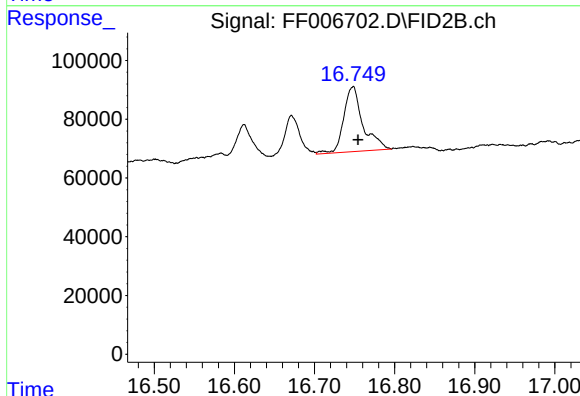


#12 N-OCTACOSANE

R.T.: 16.748 min
Delta R.T.: -0.006 min
Response: 369455
Conc: 2.58 ug/ml

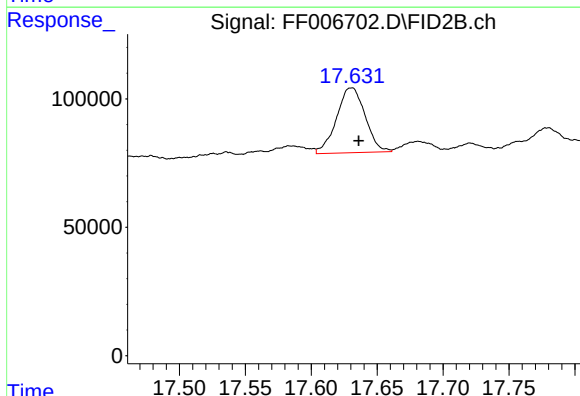


#13 N-TRIACONTANE

R.T.: 17.630 min
Delta R.T.: -0.006 min
Response: 381334
Conc: 2.69 ug/ml

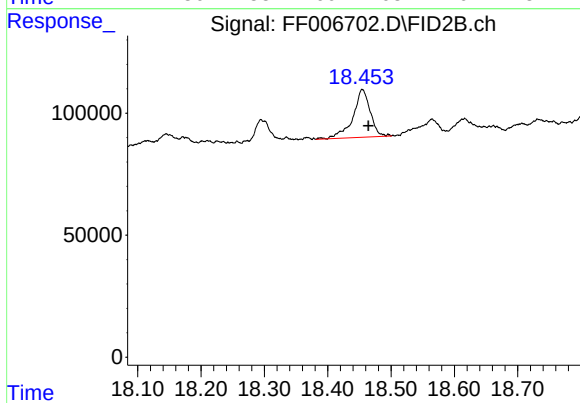

#14 N-DOTRIACONTANE

R.T.: 18.455 min
Delta R.T.: -0.009 min
Response: 371110
Conc: 2.75 ug/ml

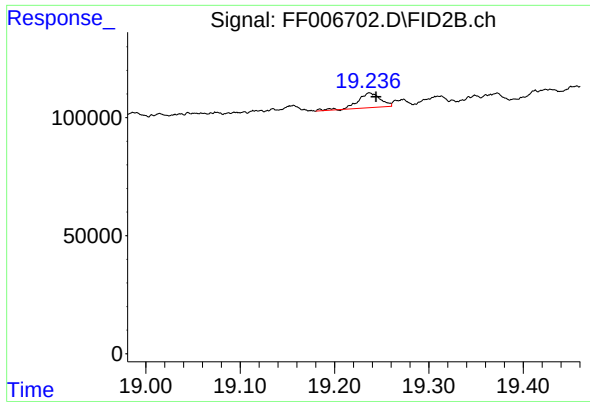

#15 N-TETRATRIACONTANE

R.T.: 19.237 min
Delta R.T.: -0.007 min
Response: 104787
Conc: 0.93 ug/ml

Instrument :
FID_F
ClientSampleId :