

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032720\
 Data File : FF006707.D
 Signal(s) : FID2B.ch
 Acq On : 27 Mar 2020 20:51
 Operator : DD\AJ
 Sample : L2055-05 2X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 28 00:46:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.583	707908	5.500 ug/ml
Target Compounds			
4) N-TETRADECANE	8.218f	284097	1.986 ug/ml
7) N-EICOSANE	12.563f	130056	0.875 ug/ml
10) N-TETRACOSANE	14.780	132210	0.895 ug/ml
11) N-HEXACOSANE	15.801	77662	0.536 ug/ml
12) N-OCTACOSANE	16.747	225525	1.575 ug/ml
13) N-TRIACONTANE	17.633	500805	3.538 ug/ml
14) N-DOTRIACONTANE	18.459	405375	3.007 ug/ml
15) N-TETRATRIACONTANE	19.243	88425	0.783 ug/ml
16) N-HEXATRIACONTANE	19.977	284040	3.093 ug/ml
17) N-OCTATRIACONTANE	20.676	94411	1.367 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032720\
Data File : FF006707.D
Signal(s) : FID2B.ch
Acq On : 27 Mar 2020 20:51
Operator : DD\AJ
Sample : L2055-05 2X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 28 00:46:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

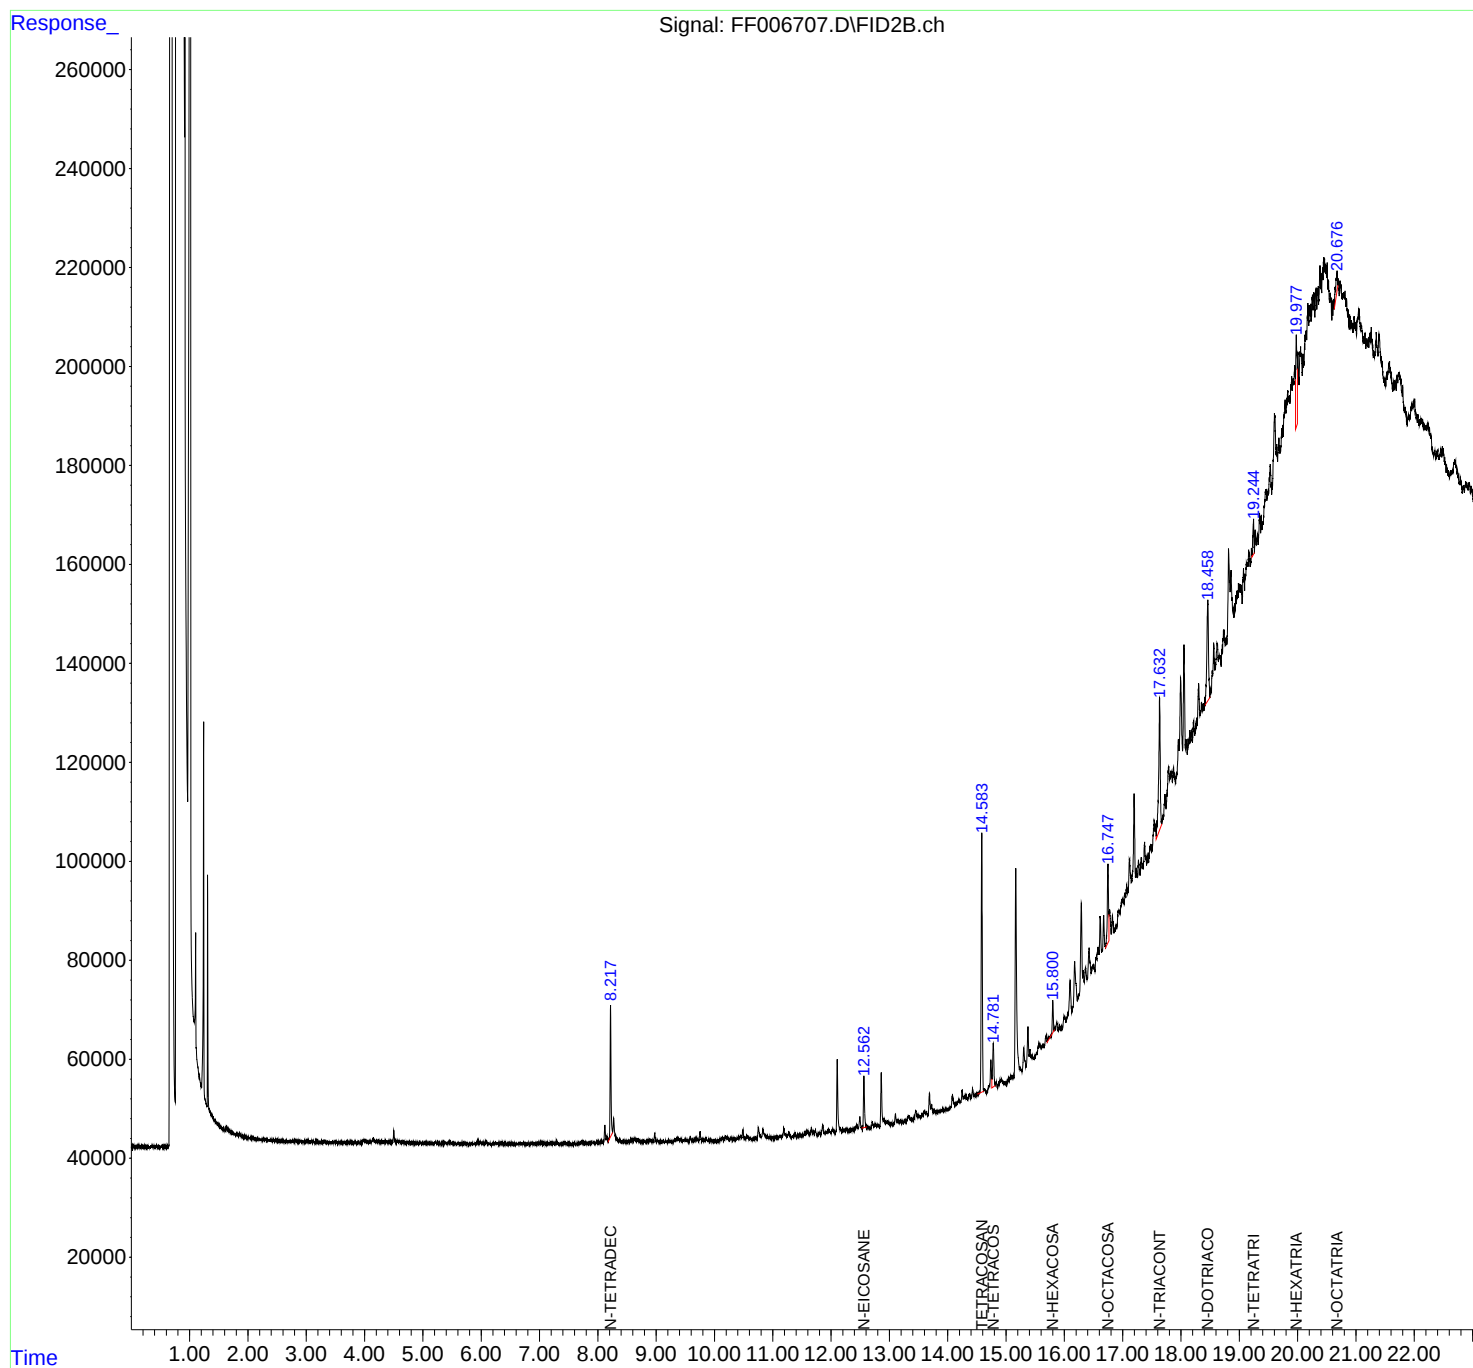


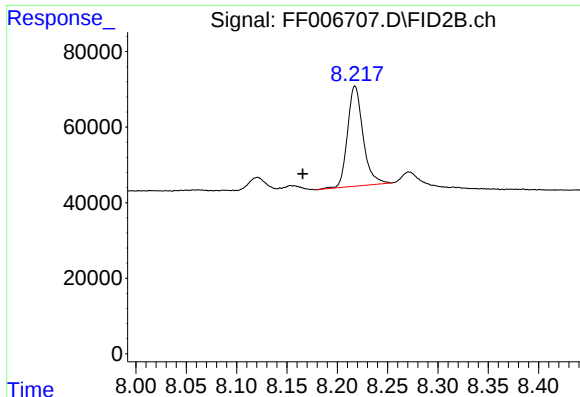

#4 N-TETRADECANE


R.T.: 8.218 min
Delta R.T.: 0.052 min
Response: 284097
Conc: 1.99 ug/ml

Instrument :
FID_F
ClientSampleId :

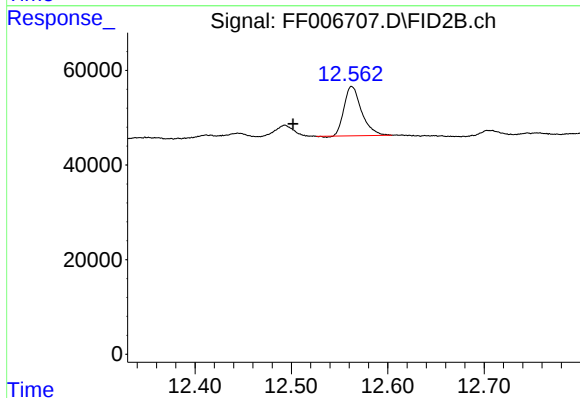


#7 N-EICOSANE

R.T.: 12.563 min
Delta R.T.: 0.061 min
Response: 130056
Conc: 0.88 ug/ml

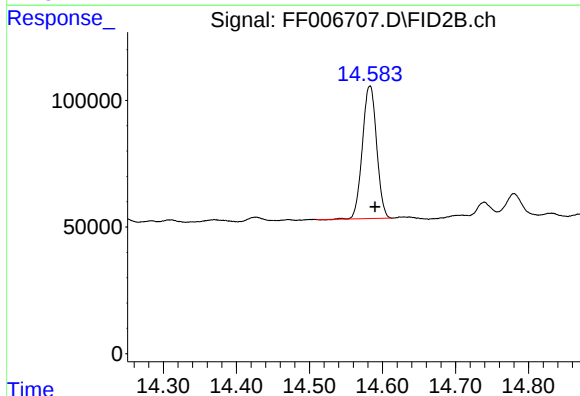


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.583 min
Delta R.T.: -0.007 min
Response: 707908
Conc: 5.50 ug/ml

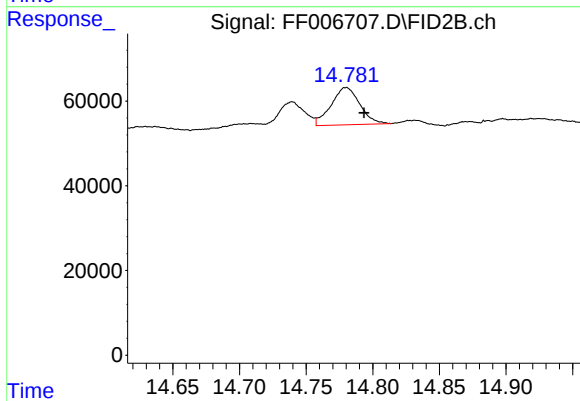

#10 N-TETRACOSANE


R.T.: 14.780 min
Delta R.T.: -0.014 min
Response: 132210
Conc: 0.89 ug/ml

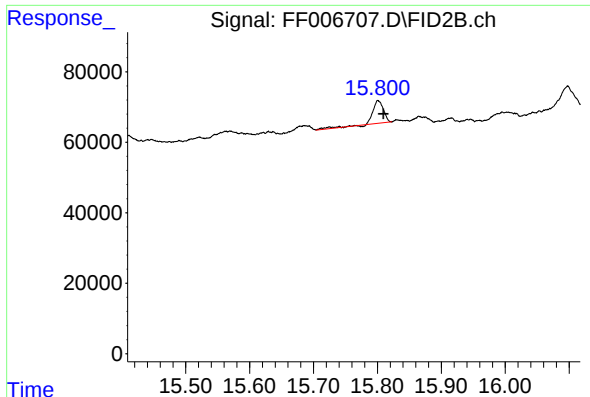

#11 N-HEXACOSANE


R.T.: 15.801 min
Delta R.T.: -0.008 min
Response: 77662
Conc: 0.54 ug/ml

Instrument :
FID_F
ClientSampleId :

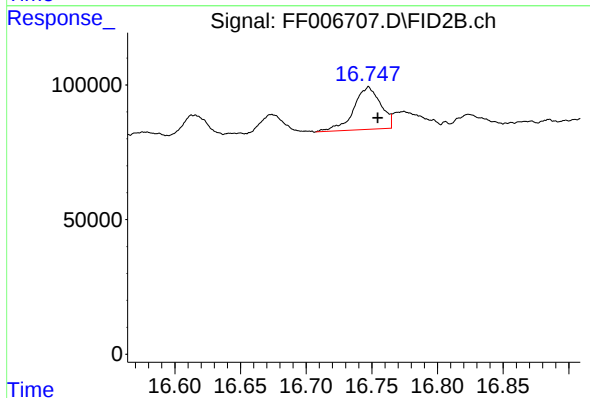


#12 N-OCTACOSANE

R.T.: 16.747 min
Delta R.T.: -0.007 min
Response: 225525
Conc: 1.57 ug/ml

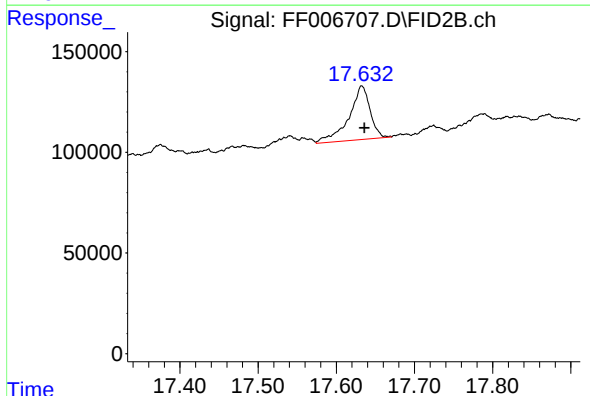


#13 N-TRIACONTANE

R.T.: 17.633 min
Delta R.T.: -0.003 min
Response: 500805
Conc: 3.54 ug/ml

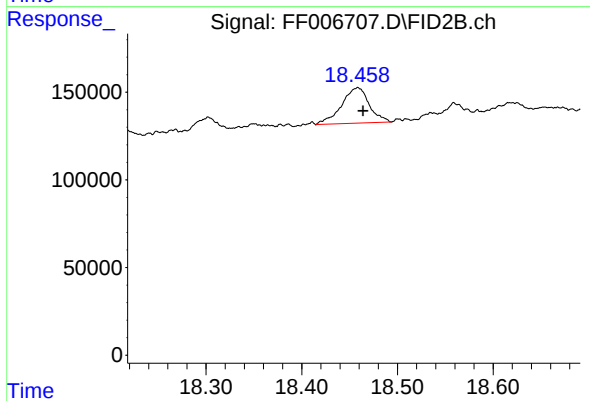

#14 N-DOTRIACONTANE


R.T.: 18.459 min
Delta R.T.: -0.005 min
Response: 405375
Conc: 3.01 ug/ml

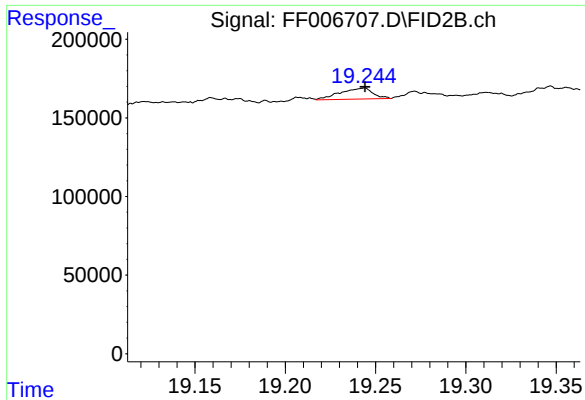

#15 N-TETRATRIACONTANE


R.T.: 19.243 min
Delta R.T.: 0.000 min
Response: 88425
Conc: 0.78 ug/ml

Instrument :
FID_F
ClientSampleId :

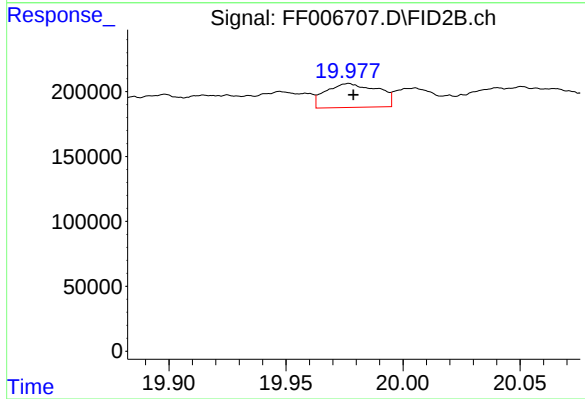

#16 N-HEXATRIACONTANE

R.T.: 19.977 min
Delta R.T.: -0.002 min
Response: 284040
Conc: 3.09 ug/ml

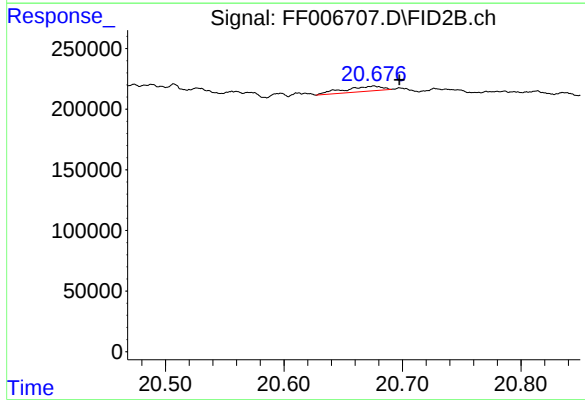

#17 N-OCTATRIACONTANE

R.T.: 20.676 min
Delta R.T.: -0.022 min
Response: 94411
Conc: 1.37 ug/ml