

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032723\
Data File : FF012356.D
Signal(s) : FID2B.ch
Acq On : 27 Mar 2023 09:04
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 28 02:27:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
15)	N-TETRATRIACONTANE	19.708	12891	0.136 ug/ml
16)	N-HEXATRIACONTANE	20.433	23389	0.267 ug/ml
18)	N-TETRACONTANE	22.134	45867	0.561 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032723\
Data File : FF012356.D
Signal(s) : FID2B.ch
Acq On : 27 Mar 2023 09:04
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 28 02:27:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

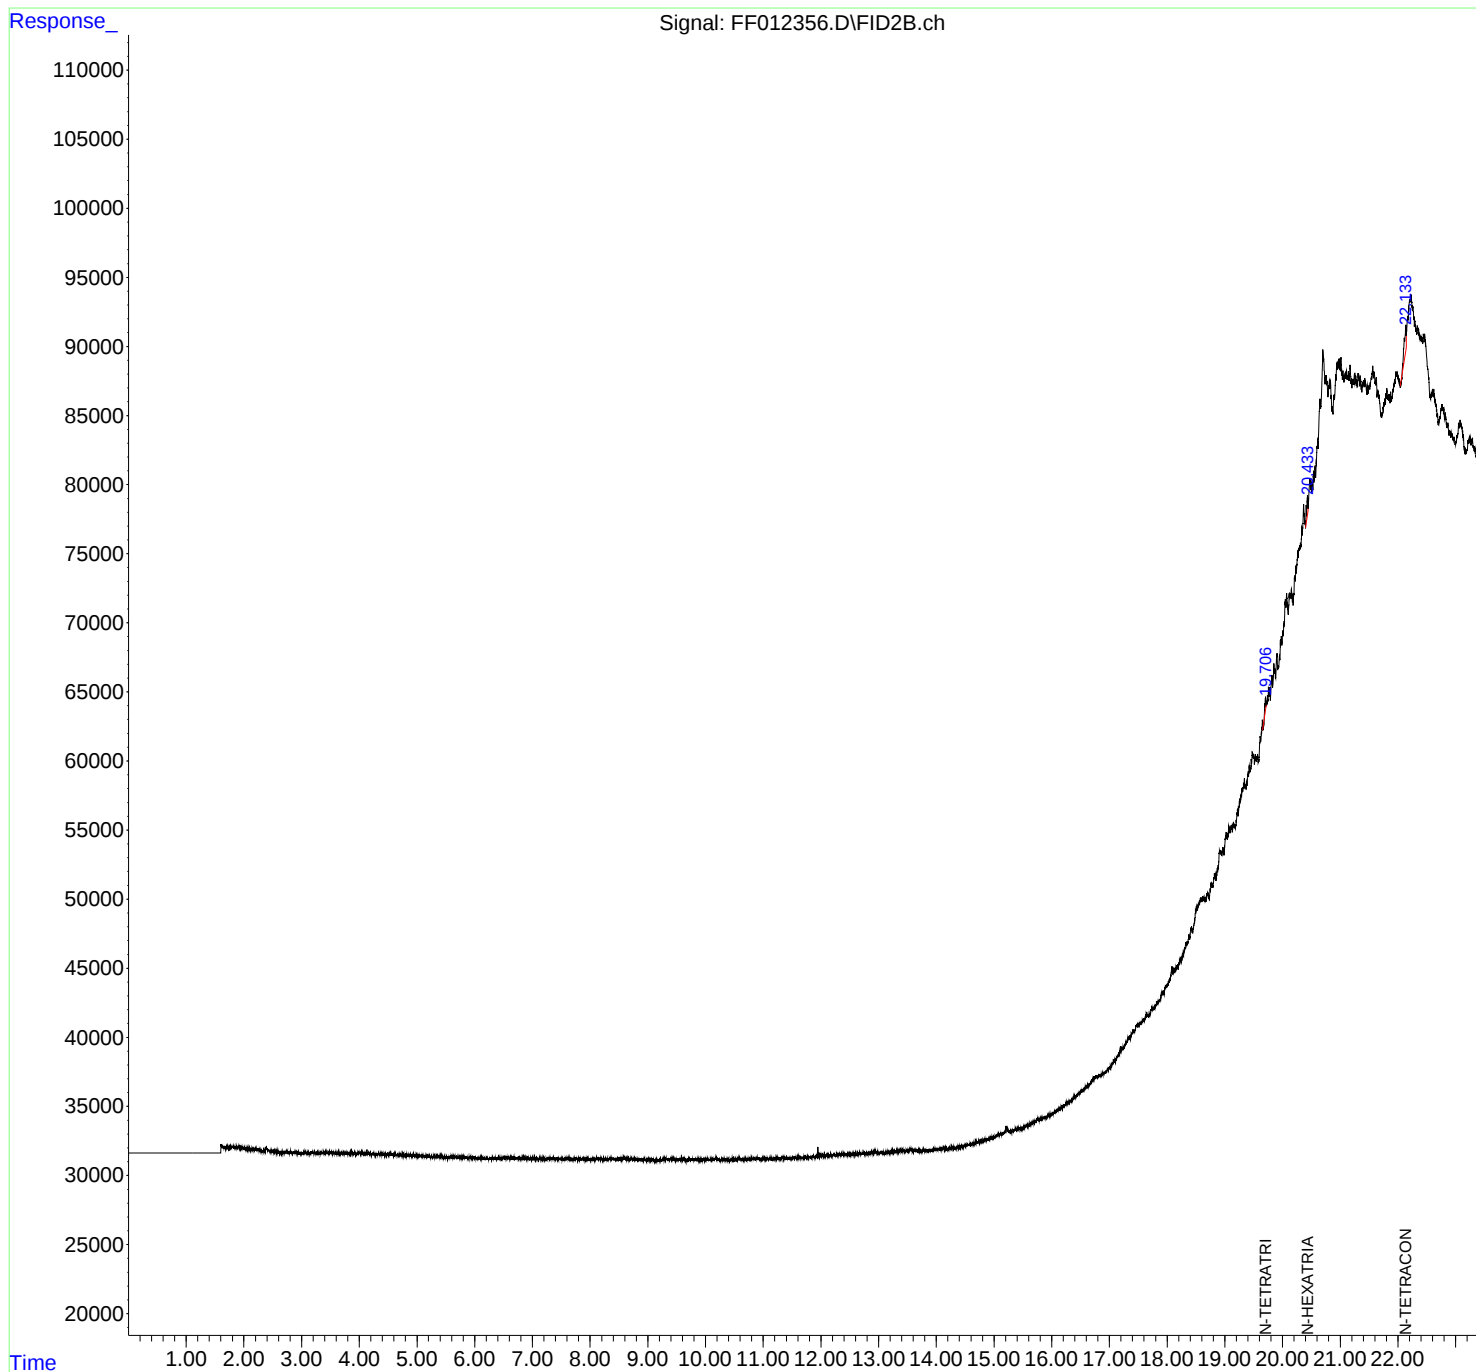


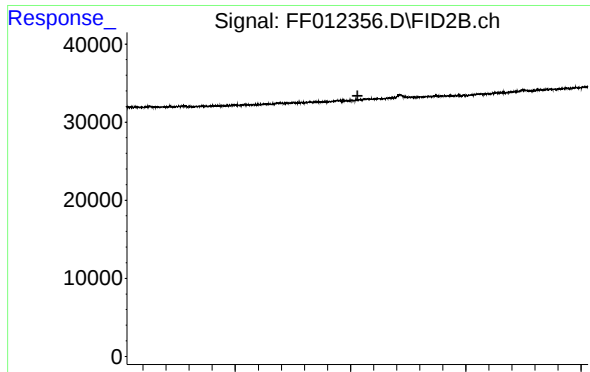

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.030 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

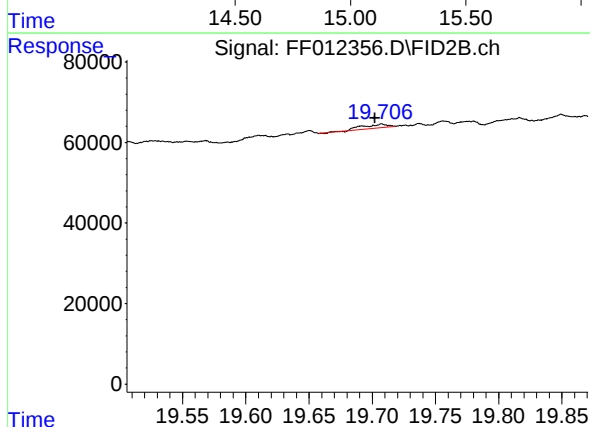


#15 N-TETRATRIACONTANE

R.T.: 19.708 min
Delta R.T.: 0.005 min
Response: 12891
Conc: 0.14 ug/ml

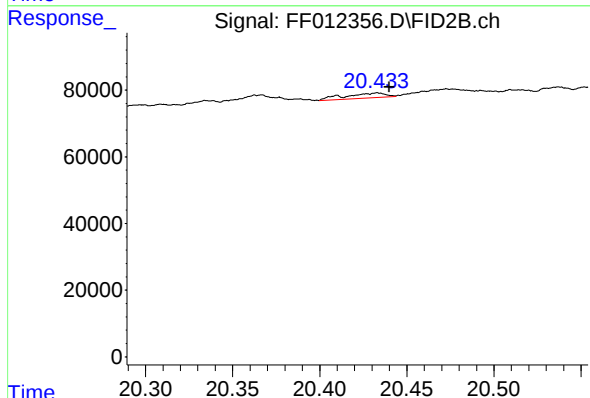

#16 N-HEXATRIACONTANE

R.T.: 20.433 min
Delta R.T.: -0.007 min
Response: 23389
Conc: 0.27 ug/ml

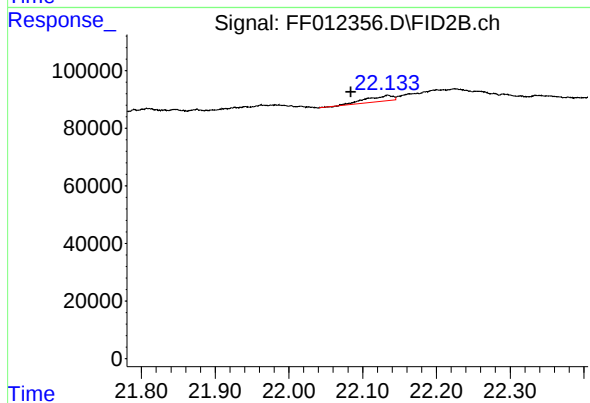

#18 N-TETRACONTANE

R.T.: 22.134 min
Delta R.T.: 0.050 min
Response: 45867
Conc: 0.56 ug/ml