

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
 Data File : FF004015.D
 Signal(s) : FID2B.ch
 Acq On : 28 Mar 2019 10:30
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 29 02:28:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.569	1967677	14.133 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.474	198950	1.399 ug/ml
16) N-HEXATRIACONTANE	20.035	443445	3.399 ug/ml
18) N-TETRACONTANE	21.623	837072	6.728 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
Data File : FF004015.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2019 10:30
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 29 02:28:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

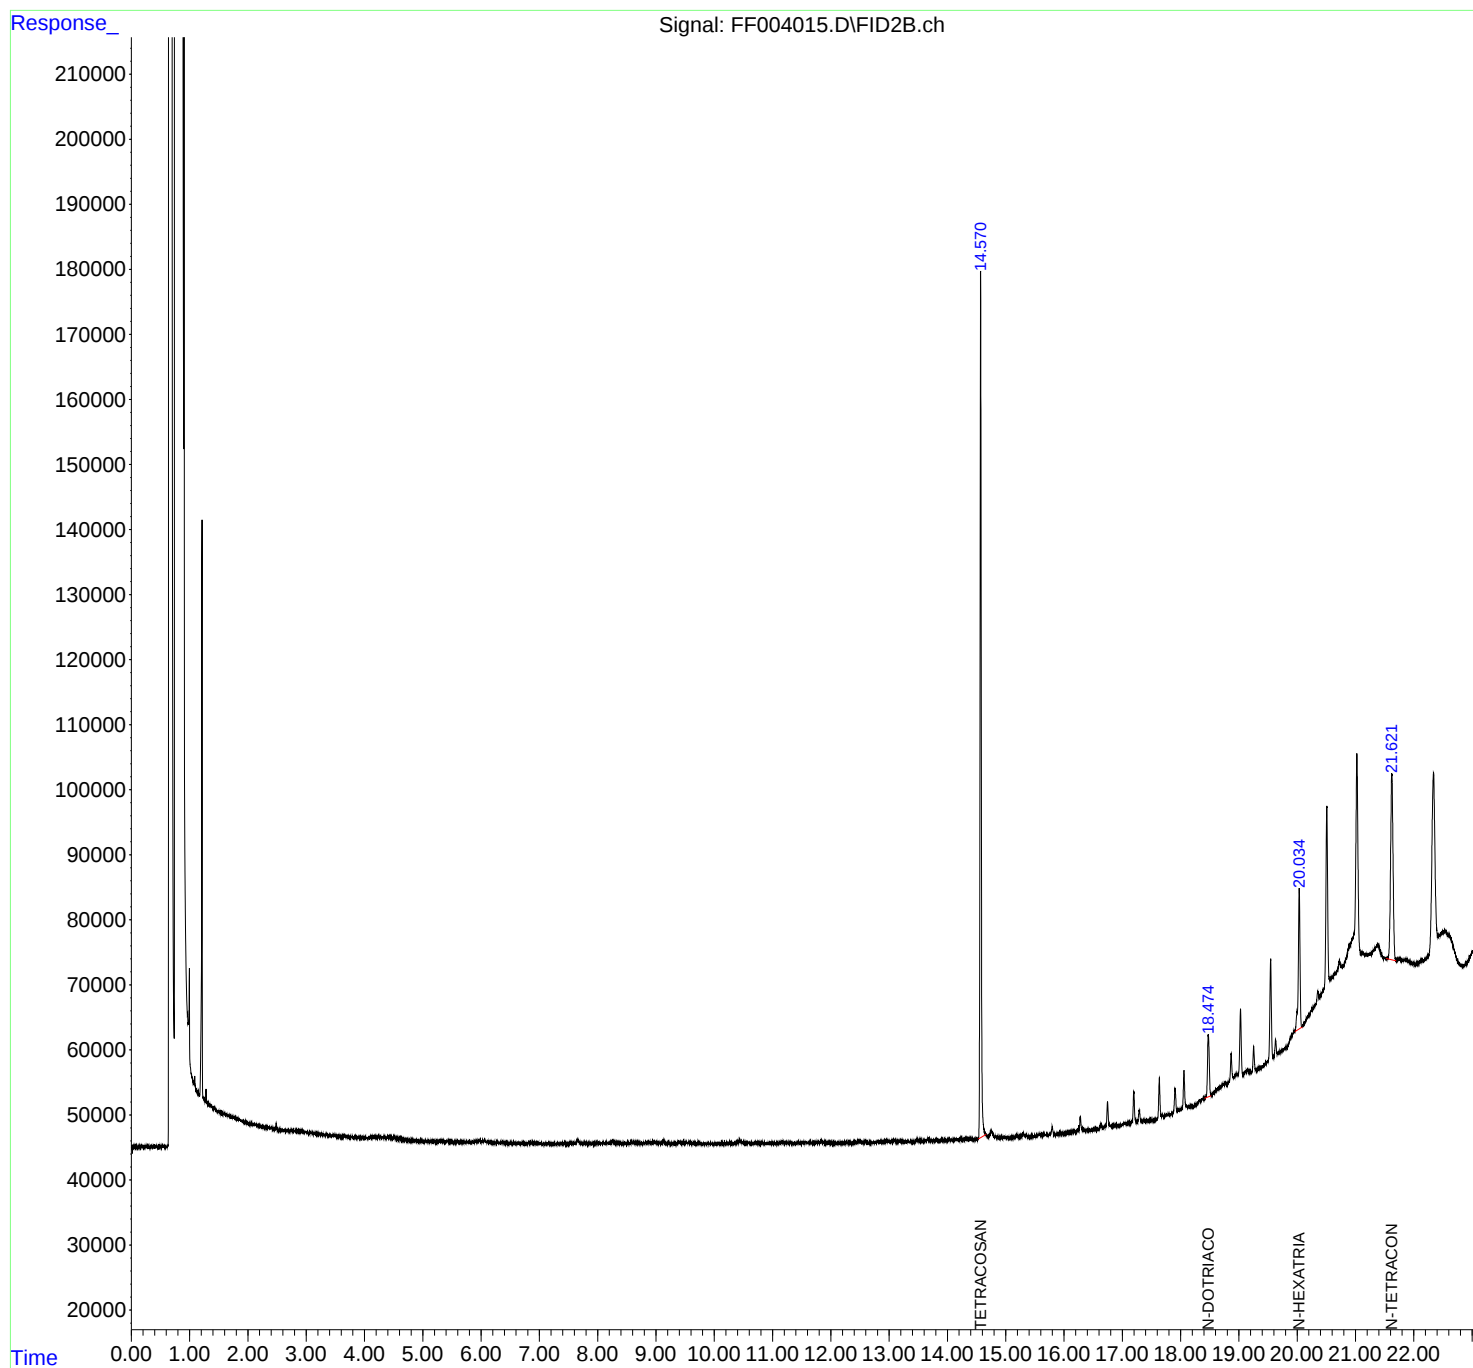


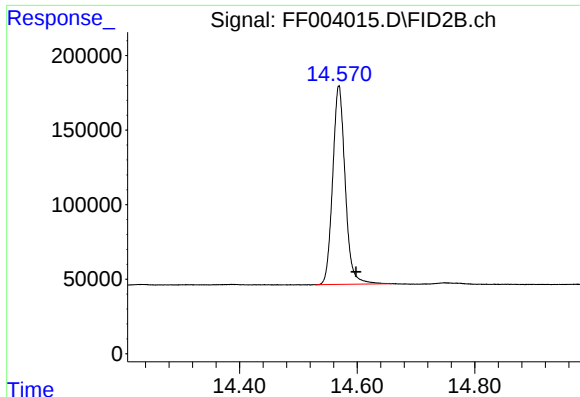

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.569 min
Delta R.T.: -0.029 min
Response: 1967677
Conc: 14.13 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

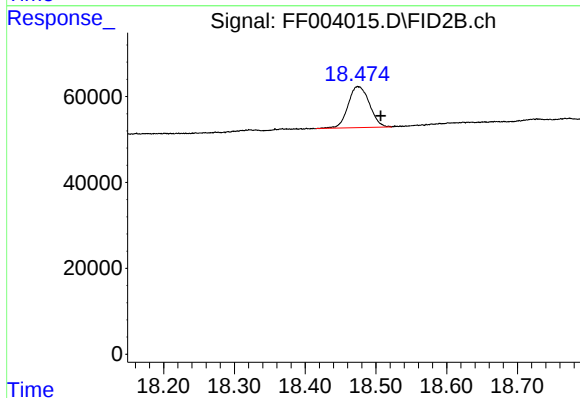


#14 N-DOTRIACONTANE

R.T.: 18.474 min
Delta R.T.: -0.032 min
Response: 198950
Conc: 1.40 ug/ml

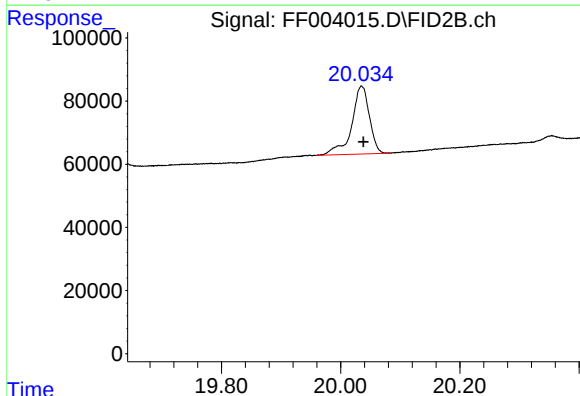

#16 N-HEXATRIACONTANE

R.T.: 20.035 min
Delta R.T.: -0.003 min
Response: 443445
Conc: 3.40 ug/ml

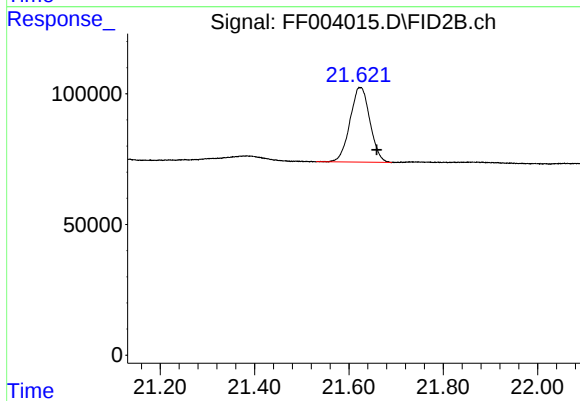

#18 N-TETRACONTANE

R.T.: 21.623 min
Delta R.T.: -0.036 min
Response: 837072
Conc: 6.73 ug/ml