

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
Data File : FF004017.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2019 11:40
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 29 02:28:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.318	3021017	19.358 ug/ml
12)	N-OCTACOSANE	16.744	2866976	18.972 ug/ml
13)	N-TRIACONTANE	17.631	129565	0.881 ug/ml
14)	N-DOTRIACONTANE	18.466	170300	1.198 ug/ml
15)	N-TETRATRIACONTANE	19.250	105744	0.790 ug/ml
16)	N-HEXATRIACONTANE	20.035	187233	1.435 ug/ml
18)	N-TETRACONTANE	21.623	297050	2.388 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
Data File : FF004017.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2019 11:40
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 29 02:28:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

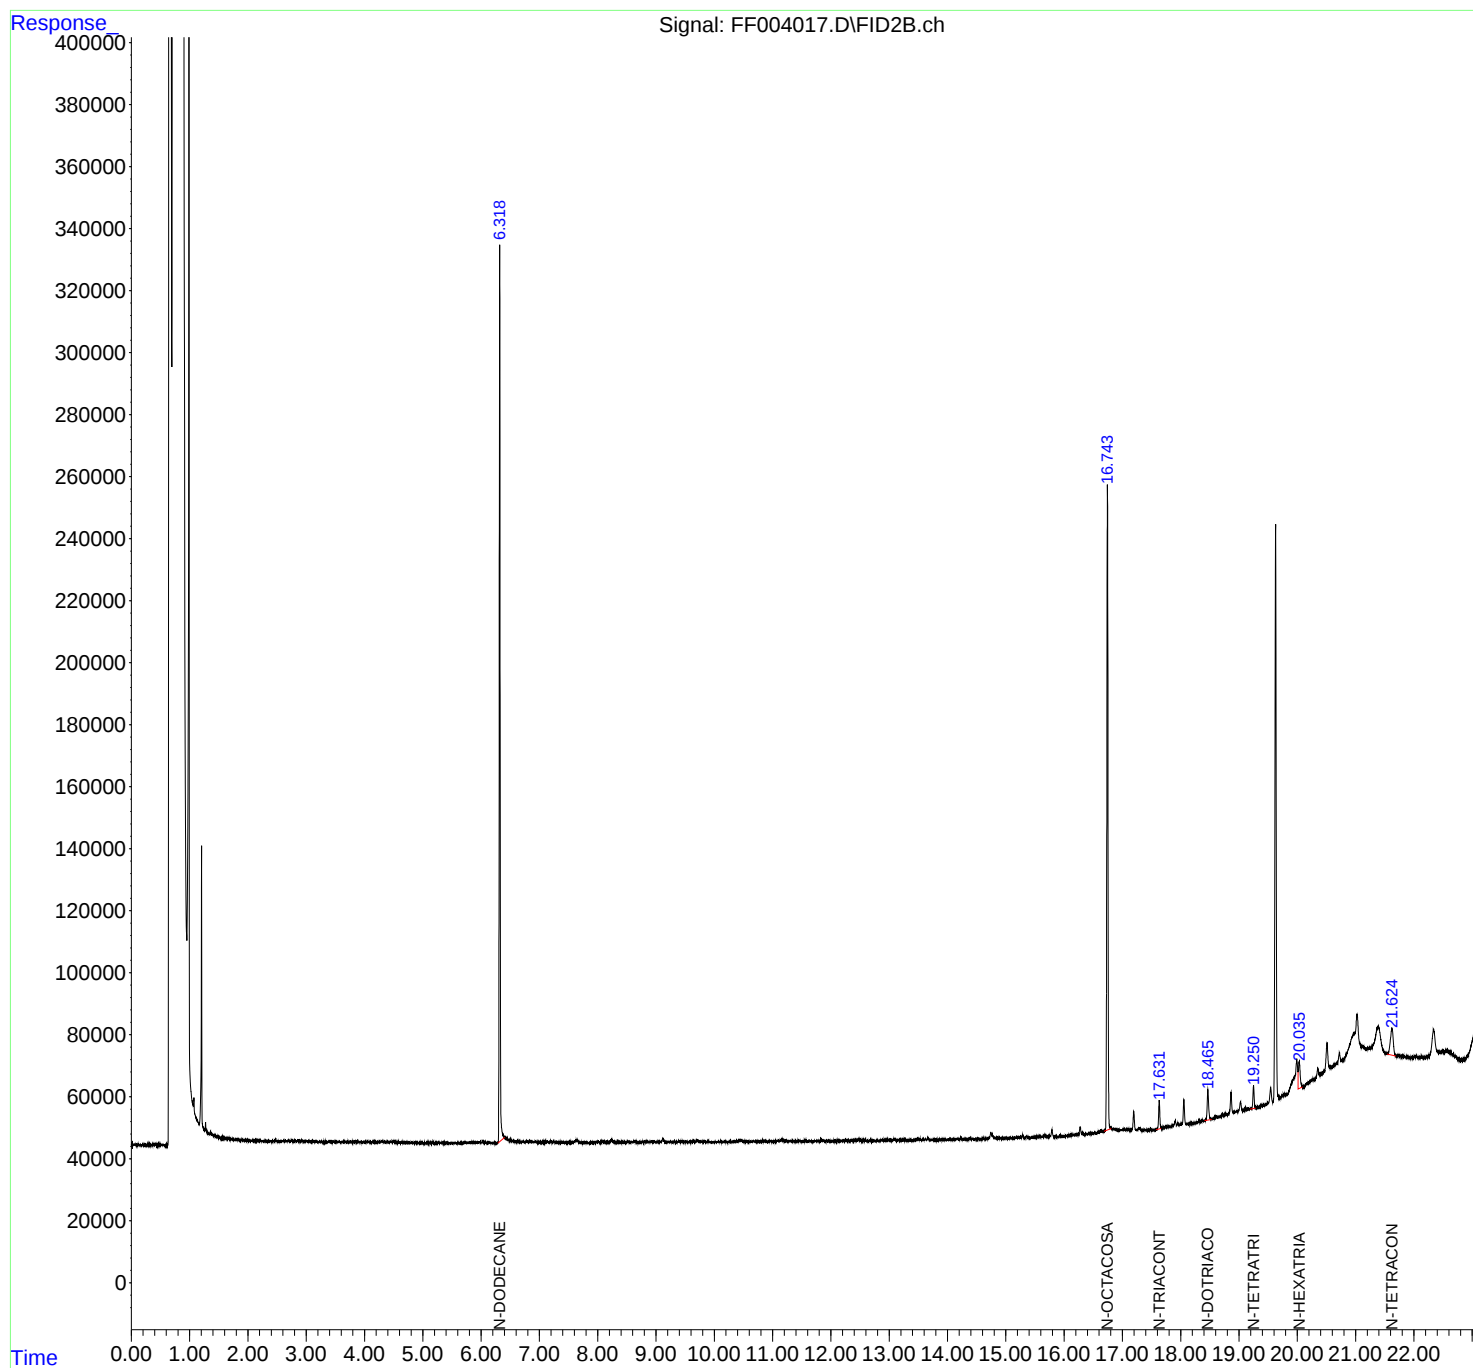


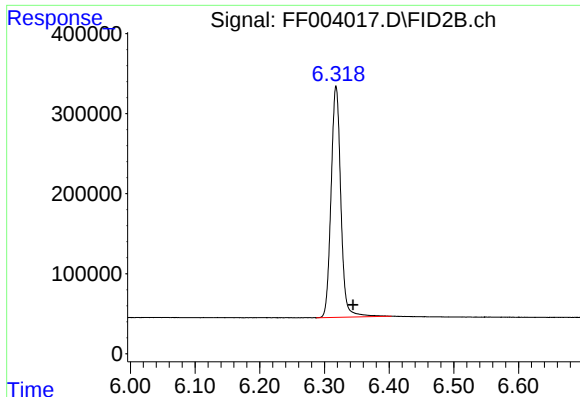

#3 N-DODECANE


R.T.: 6.318 min
Delta R.T.: -0.026 min
Response: 3021017
Conc: 19.36 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

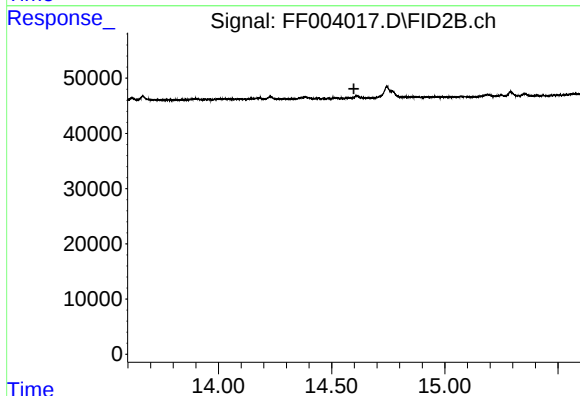


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

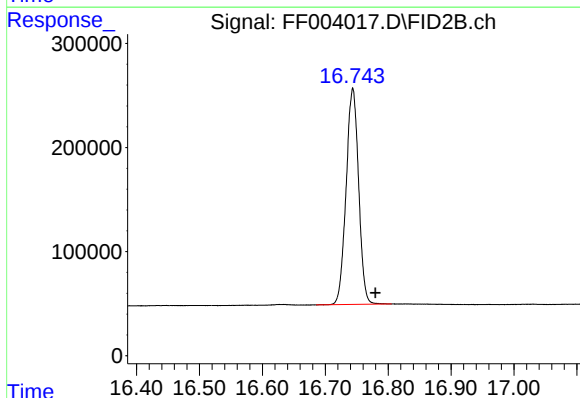


#12 N-OCTACOSANE

R.T.: 16.744 min
Delta R.T.: -0.036 min
Response: 2866976
Conc: 18.97 ug/ml

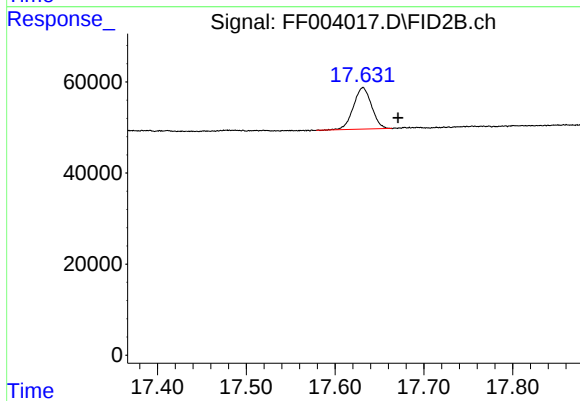

#13 N-TRIACONTANE


R.T.: 17.631 min
Delta R.T.: -0.039 min
Response: 129565
Conc: 0.88 ug/ml

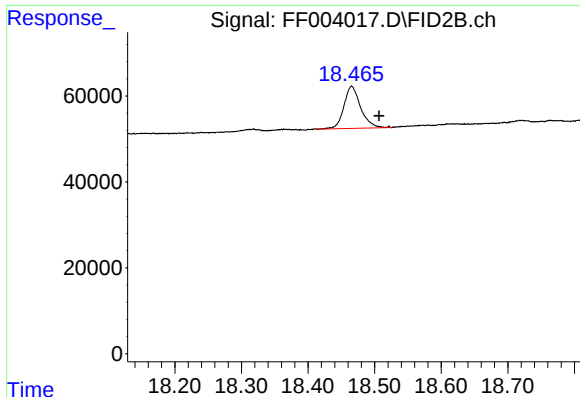

#14 N-DOTRIACONTANE


R.T.: 18.466 min
Delta R.T.: -0.041 min
Response: 170300
Conc: 1.20 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

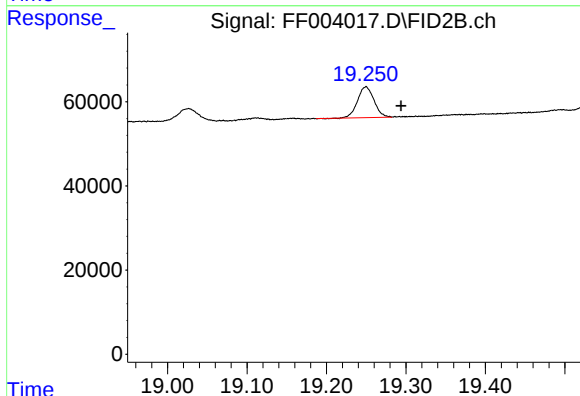


#15 N-TETRATRIACONTANE

R.T.: 19.250 min
Delta R.T.: -0.044 min
Response: 105744
Conc: 0.79 ug/ml

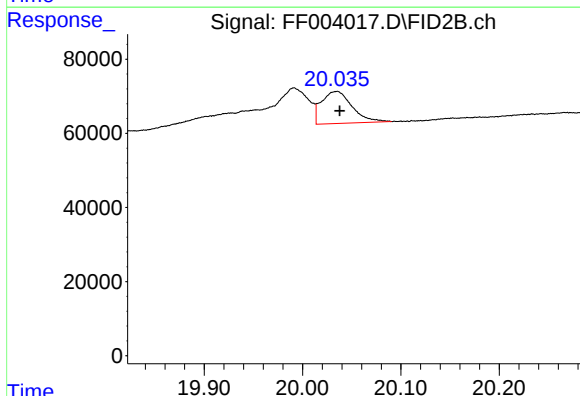

#16 N-HEXATRIACONTANE

R.T.: 20.035 min
Delta R.T.: -0.003 min
Response: 187233
Conc: 1.43 ug/ml

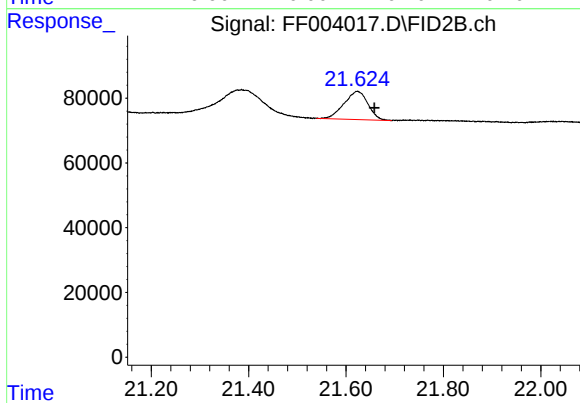

#18 N-TETRACONTANE

R.T.: 21.623 min
Delta R.T.: -0.036 min
Response: 297050
Conc: 2.39 ug/ml