

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
 Data File : FF004018.D
 Signal(s) : FID2B.ch
 Acq On : 28 Mar 2019 12:13
 Operator : AJ\SJ
 Sample : K2086-01 2X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CS-11

Integration File: autoint1.e
 Quant Time: Mar 29 02:28:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.565	1313352	9.433 ug/ml
Target Compounds			
7) N-EICOSANE	12.521	3342219	20.430 ug/ml
8) N-DOCOSANE	13.690	183342	1.136 ug/ml
10) N-TETRACOSANE	14.746f	2871111	18.146 ug/ml
11) N-HEXACOSANE	15.786	366763	2.376 ug/ml
12) N-OCTACOSANE	16.755	1099062	7.273 ug/ml
13) N-TRIACONTANE	17.631	419914	2.855 ug/ml
14) N-DOTRIACONTANE	18.464	293935	2.067 ug/ml
16) N-HEXATRIACONTANE	19.989	90833	0.696 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
Data File : FF004018.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2019 12:13
Operator : AJ\SJ
Sample : K2086-01 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CS-11

Integration File: autoint1.e
Quant Time: Mar 29 02:28:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

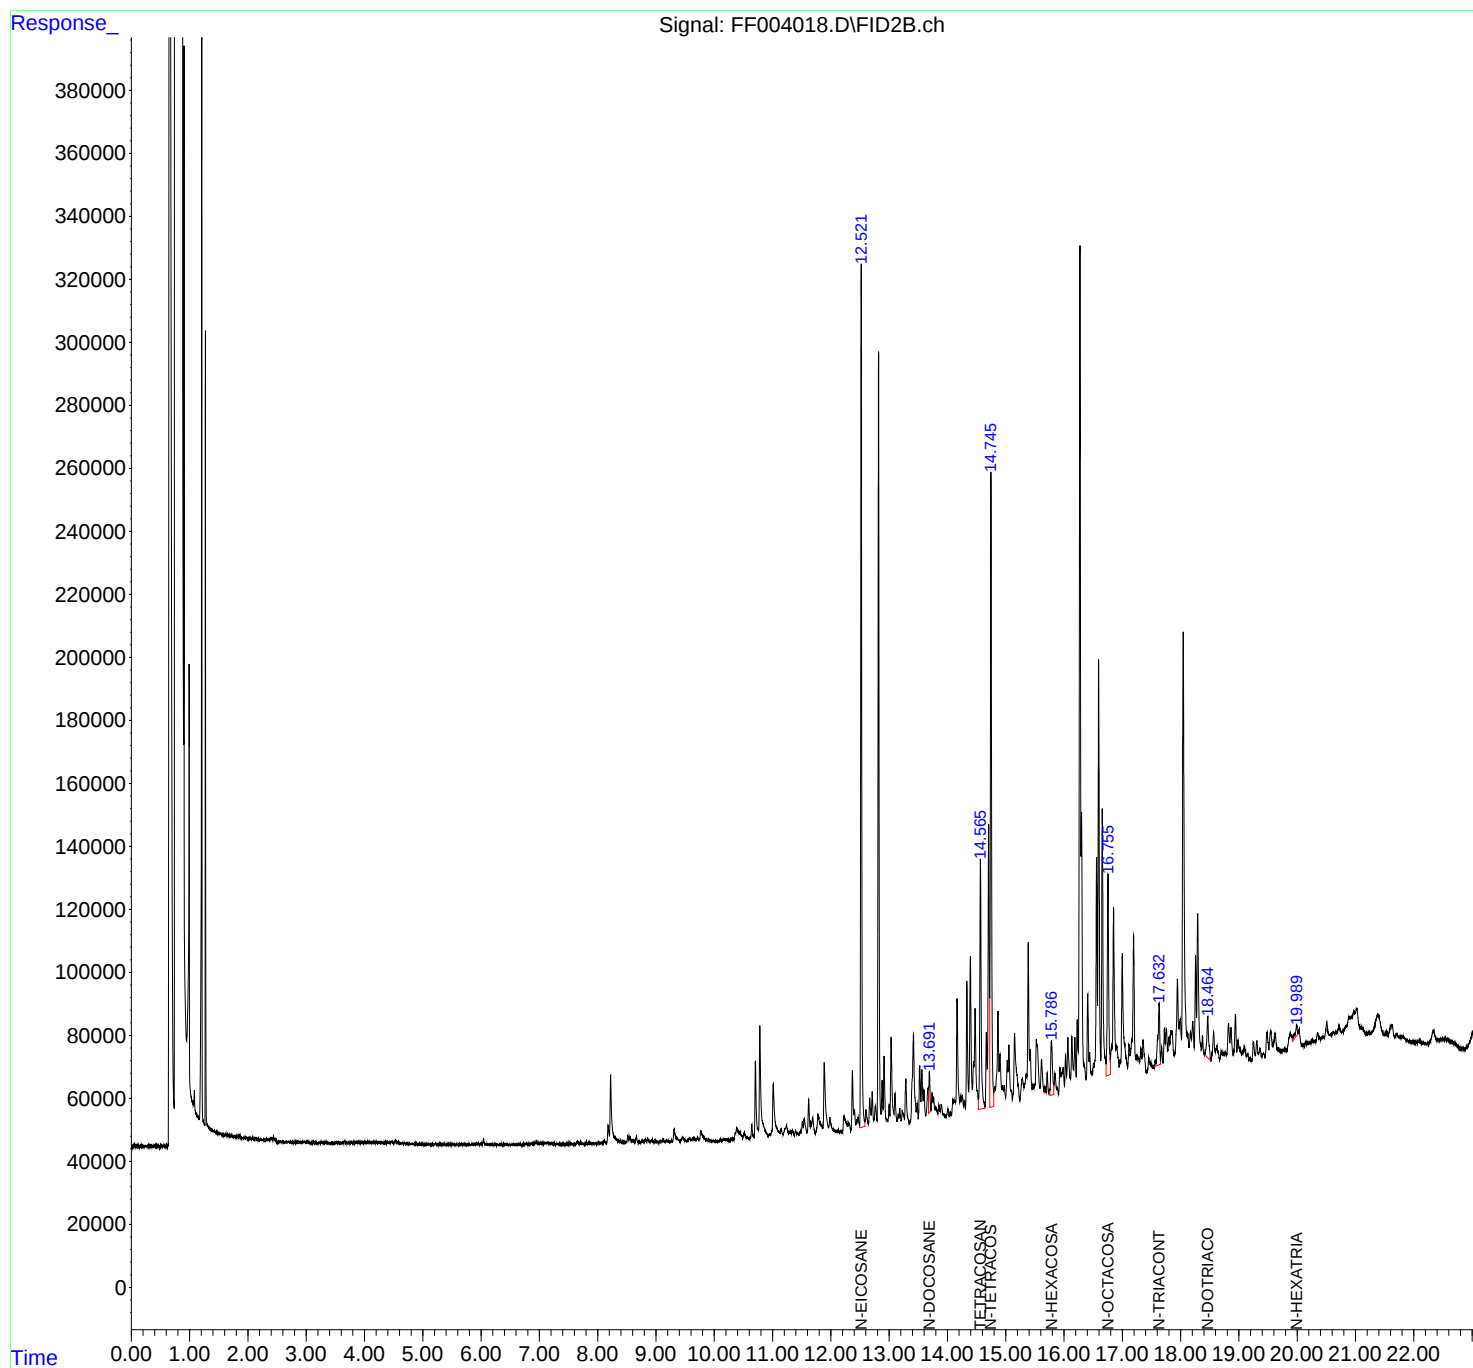


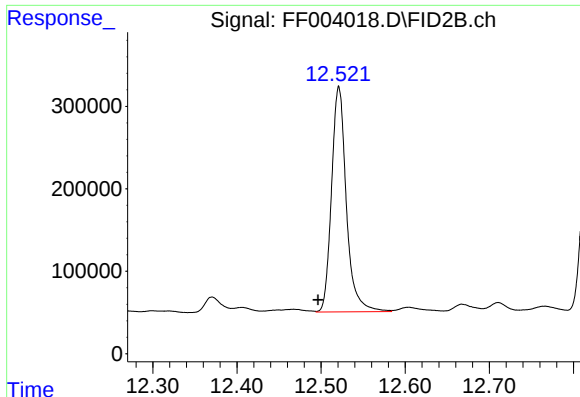

#7 N-EICOSANE


R.T.: 12.521 min
Delta R.T.: 0.025 min
Response: 3342219
Conc: 20.43 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-11

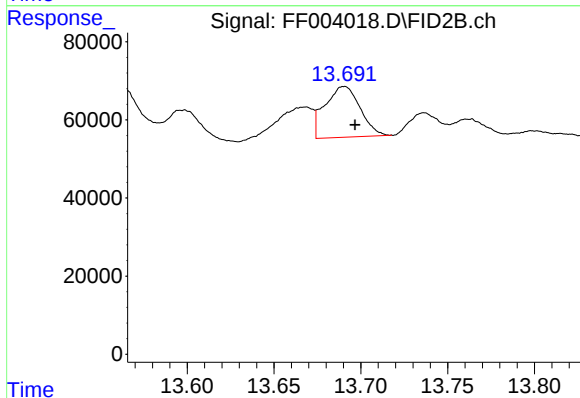


#8 N-DOCOSANE

R.T.: 13.690 min
Delta R.T.: -0.006 min
Response: 183342
Conc: 1.14 ug/ml

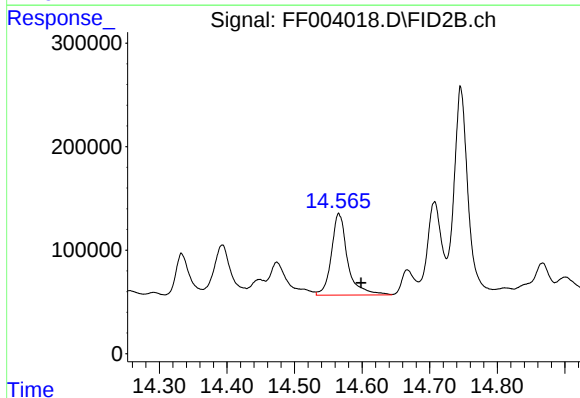


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.565 min
Delta R.T.: -0.033 min
Response: 1313352
Conc: 9.43 ug/ml

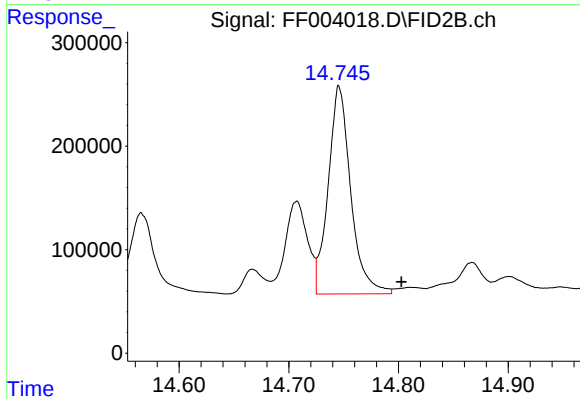

#10 N-TETRACOSANE


R.T.: 14.746 min
Delta R.T.: -0.057 min
Response: 2871111
Conc: 18.15 ug/ml

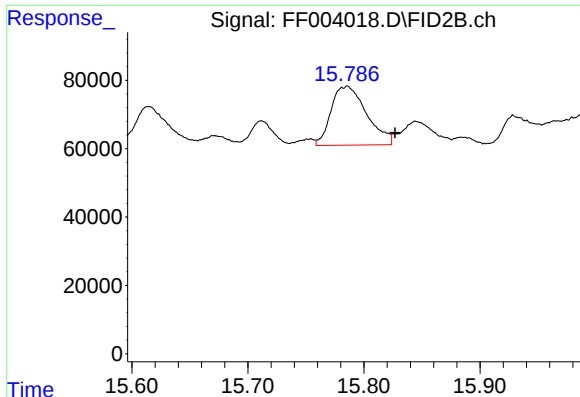

#11 N-HEXACOSANE


R.T.: 15.786 min
Delta R.T.: -0.041 min
Response: 366763
Conc: 2.38 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-11

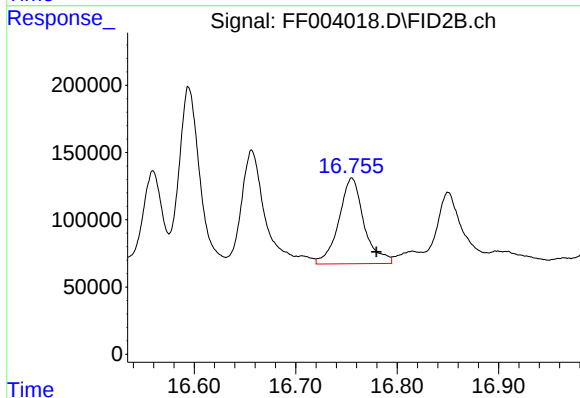


#12 N-OCTACOSANE

R.T.: 16.755 min
Delta R.T.: -0.024 min
Response: 1099062
Conc: 7.27 ug/ml

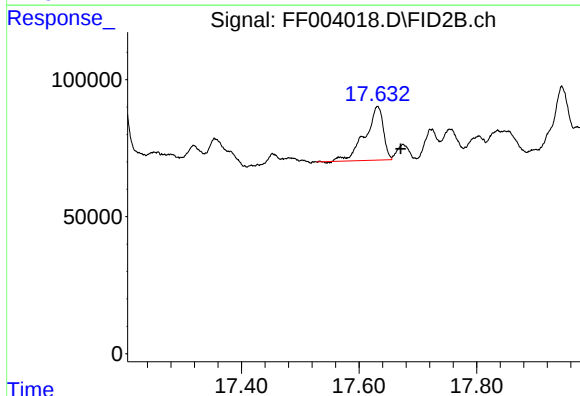


#13 N-TRIACONTANE

R.T.: 17.631 min
Delta R.T.: -0.039 min
Response: 419914
Conc: 2.85 ug/ml

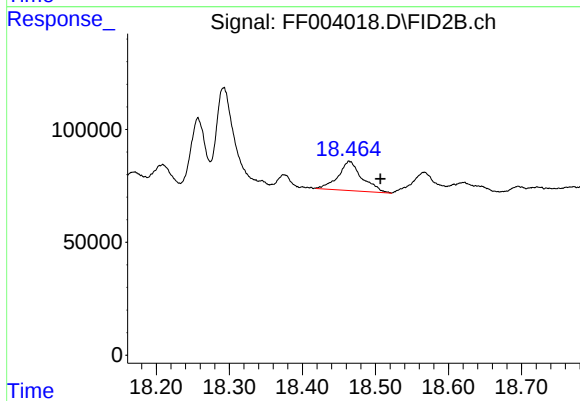

#14 N-DOTRIACONTANE

R.T.: 18.464 min
Delta R.T.: -0.042 min
Response: 293935
Conc: 2.07 ug/ml

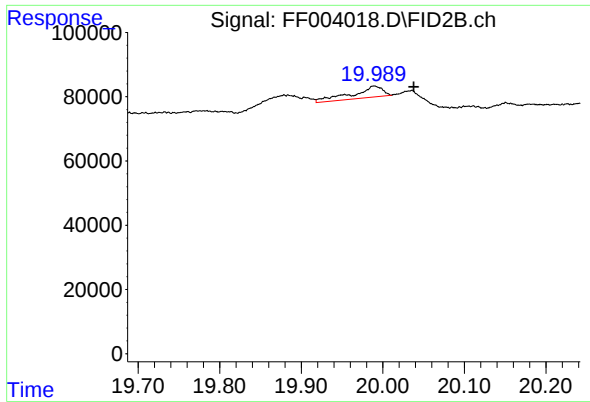

#16 N-HEXATRIACONTANE

R.T.: 19.989 min
Delta R.T.: -0.049 min
Response: 90833
Conc: 0.70 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-11