

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
 Data File : FF004019.D
 Signal(s) : FID2B.ch
 Acq On : 28 Mar 2019 12:43
 Operator : AJ\SJ
 Sample : K2086-03 5X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CS-13

Integration File: autoint1.e
 Quant Time: Mar 29 02:29:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.566	748673	5.377 ug/ml
Target Compounds			
6) N-OCTADECANE	11.240f	116263	0.706 ug/ml
7) N-EICOSANE	12.527	8569317	52.382 ug/ml
8) N-DOCOSANE	13.691	214595	1.330 ug/ml
10) N-TETRACOSANE	14.749f	4106740	25.956 ug/ml
11) N-HEXACOSANE	15.783	348744	2.260 ug/ml
12) N-OCTACOSANE	16.758	380678	2.519 ug/ml
13) N-TRIACONTANE	17.631	112864	0.767 ug/ml
14) N-DOTRIACONTANE	18.464	280371	1.972 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
Data File : FF004019.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2019 12:43
Operator : AJ\SJ
Sample : K2086-03 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CS-13

Integration File: autoint1.e
Quant Time: Mar 29 02:29:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

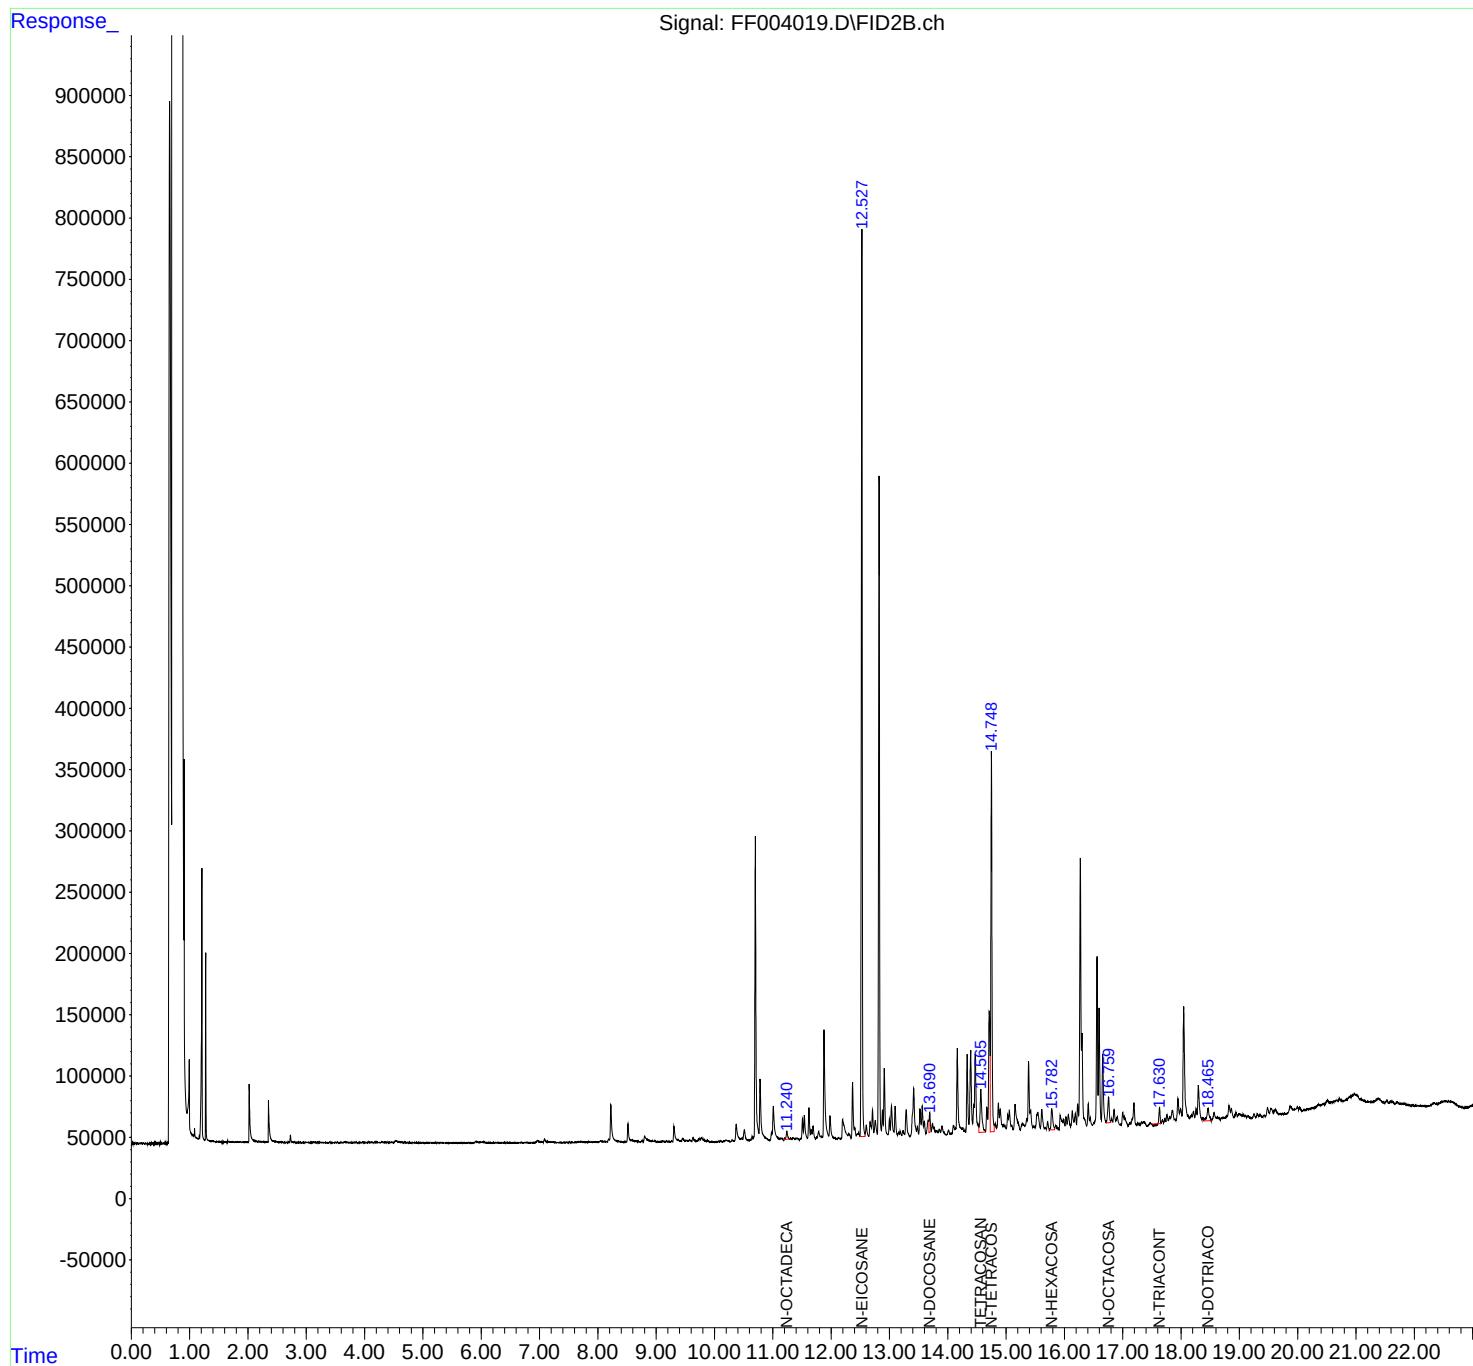


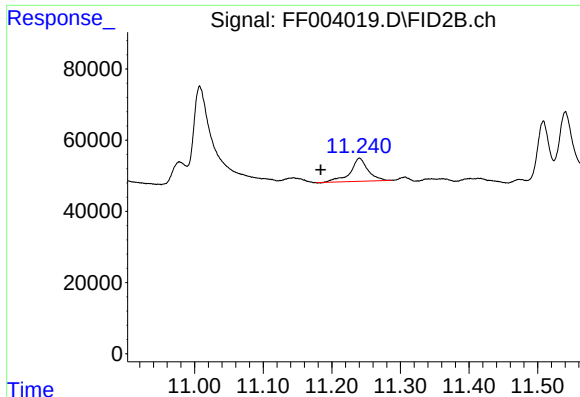

#6 N-OCTADECANE


R.T.: 11.240 min
Delta R.T.: 0.057 min
Response: 116263
Conc: 0.71 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-13

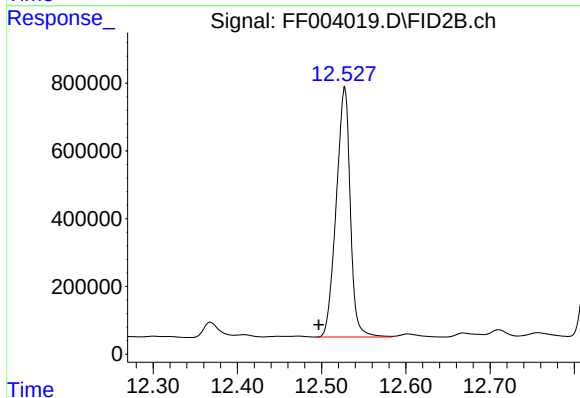


#7 N-EICOSANE

R.T.: 12.527 min
Delta R.T.: 0.031 min
Response: 8569317
Conc: 52.38 ug/ml

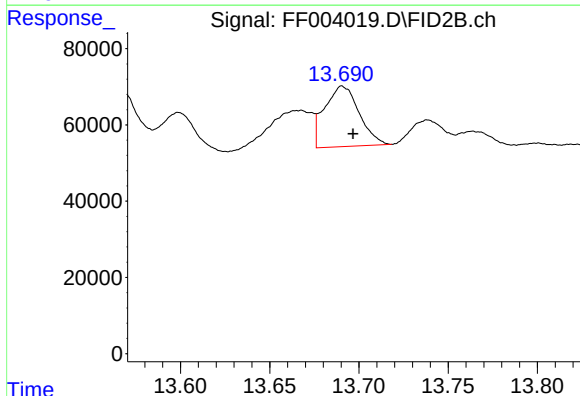


#8 N-DOCOSANE

R.T.: 13.691 min
Delta R.T.: -0.006 min
Response: 214595
Conc: 1.33 ug/ml

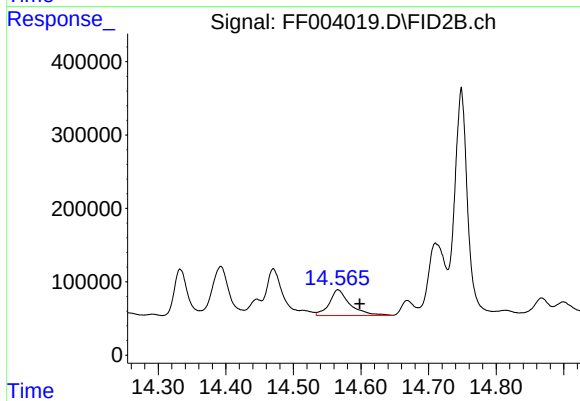

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.566 min
Delta R.T.: -0.032 min
Response: 748673
Conc: 5.38 ug/ml

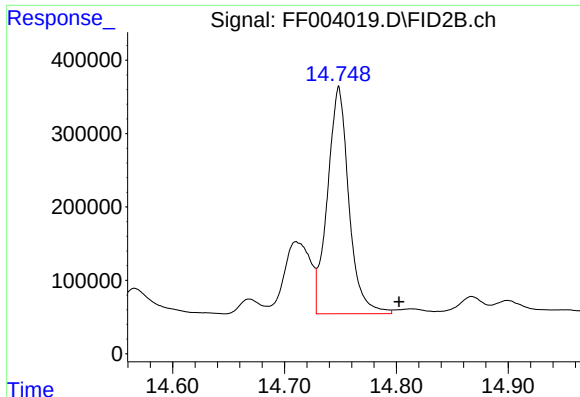

#10 N-TETRACOSANE


R.T.: 14.749 min
Delta R.T.: -0.054 min
Response: 4106740
Conc: 25.96 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-13

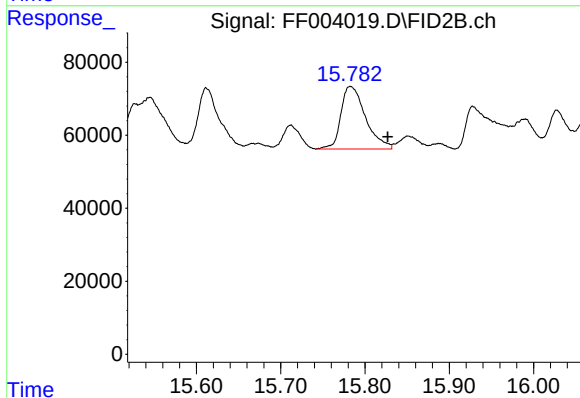


#11 N-HEXACOSANE

R.T.: 15.783 min
Delta R.T.: -0.044 min
Response: 348744
Conc: 2.26 ug/ml

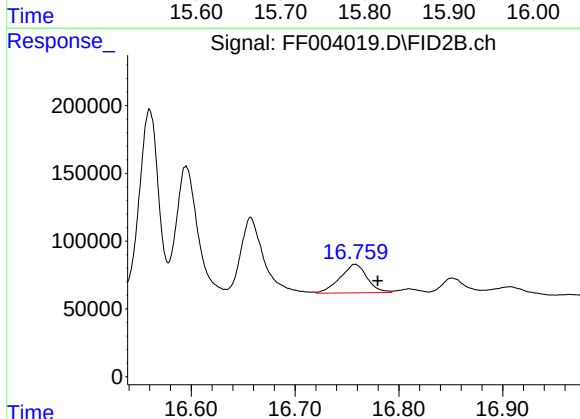


#12 N-OCTACOSANE

R.T.: 16.758 min
Delta R.T.: -0.022 min
Response: 380678
Conc: 2.52 ug/ml

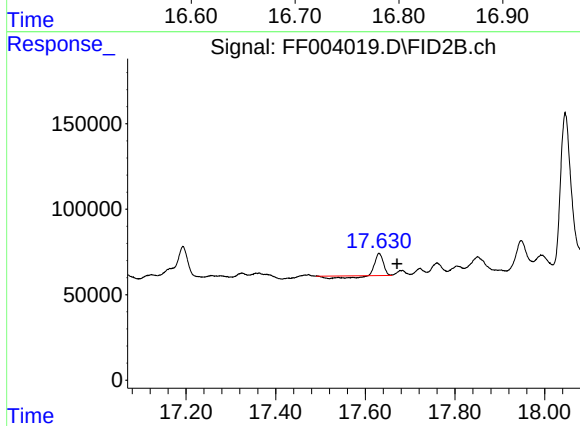

#13 N-TRIACONTANE

R.T.: 17.631 min
Delta R.T.: -0.040 min
Response: 112864
Conc: 0.77 ug/ml

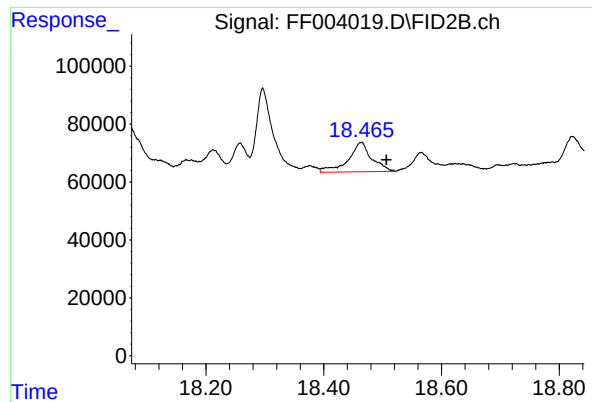

#14 N-DOTRIACONTANE

R.T.: 18.464 min
Delta R.T.: -0.043 min
Response: 280371
Conc: 1.97 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-13