

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
 Data File : FF004021.D
 Signal(s) : FID2B.ch
 Acq On : 28 Mar 2019 14:00
 Operator : AJ\SJ
 Sample : K2086-05 2X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CS-15

Integration File: autoint1.e
 Quant Time: Mar 29 02:29:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.566	1377202	9.892 ug/ml
Target Compounds			
7) N-EICOSANE	12.521	4566905	27.916 ug/ml
8) N-DOCOSANE	13.689	453867	2.812 ug/ml
10) N-TETRACOSANE	14.747f	2791165	17.641 ug/ml
11) N-HEXACOSANE	15.780	399242	2.587 ug/ml
12) N-OCTACOSANE	16.752	651165	4.309 ug/ml
13) N-TRIACONTANE	17.631	349369	2.375 ug/ml
14) N-DOTRIACONTANE	18.479	694672	4.885 ug/ml
15) N-TETRATRIACONTANE	19.308	278491	2.080 ug/ml
16) N-HEXATRIACONTANE	20.036	1347004	10.323 ug/ml
18) N-TETRACONTANE	21.627	2360206	18.972 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
Data File : FF004021.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2019 14:00
Operator : AJ\SJ
Sample : K2086-05 2X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CS-15

Integration File: autoint1.e
Quant Time: Mar 29 02:29:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

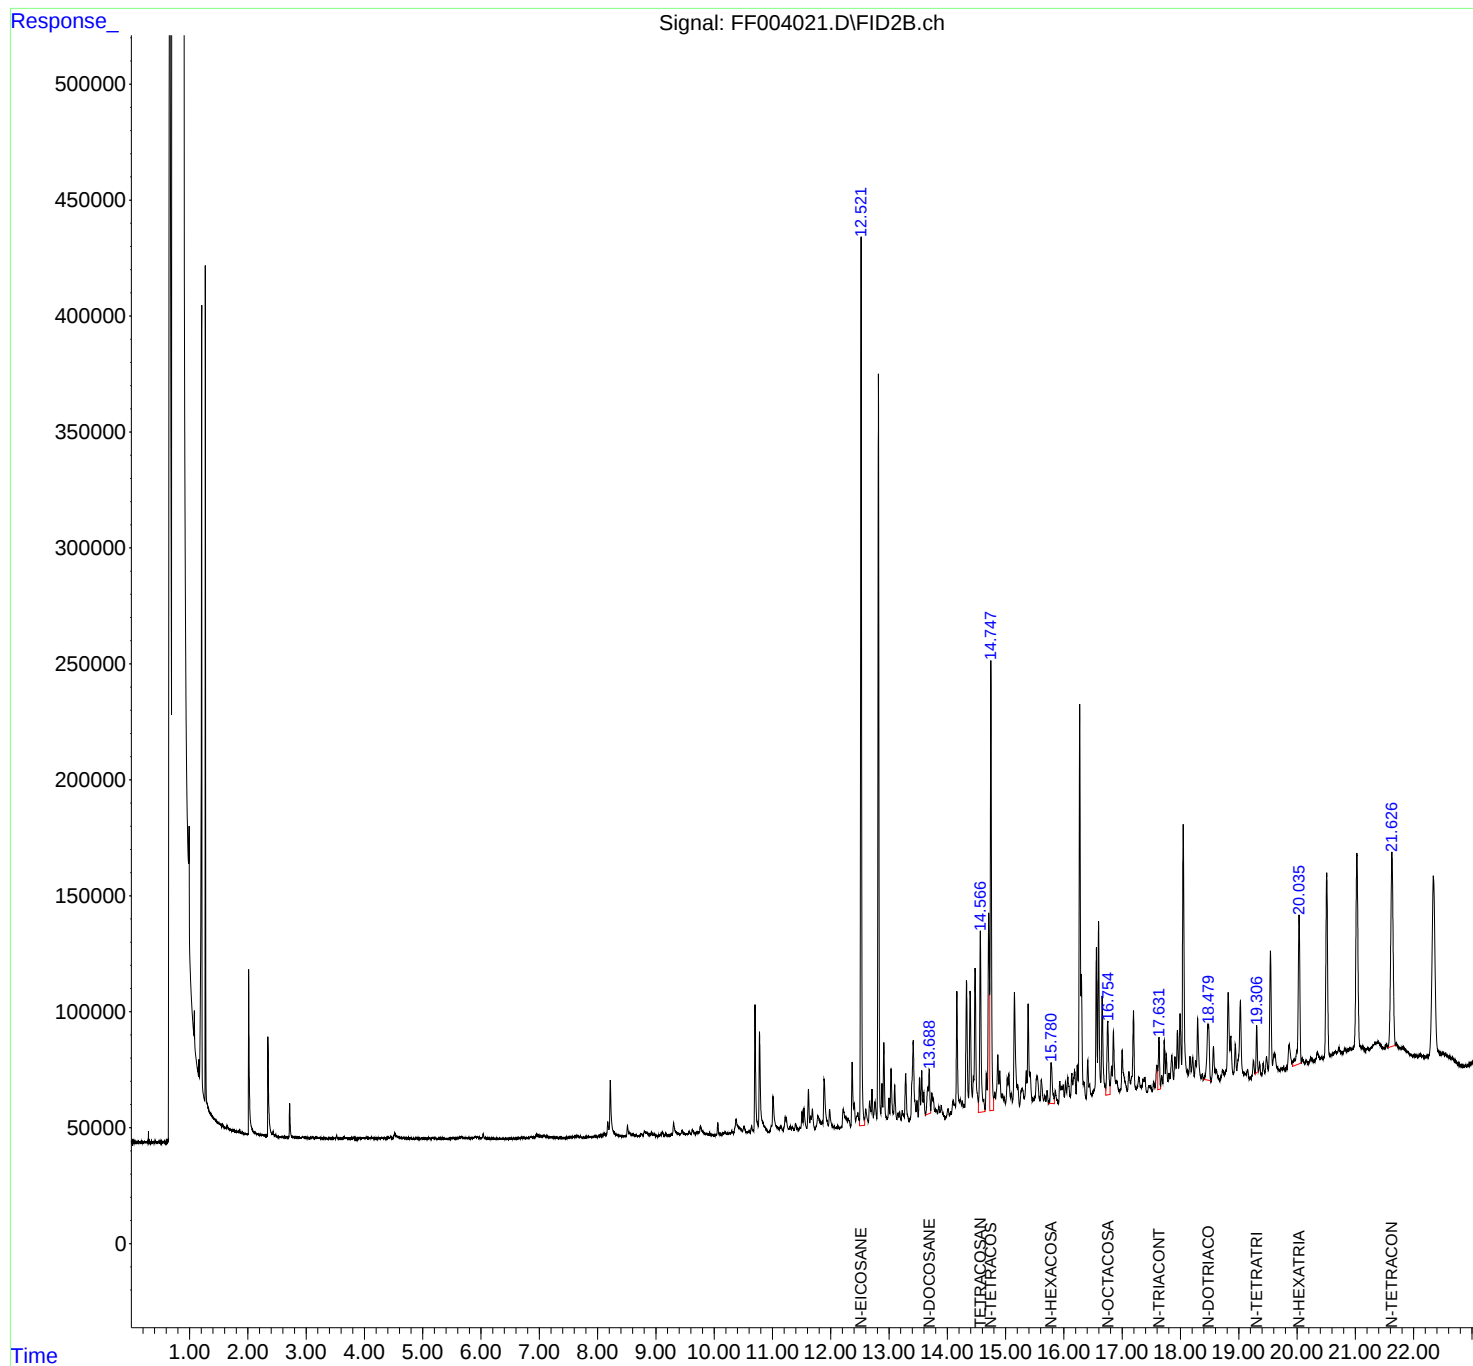


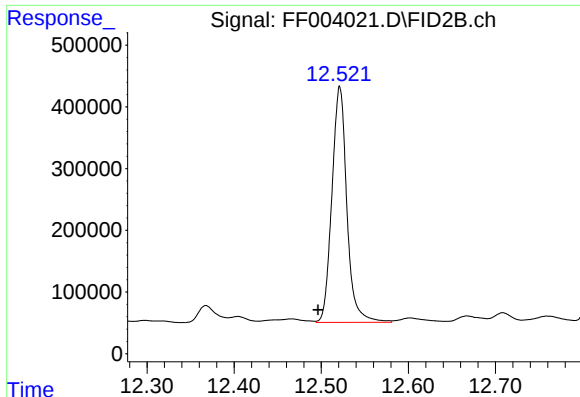

#7 N-EICOSANE


R.T.: 12.521 min
Delta R.T.: 0.025 min
Response: 4566905
Conc: 27.92 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-15

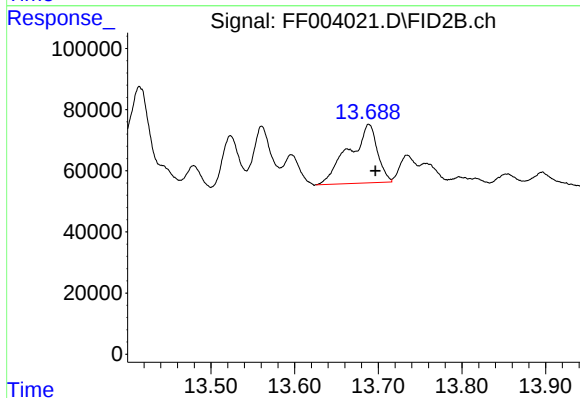


#8 N-DOCOSANE

R.T.: 13.689 min
Delta R.T.: -0.008 min
Response: 453867
Conc: 2.81 ug/ml

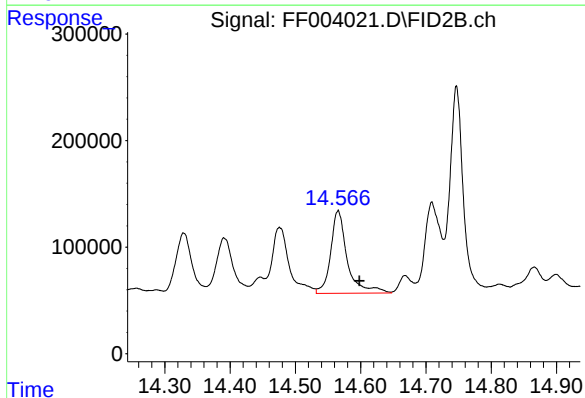


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.566 min
Delta R.T.: -0.033 min
Response: 1377202
Conc: 9.89 ug/ml

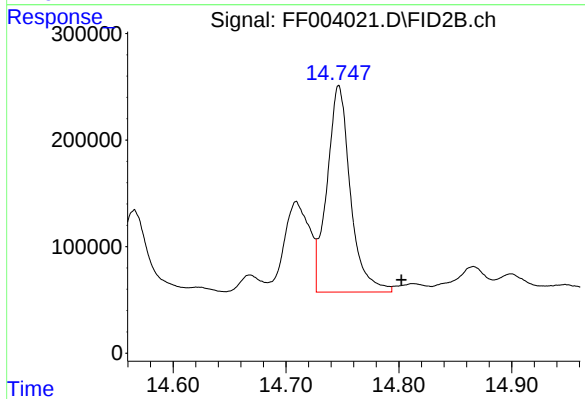

#10 N-TETRACOSANE


R.T.: 14.747 min
Delta R.T.: -0.056 min
Response: 2791165
Conc: 17.64 ug/ml

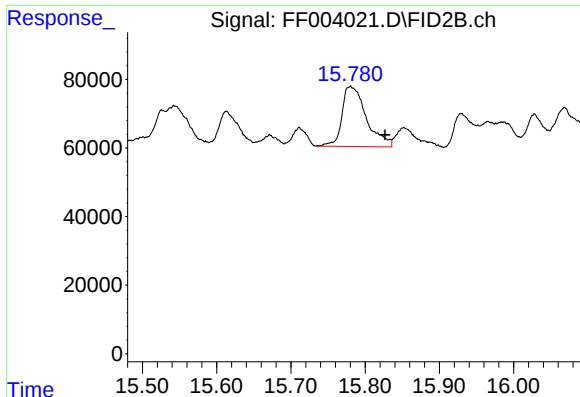

#11 N-HEXACOSANE


R.T.: 15.780 min
Delta R.T.: -0.046 min
Response: 399242
Conc: 2.59 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-15

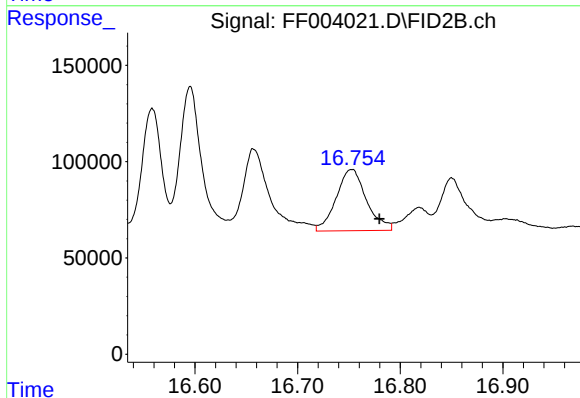


#12 N-OCTACOSANE

R.T.: 16.752 min
Delta R.T.: -0.027 min
Response: 651165
Conc: 4.31 ug/ml

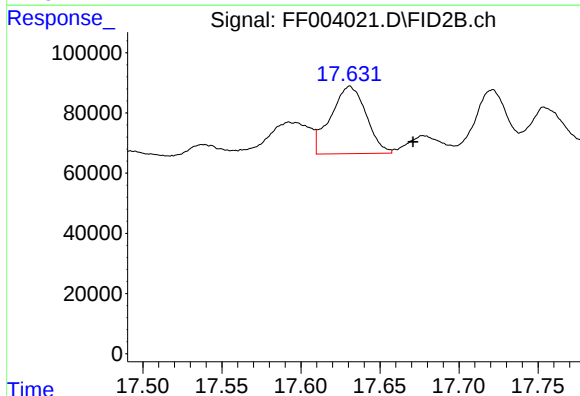


#13 N-TRIACONTANE

R.T.: 17.631 min
Delta R.T.: -0.040 min
Response: 349369
Conc: 2.38 ug/ml

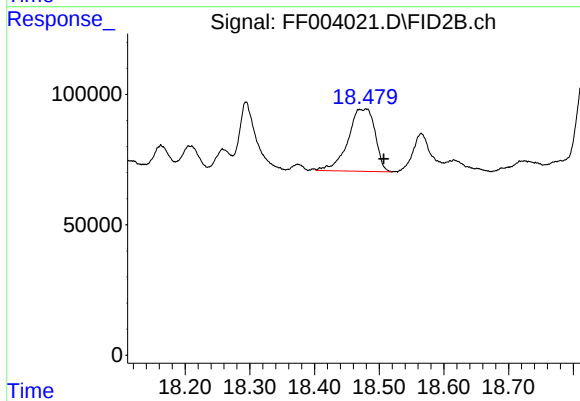

#14 N-DOTRIACONTANE


R.T.: 18.479 min
Delta R.T.: -0.028 min
Response: 694672
Conc: 4.88 ug/ml

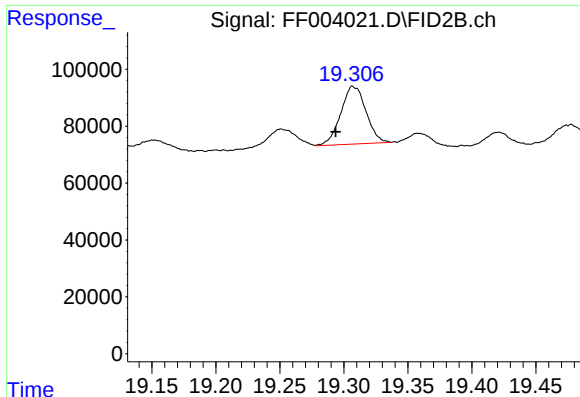

#15 N-TETRATRIACONTANE


R.T.: 19.308 min
Delta R.T.: 0.014 min
Response: 278491
Conc: 2.08 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-15

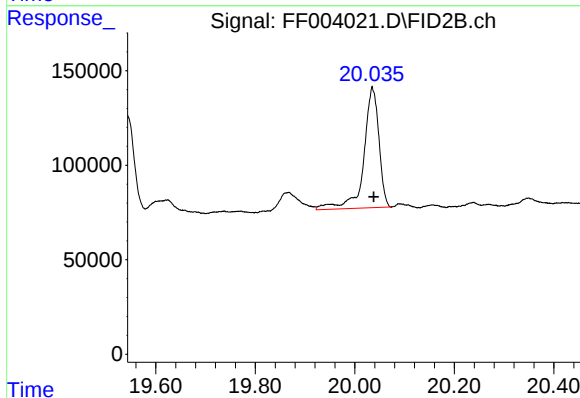

#16 N-HEXATRIACONTANE

R.T.: 20.036 min
Delta R.T.: -0.002 min
Response: 1347004
Conc: 10.32 ug/ml

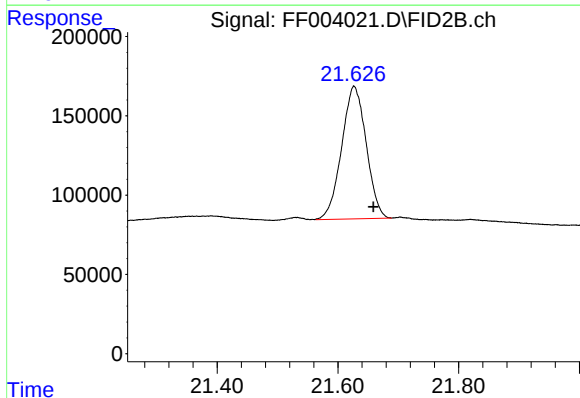

#18 N-TETRACONTANE

R.T.: 21.627 min
Delta R.T.: -0.032 min
Response: 2360206
Conc: 18.97 ug/ml