

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
 Data File : FF004025.D
 Signal(s) : FID2B.ch
 Acq On : 28 Mar 2019 16:08
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 29 02:30:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.569	2055743	14.765 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.746	174155	1.152 ug/ml
13) N-TRIACONTANE	17.637	87049	0.592 ug/ml
14) N-DOTRIACONTANE	18.535	40189	0.283 ug/ml
15) N-TETRATRIACONTANE	19.277	162202	1.211 ug/ml
16) N-HEXATRIACONTANE	20.043	1250291	9.582 ug/ml
17) N-OCTATRIACONTANE	20.760	633568	5.487 ug/ml
18) N-TETRACONTANE	21.630	340470	2.737 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
Data File : FF004025.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2019 16:08
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 29 02:30:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

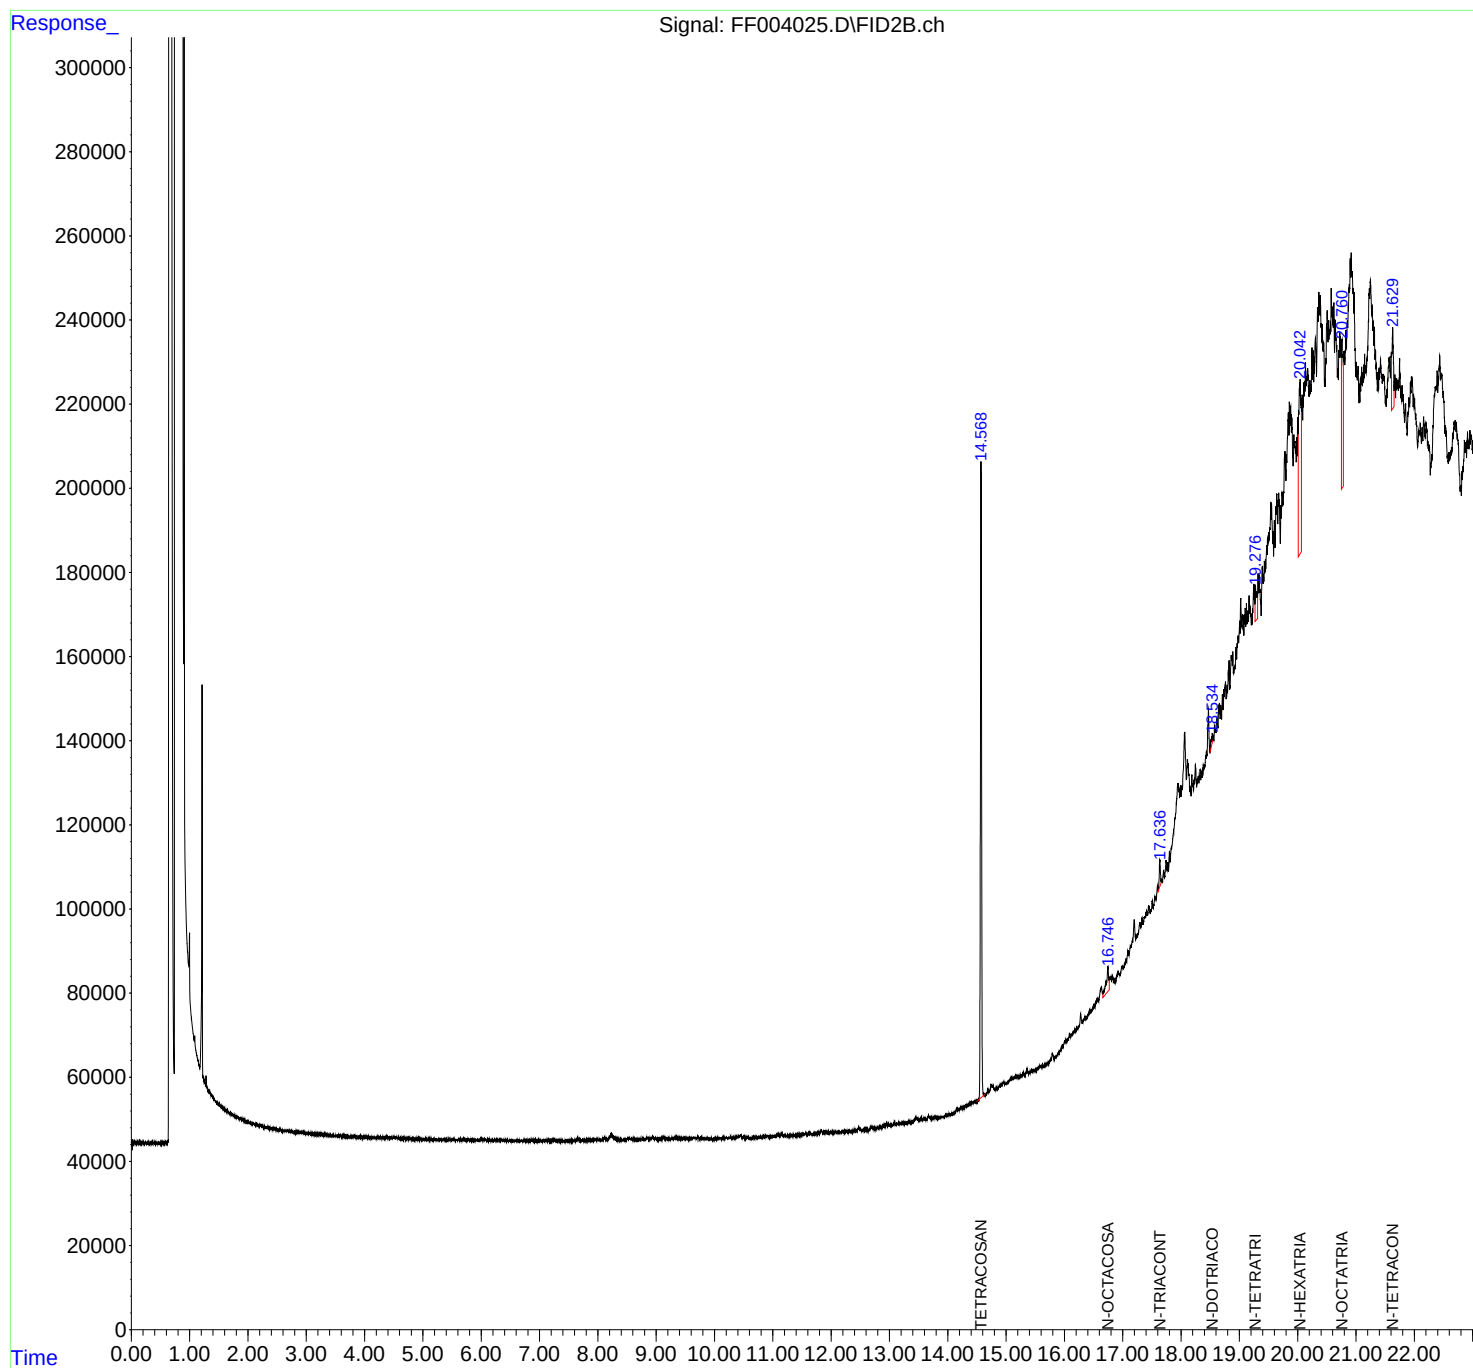


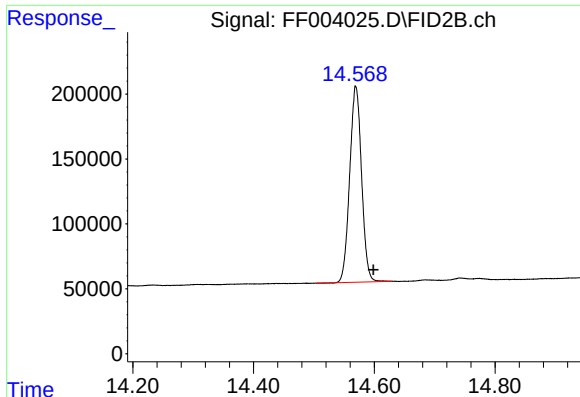

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.569 min
Delta R.T.: -0.029 min
Response: 2055743
Conc: 14.77 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

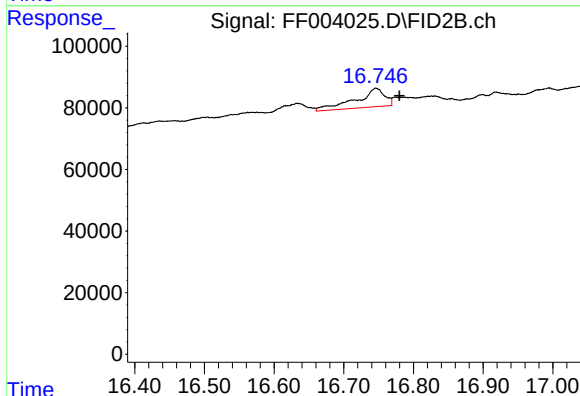


#12 N-OCTACOSANE

R.T.: 16.746 min
Delta R.T.: -0.033 min
Response: 174155
Conc: 1.15 ug/ml

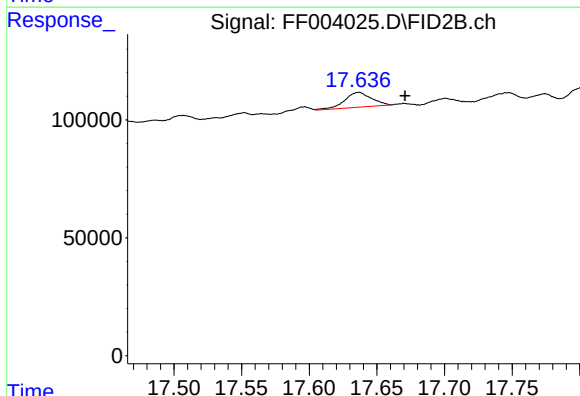


#13 N-TRIACONTANE

R.T.: 17.637 min
Delta R.T.: -0.034 min
Response: 87049
Conc: 0.59 ug/ml

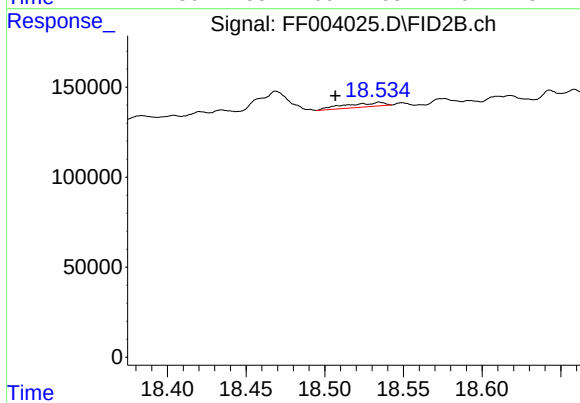

#14 N-DOTRIACONTANE


R.T.: 18.535 min
Delta R.T.: 0.028 min
Response: 40189
Conc: 0.28 ug/ml

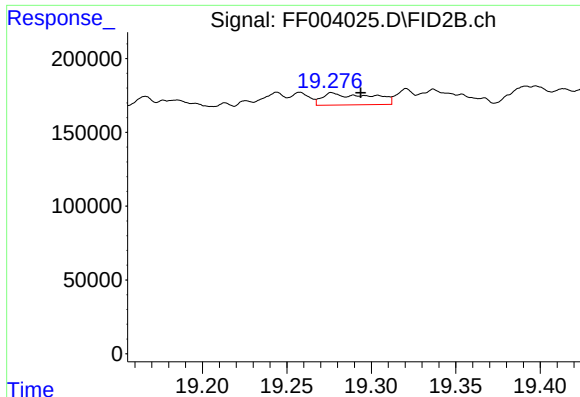

#15 N-TETRATRIACONTANE


R.T.: 19.277 min
Delta R.T.: -0.017 min
Response: 162202
Conc: 1.21 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

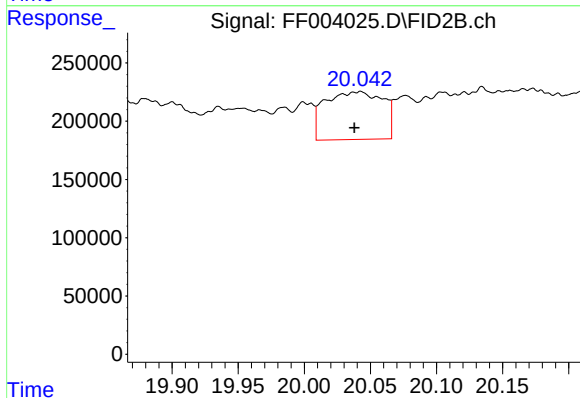


#16 N-HEXATRIACONTANE

R.T.: 20.043 min
Delta R.T.: 0.005 min
Response: 1250291
Conc: 9.58 ug/ml

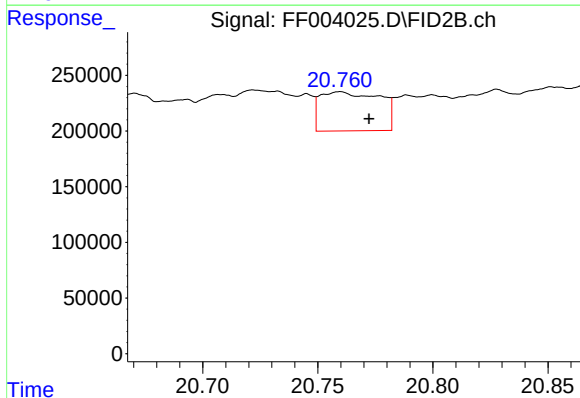

#17 N-OCTATRIACONTANE

R.T.: 20.760 min
Delta R.T.: -0.013 min
Response: 633568
Conc: 5.49 ug/ml

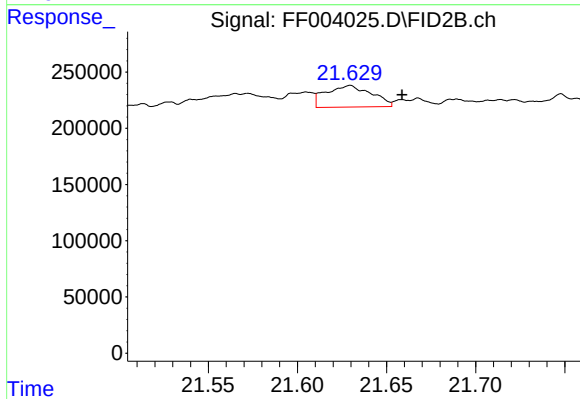

#18 N-TETRACONTANE

R.T.: 21.630 min
Delta R.T.: -0.029 min
Response: 340470
Conc: 2.74 ug/ml