

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
 Data File : FF004030.D
 Signal(s) : FID2B.ch
 Acq On : 28 Mar 2019 18:47
 Operator : AJ\SJ
 Sample : K2121-07
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 FIELD-BLANK

Integration File: autoint1.e
 Quant Time: Mar 29 02:32:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.569	1897884	13.631 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.635	71545	0.486 ug/ml
14) N-DOTRIACONTANE	18.470	111070	0.781 ug/ml
16) N-HEXATRIACONTANE	20.039	121449	0.931 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
Data File : FF004030.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2019 18:47
Operator : AJ\SJ
Sample : K2121-07
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
FIELD-BLANK

Integration File: autoint1.e
Quant Time: Mar 29 02:32:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

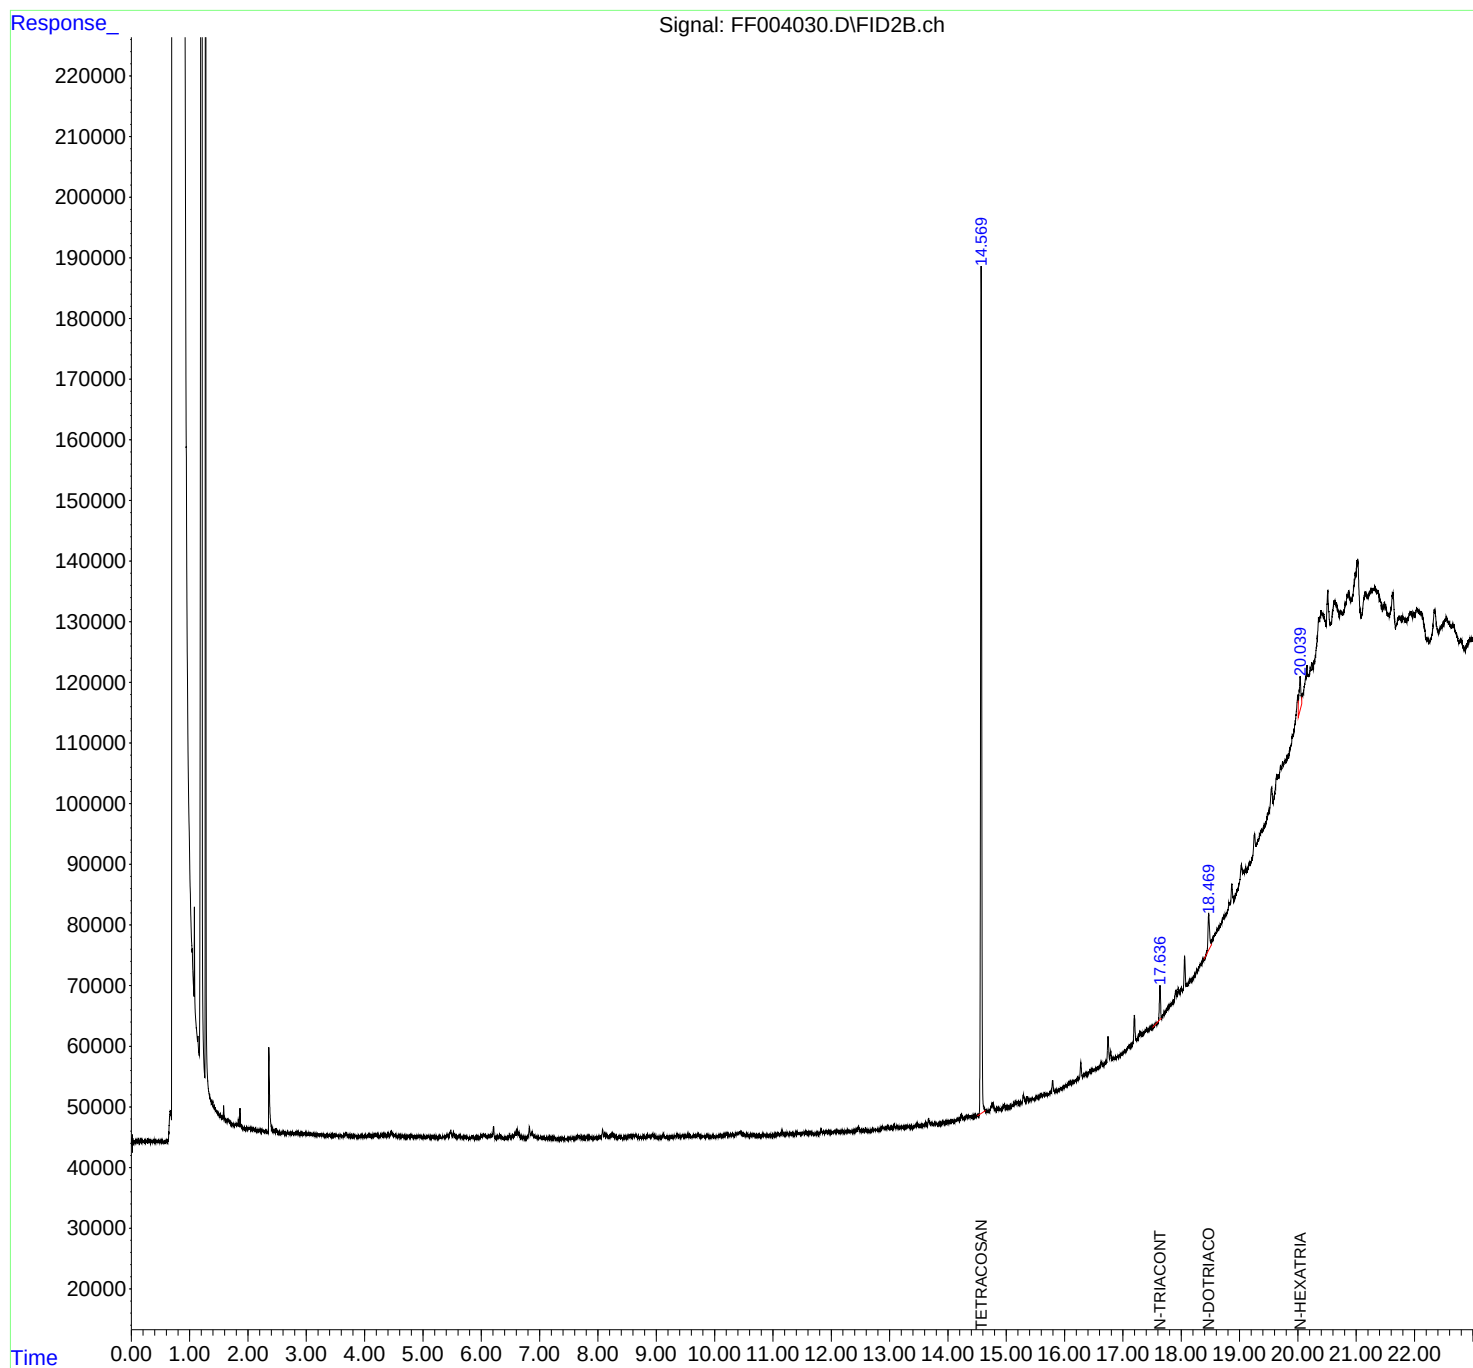


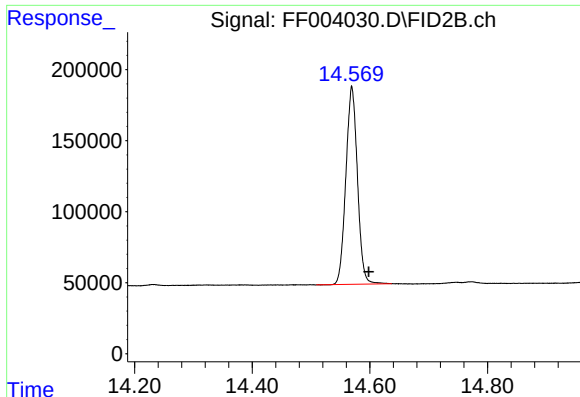

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.569 min
Delta R.T.: -0.029 min
Response: 1897884
Conc: 13.63 ug/ml

Instrument :
FID_F
ClientSampleId :
FIELD-BLANK

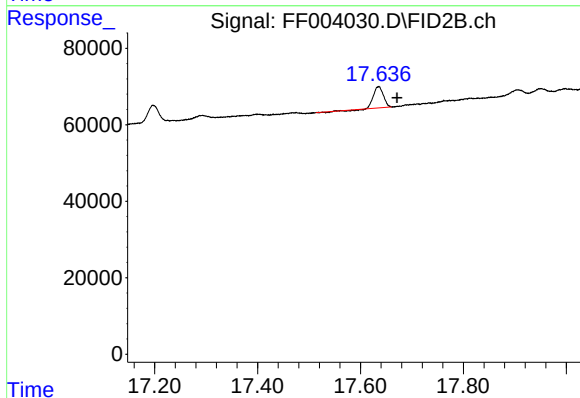


#13 N-TRIACONTANE

R.T.: 17.635 min
Delta R.T.: -0.036 min
Response: 71545
Conc: 0.49 ug/ml

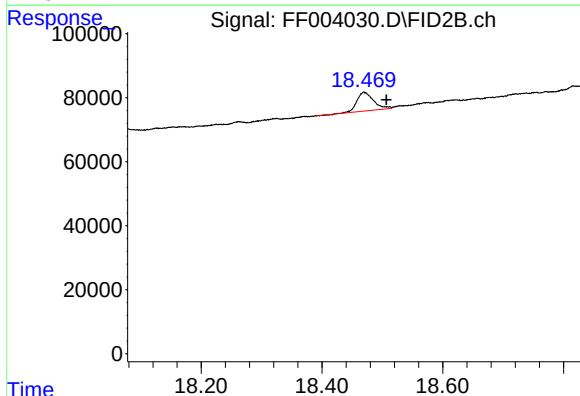

#14 N-DOTRIACONTANE

R.T.: 18.470 min
Delta R.T.: -0.037 min
Response: 111070
Conc: 0.78 ug/ml

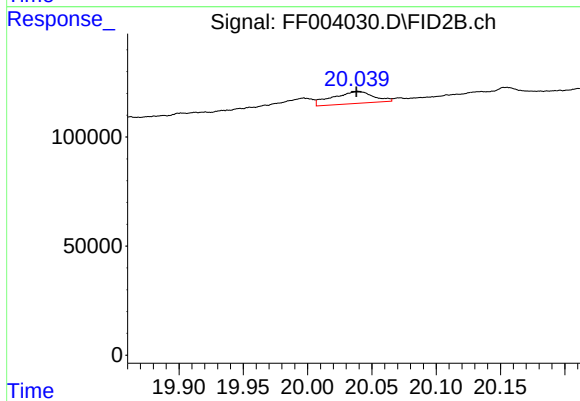

#16 N-HEXATRIACONTANE

R.T.: 20.039 min
Delta R.T.: 0.001 min
Response: 121449
Conc: 0.93 ug/ml