

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
 Data File : FF004031.D
 Signal(s) : FID2B.ch
 Acq On : 28 Mar 2019 19:18
 Operator : AJ\SJ
 Sample : K2112-03
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 DR-WC-001

Integration File: autoint1.e
 Quant Time: Mar 29 02:32:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.568	1387658	9.967 ug/ml
Target Compounds			
4) N-TETRADECANE	8.179	254565	1.588 ug/ml
12) N-OCTACOSANE	16.745	158276	1.047 ug/ml
13) N-TRIACONTANE	17.634	225775	1.535 ug/ml
14) N-DOTRIACONTANE	18.469	184030	1.294 ug/ml
15) N-TETRATRIACONTANE	19.255	567	0.004 ug/ml
16) N-HEXATRIACONTANE	20.038	69736	0.534 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
Data File : FF004031.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2019 19:18
Operator : AJ\SJ
Sample : K2112-03
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
DR-WC-001

Integration File: autoint1.e
Quant Time: Mar 29 02:32:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

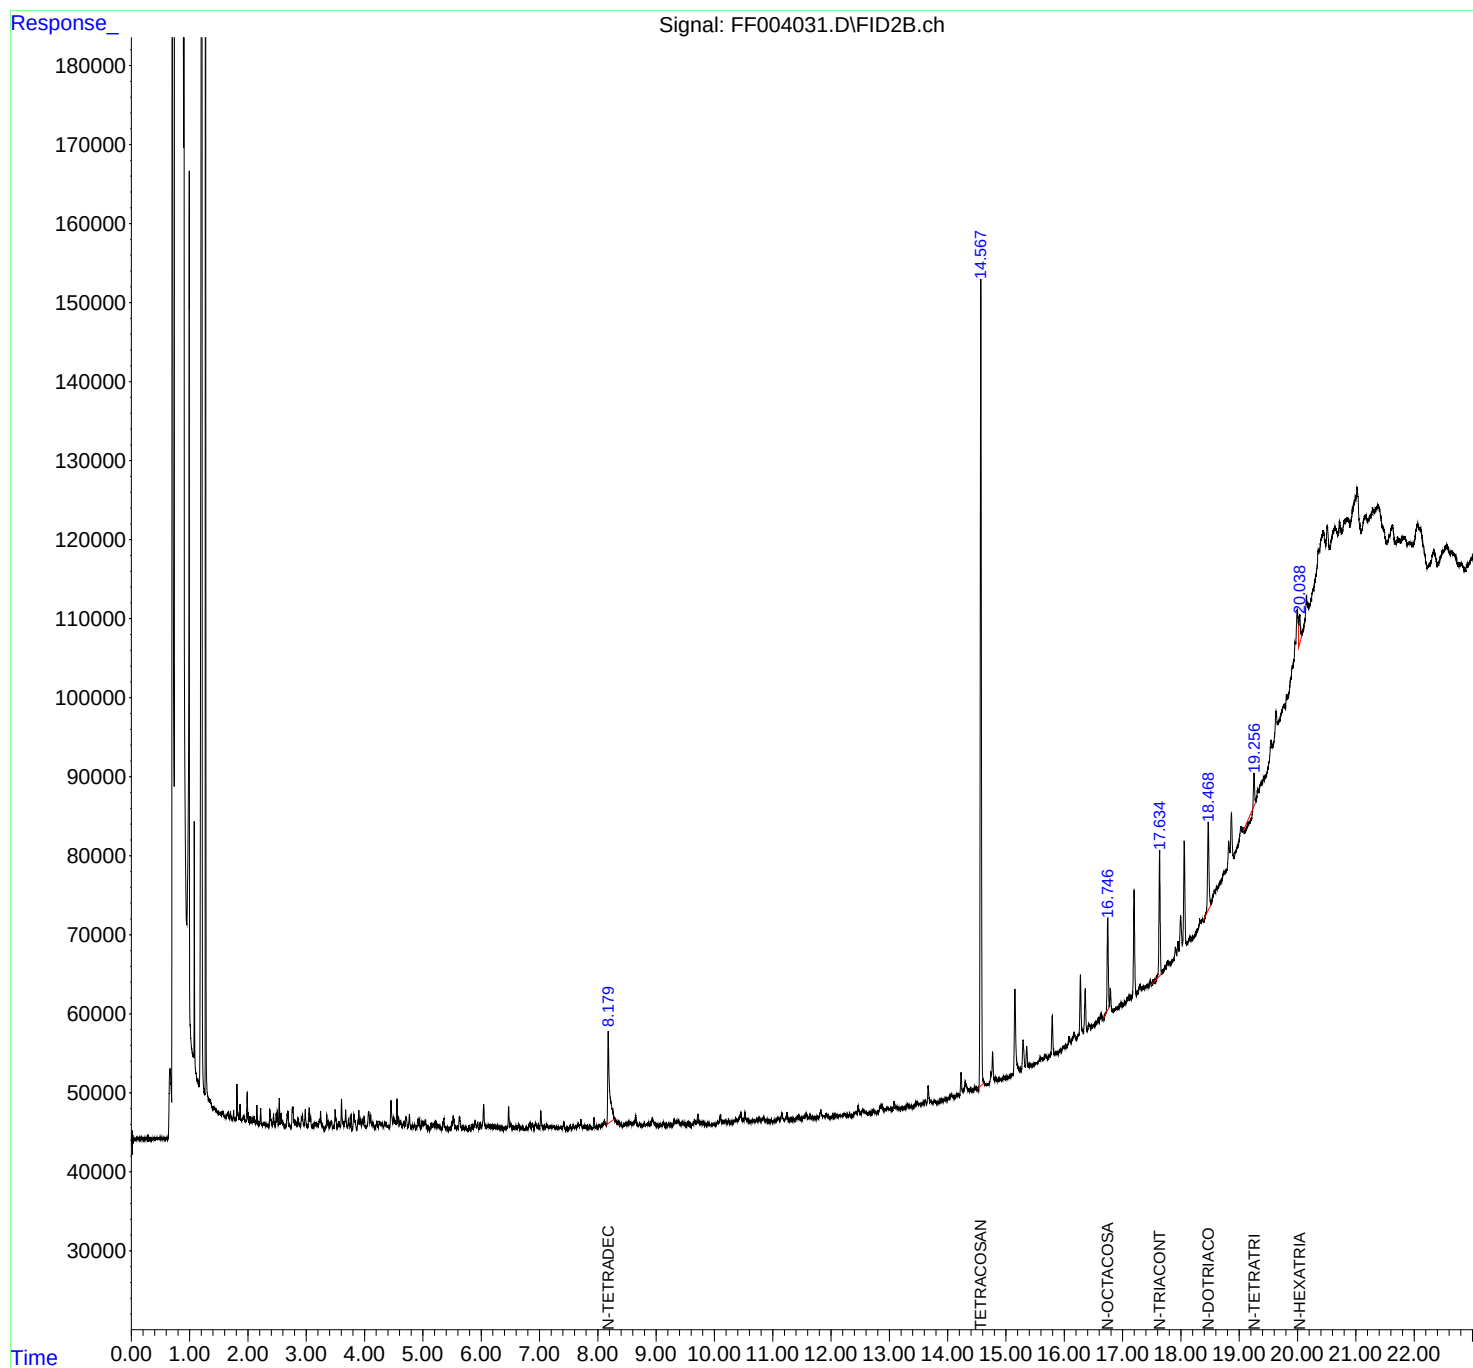


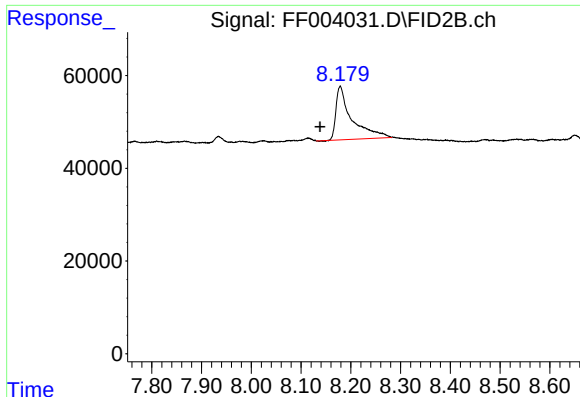

#4 N-TETRADECANE


R.T.: 8.179 min
Delta R.T.: 0.040 min
Response: 254565
Conc: 1.59 ug/ml

Instrument :
FID_F
ClientSampleId :
DR-WC-001

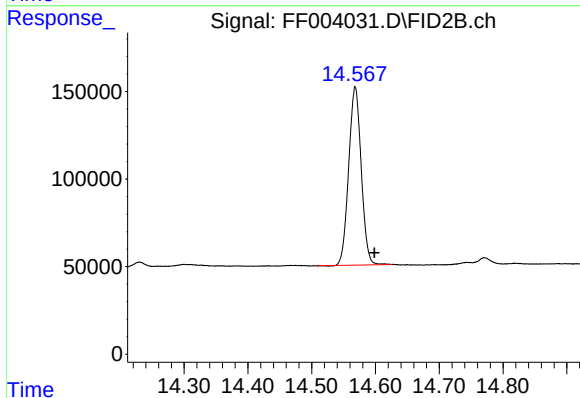


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.568 min
Delta R.T.: -0.030 min
Response: 1387658
Conc: 9.97 ug/ml

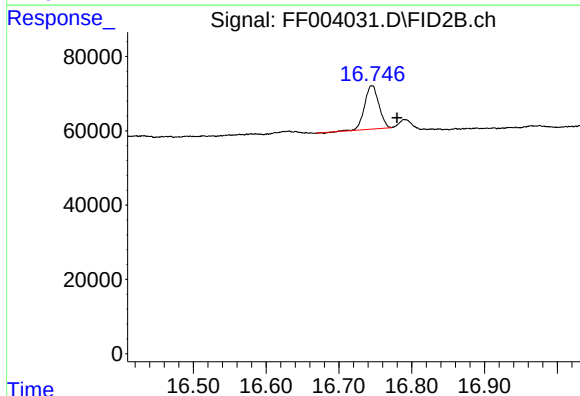


#12 N-OCTACOSANE

R.T.: 16.745 min
Delta R.T.: -0.034 min
Response: 158276
Conc: 1.05 ug/ml

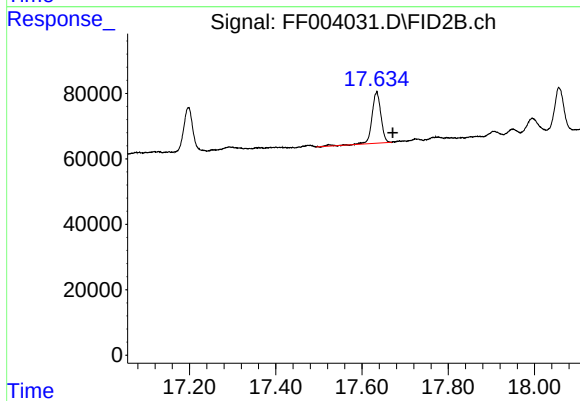

#13 N-TRIACONTANE


R.T.: 17.634 min
Delta R.T.: -0.037 min
Response: 225775
Conc: 1.53 ug/ml

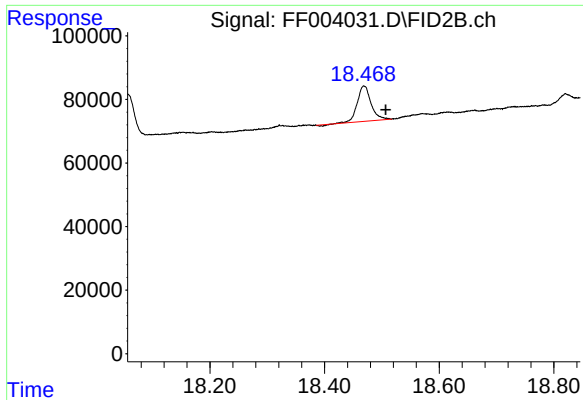

#14 N-DOTRIACONTANE


R.T.: 18.469 min
Delta R.T.: -0.038 min
Response: 184030
Conc: 1.29 ug/ml

Instrument :
FID_F
ClientSampleId :
DR-WC-001

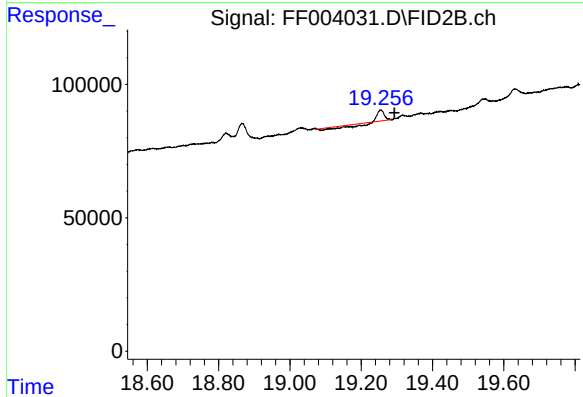

#15 N-TETRATRIACONTANE

R.T.: 19.255 min
Delta R.T.: -0.039 min
Response: 567
Conc: 0.00 ug/ml

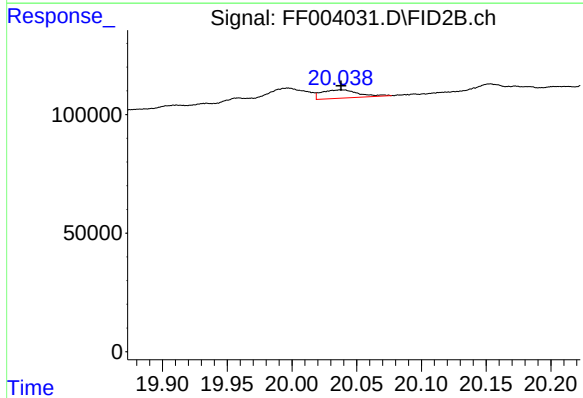

#16 N-HEXATRIACONTANE

R.T.: 20.038 min
Delta R.T.: 0.000 min
Response: 69736
Conc: 0.53 ug/ml