

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
Data File : FF004034.D
Signal(s) : FID2B.ch
Acq On : 29 Mar 2019 01:58
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Mar 29 02:33:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.466	125375	0.882 ug/ml
16)	N-HEXATRIACONTANE	19.991	56516	0.433 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032819\
Data File : FF004034.D
Signal(s) : FID2B.ch
Acq On : 29 Mar 2019 01:58
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Mar 29 02:33:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

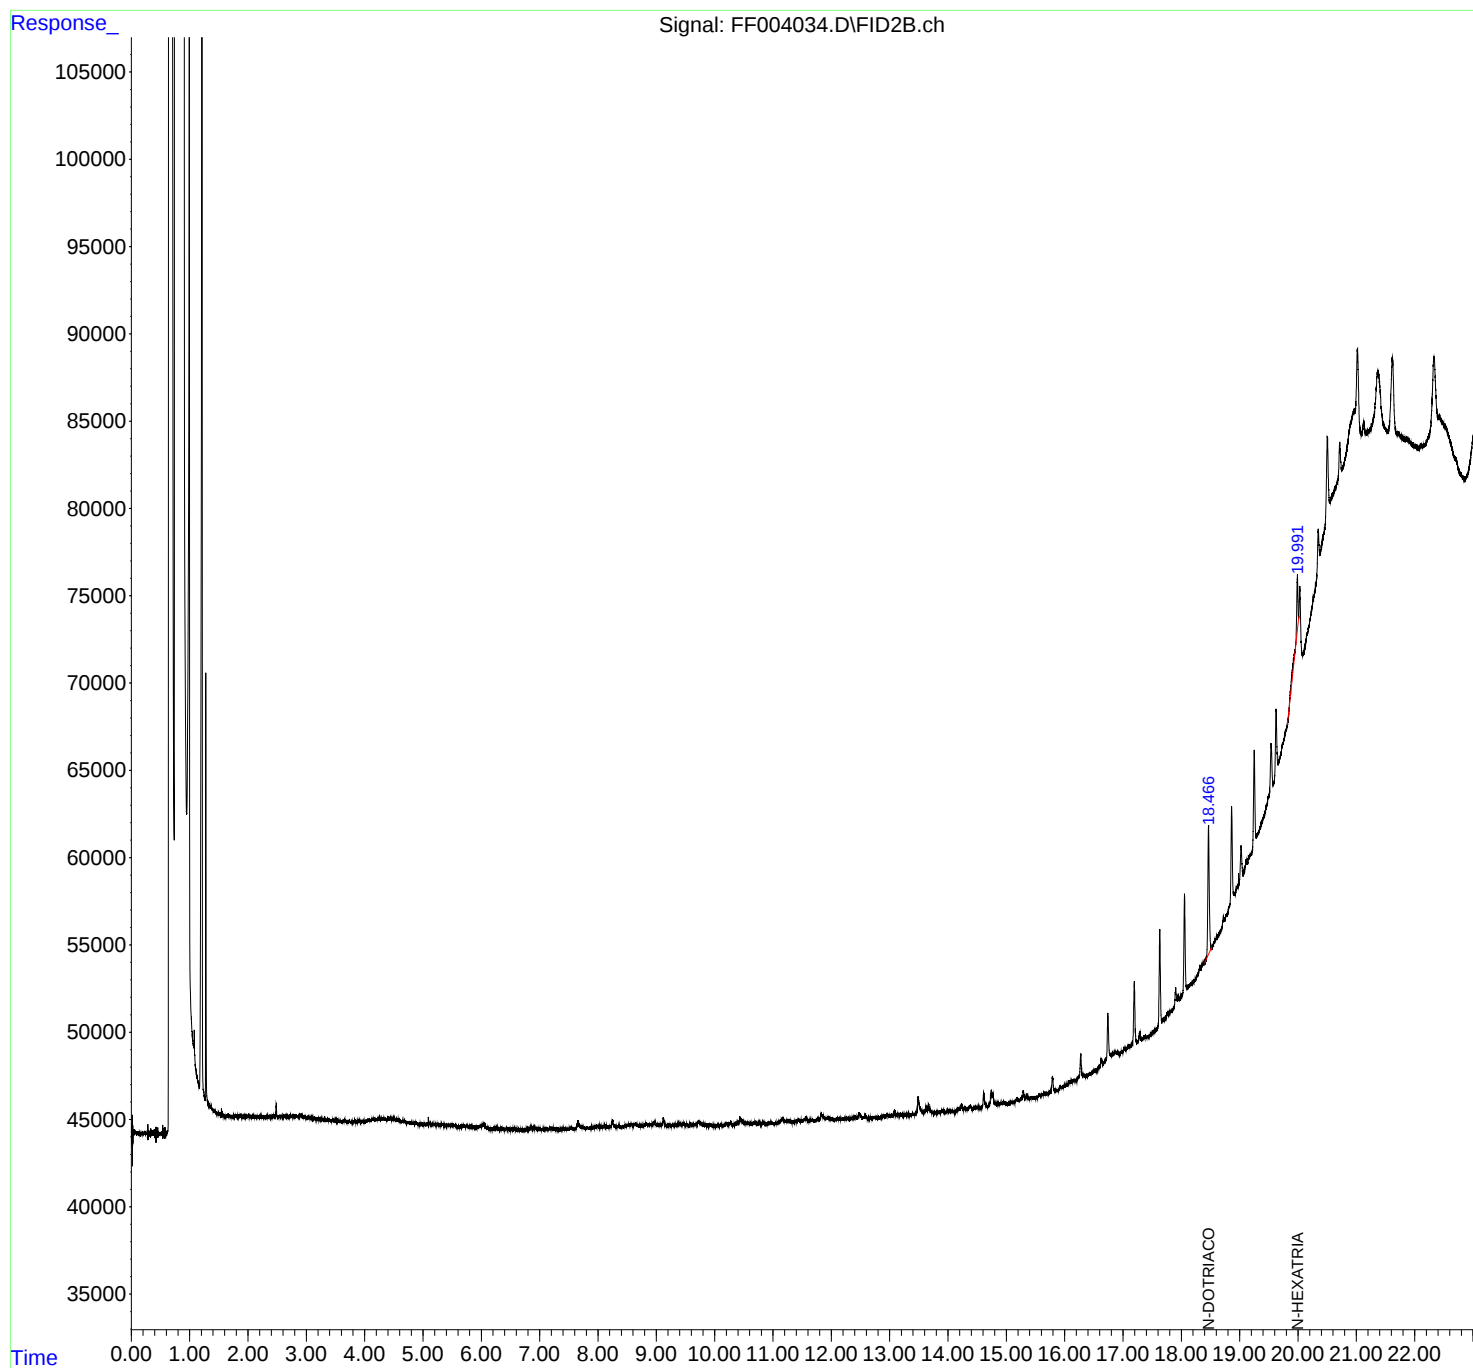


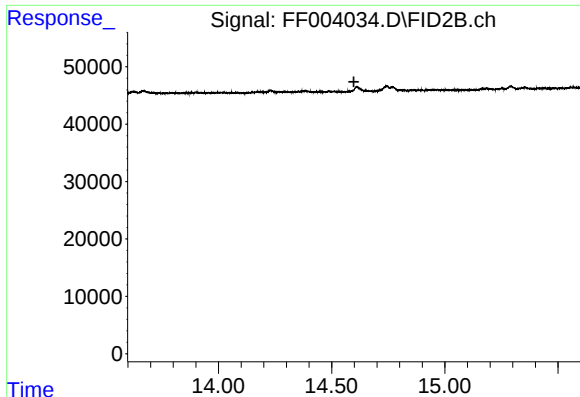

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.598 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
MECL2

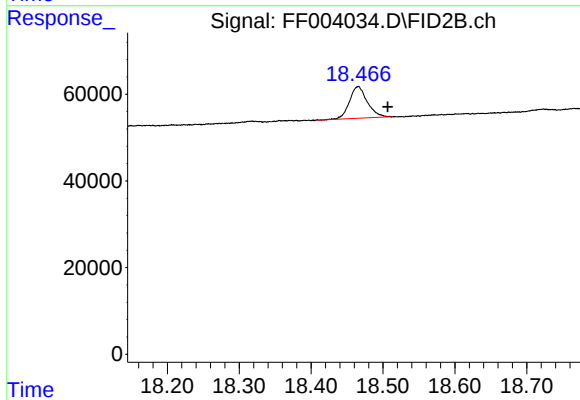

#14 N-DOTRIACONTANE

R.T.: 18.466 min
Delta R.T.: -0.041 min
Response: 125375
Conc: 0.88 ug/ml

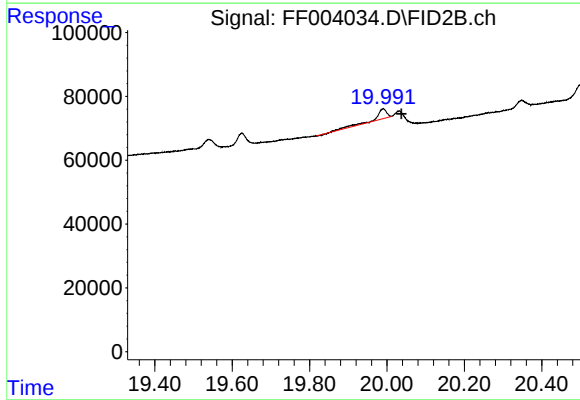

#16 N-HEXATRIACONTANE

R.T.: 19.991 min
Delta R.T.: -0.047 min
Response: 56516
Conc: 0.43 ug/ml