

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032822\
Data File : FF010186.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2022 10:23
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 29 02:16:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.637	1928337	15.787 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032822\
Data File : FF010186.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2022 10:23
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 29 02:16:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

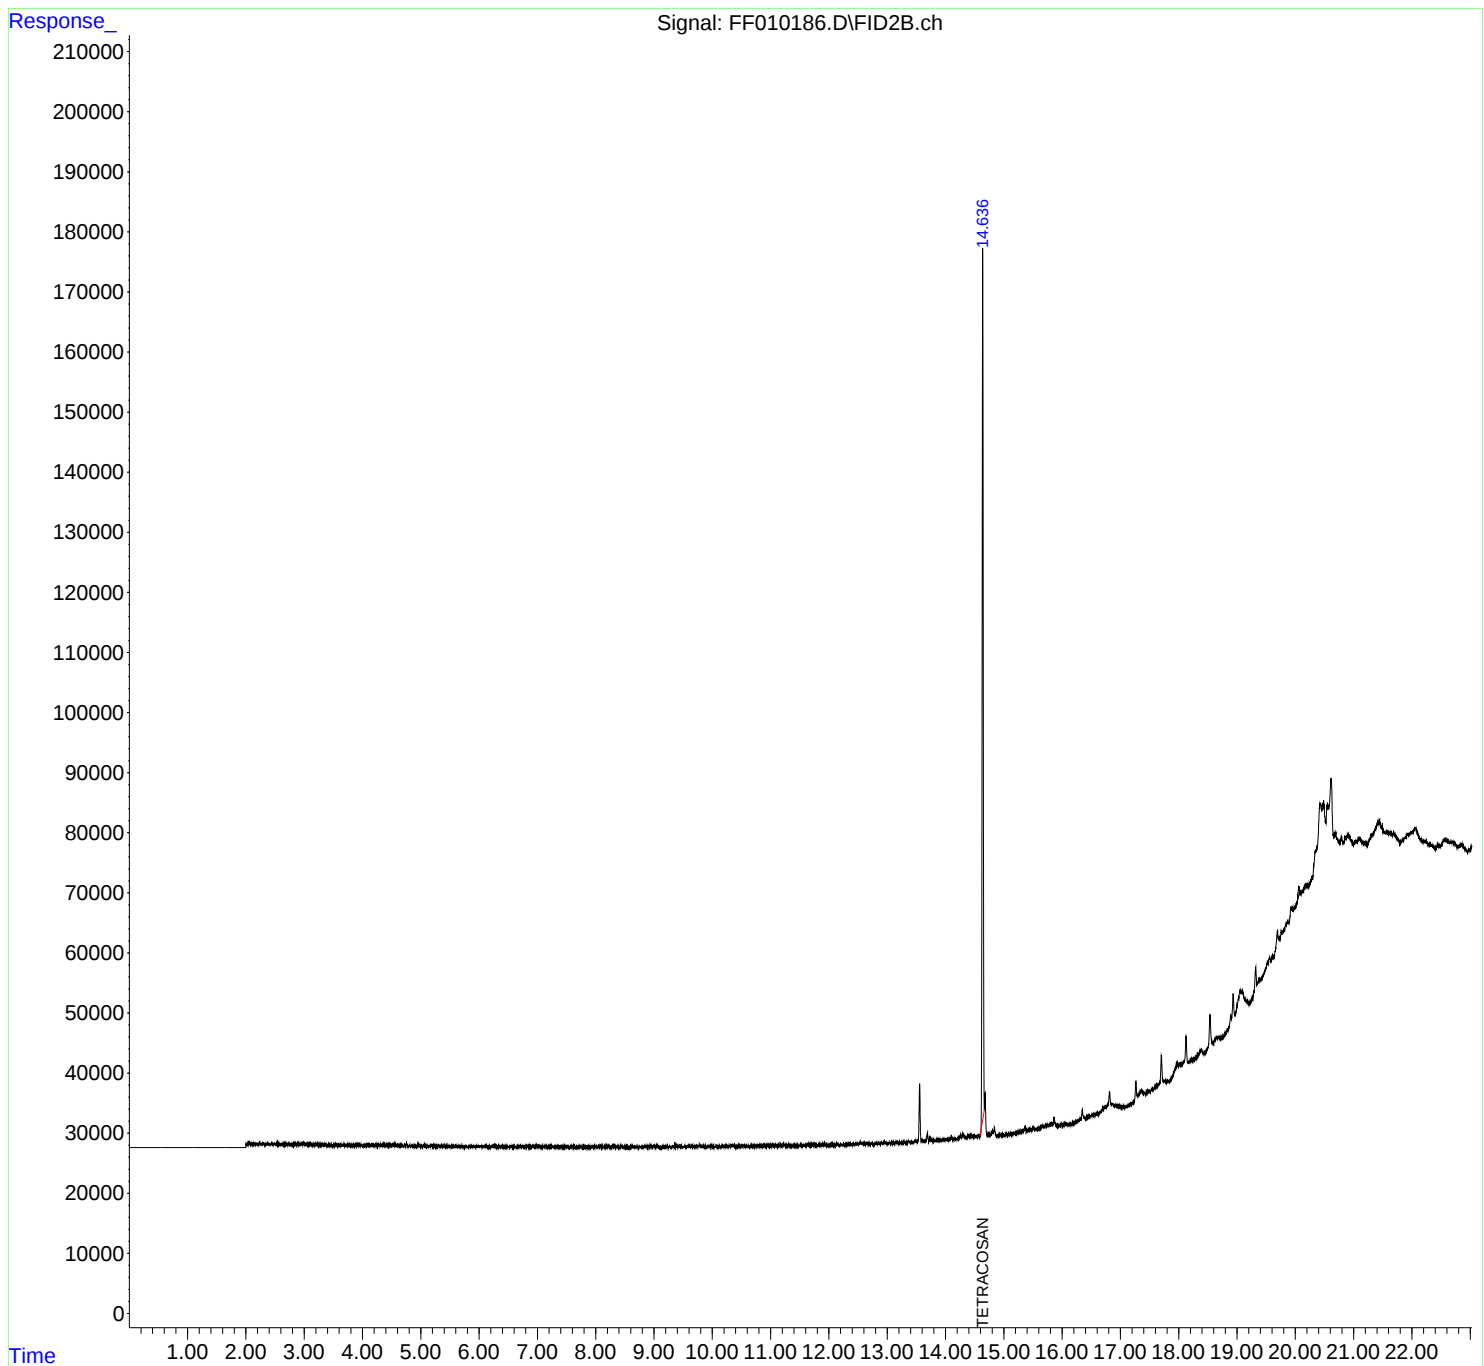

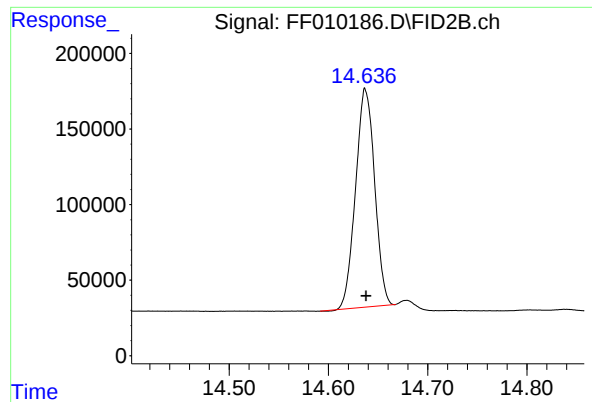

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.637 min
Delta R.T.: 0.000 min
Response: 1928337
Conc: 15.79 ug/ml

Instrument :
FID_F
ClientSampleId :