

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032822\
 Data File : FF010193.D
 Signal(s) : FID2B.ch
 Acq On : 28 Mar 2022 14:17
 Operator : AJ\MA
 Sample : N1974-09 5X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 29 02:17:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
 Quant Title :
 QLast Update : Sat Mar 26 09:58:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.636	377558	3.091 ug/ml
Target Compounds			
7) N-EICOSANE	12.591f	1239671	8.866 ug/ml
8) N-DOCOSANE	13.755	115465	0.838 ug/ml
10) N-TETRACOSANE	14.809	495655	3.624 ug/ml
12) N-OCTACOSANE	16.808	109174	0.830 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032822\
Data File : FF010193.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2022 14:17
Operator : AJ\MA
Sample : N1974-09 5X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 29 02:17:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

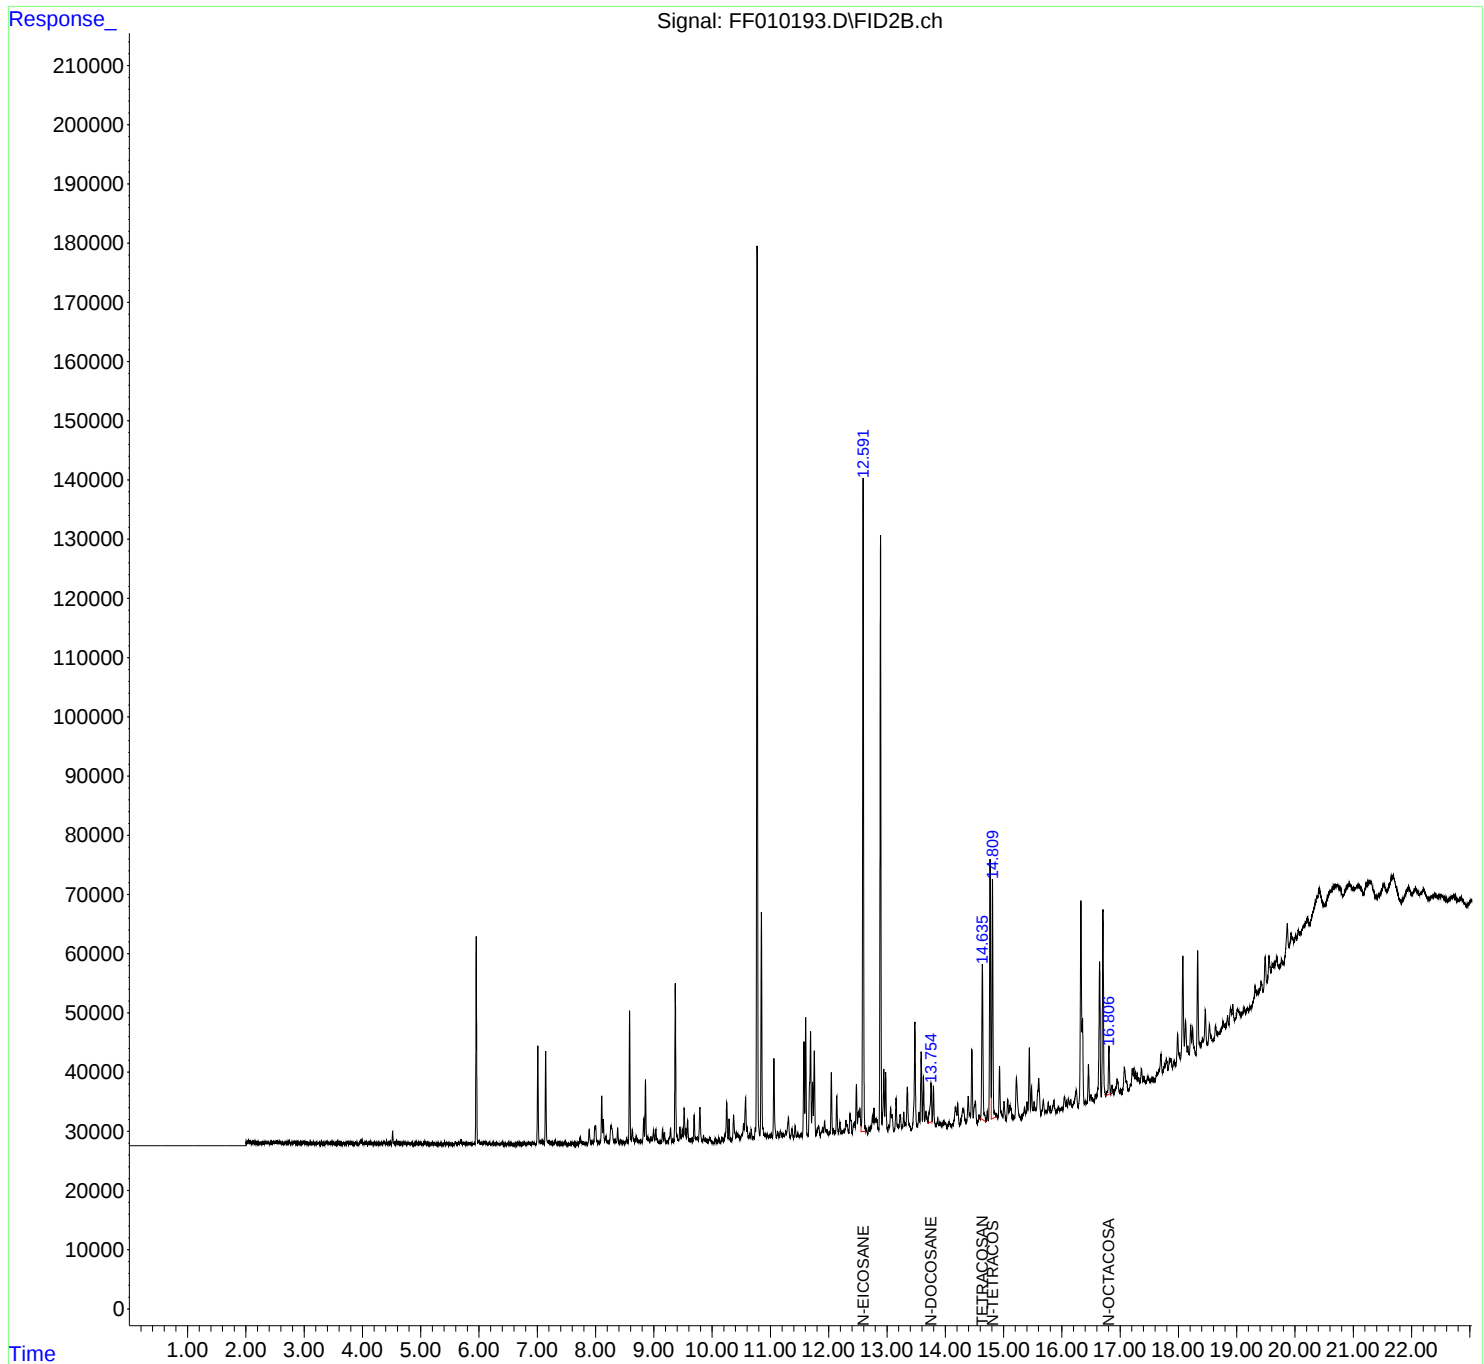


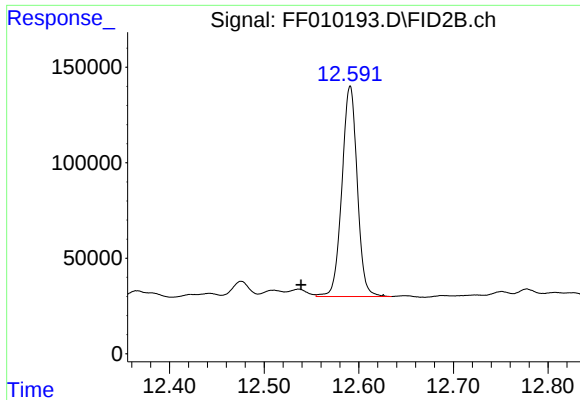

#7 N-EICOSANE


R.T.: 12.591 min
Delta R.T.: 0.052 min
Response: 1239671
Conc: 8.87 ug/ml

Instrument :
FID_F
ClientSampleId :

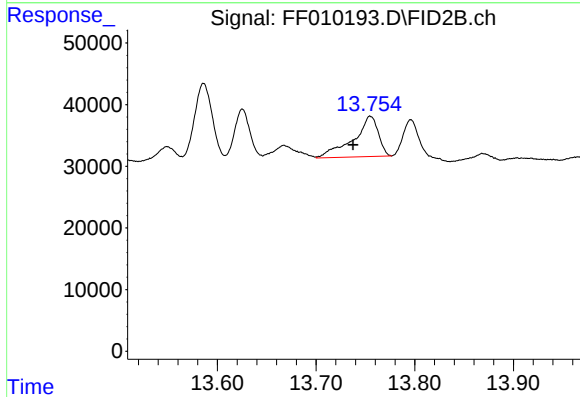


#8 N-DOCOSANE

R.T.: 13.755 min
Delta R.T.: 0.018 min
Response: 115465
Conc: 0.84 ug/ml

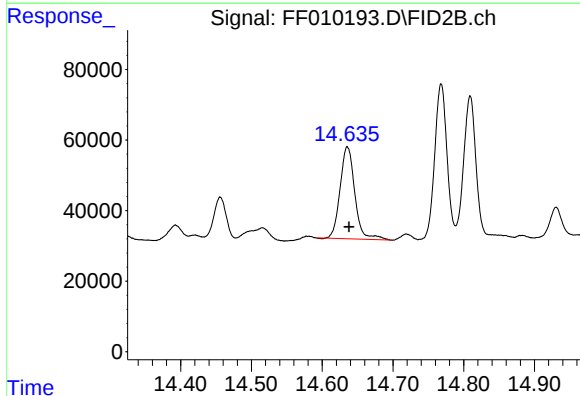


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.636 min
Delta R.T.: -0.002 min
Response: 377558
Conc: 3.09 ug/ml

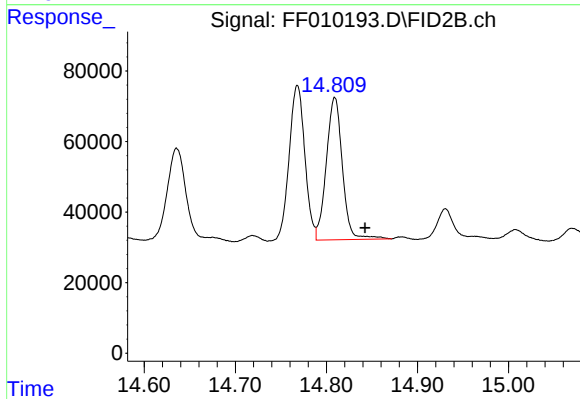

#10 N-TETRACOSANE

R.T.: 14.809 min
Delta R.T.: -0.033 min
Response: 495655
Conc: 3.62 ug/ml

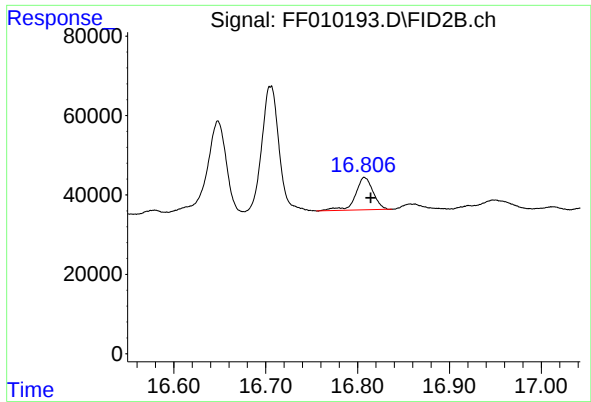

#12 N-OCTACOSANE

R.T.: 16.808 min
Delta R.T.: -0.006 min
Response: 109174
Conc: 0.83 ug/ml

Instrument :

FID_F

ClientSampleId :