

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032822\
 Data File : FF010193.D
 Signal(s) : FID2B.ch
 Acq On : 28 Mar 2022 14:17
 Operator : AJ\MA
 Sample : N1974-09 5X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 G-6-6-12-13

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/29/2022
 Supervised By :mohammad ahmed 03/30/2022

Integration File: autoint1.e
 Quant Time: Mar 29 02:17:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
 Quant Title :
 QLast Update : Sat Mar 26 09:58:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.635	367146	3.006 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032822\
Data File : FF010193.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2022 14:17
Operator : AJ\MA
Sample : N1974-09 5X
Misc :
ALS Vial : 59 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
G-6-6-12-13


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/29/2022
Supervised By :mohammad ahmed 03/30/2022

Integration File: autoint1.e
Quant Time: Mar 29 02:17:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

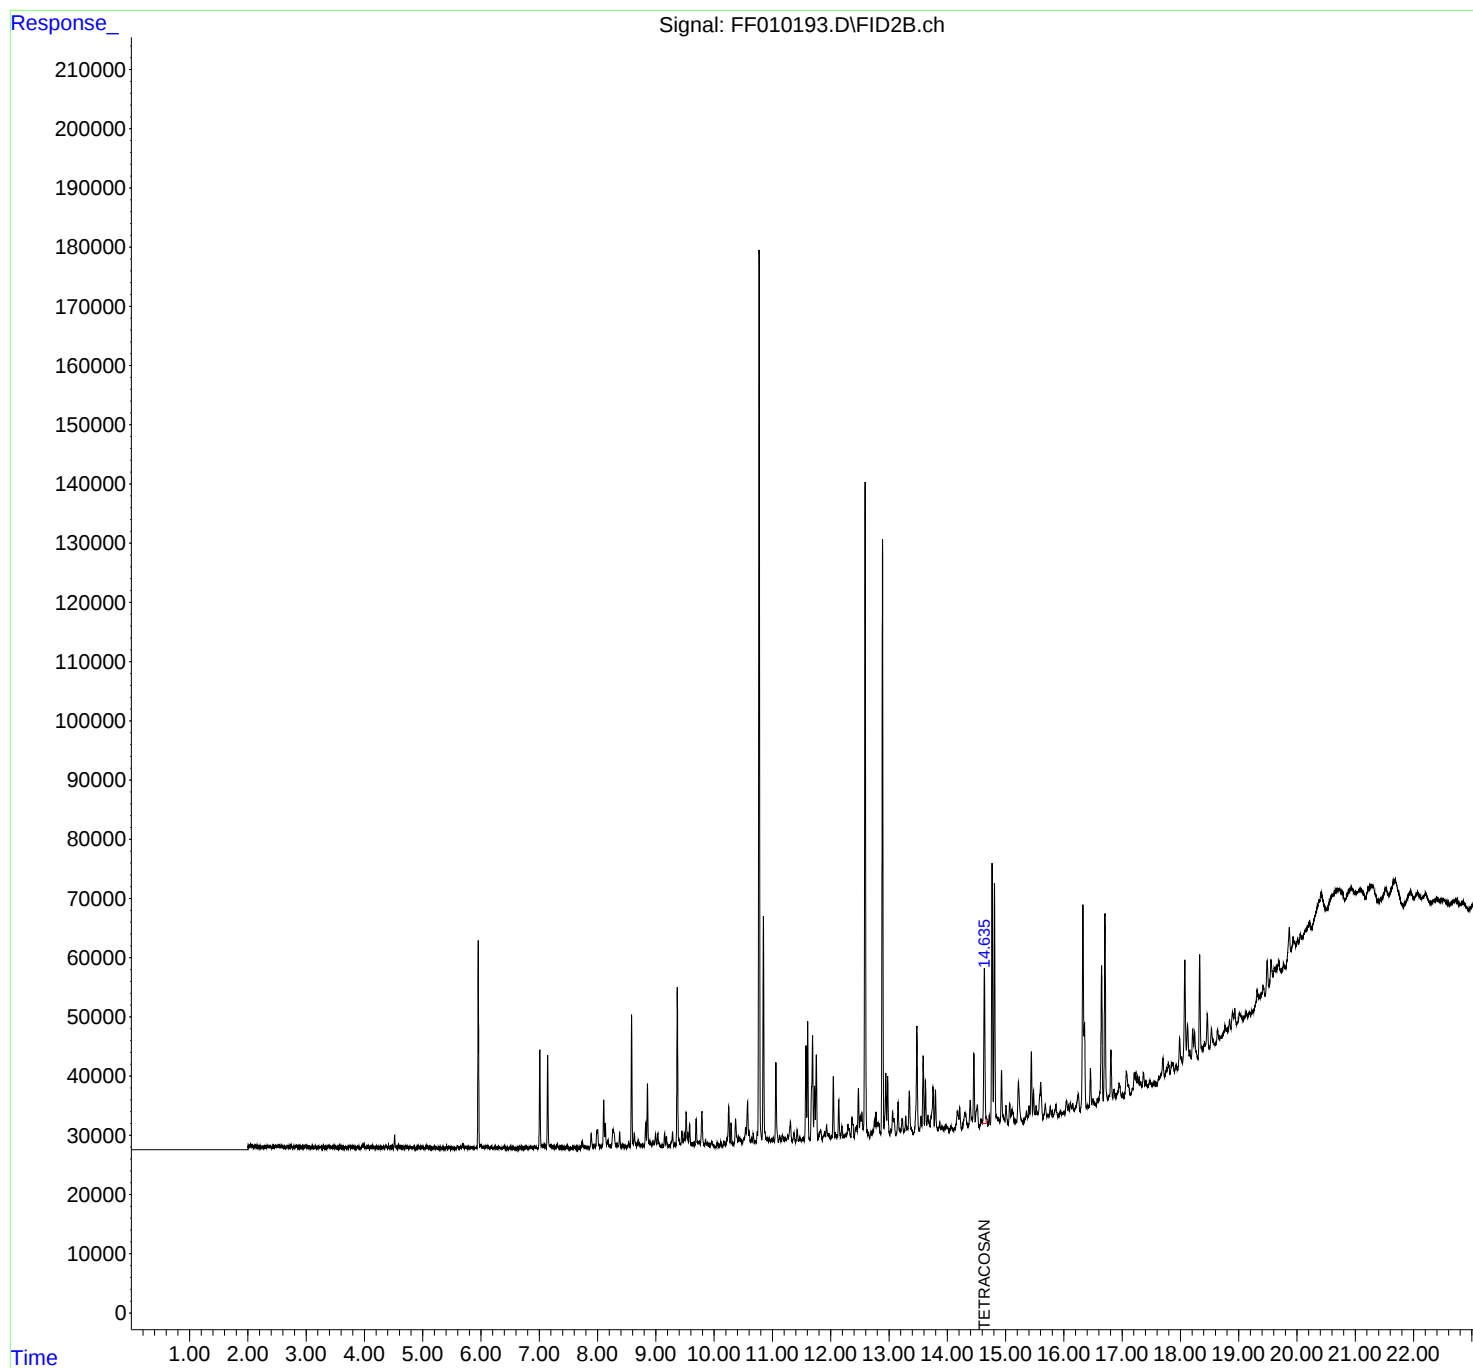

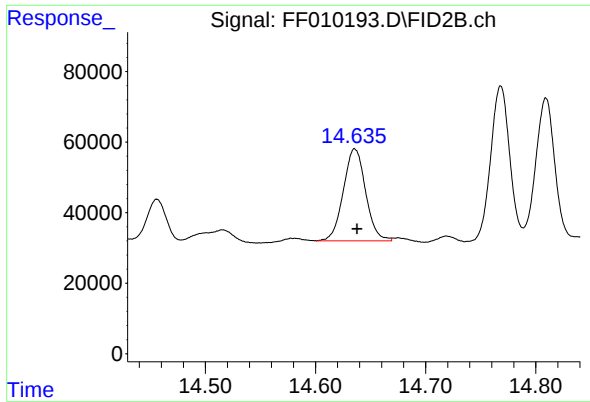

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.635 min
Delta R.T.: -0.003 min
Response: 367146
Conc: 3.01 ug/ml

Instrument :
FID_F
ClientSampleId :
G-6-6-12-13

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/29/2022
Supervised By :mohammad ahmed 03/30/2022