

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032825AL\
Data File : FF015740.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2025 09:12
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 29 01:00:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 031725.M
Quant Title : GC Extractables
QLast Update : Tue Mar 18 02:31:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.933	400485	3.071 ug/ml
19) T	n-Tetratriacontane (C34)	19.712	178539	1.529 ug/ml
20) T	n-Hexatriacontane (C36)	20.489	378876	3.817 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032825AL\
Data File : FF015740.D
Signal(s) : FID2B.ch
Acq On : 28 Mar 2025 09:12
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 29 01:00:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 031725.M
Quant Title : GC Extractables
QLast Update : Tue Mar 18 02:31:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

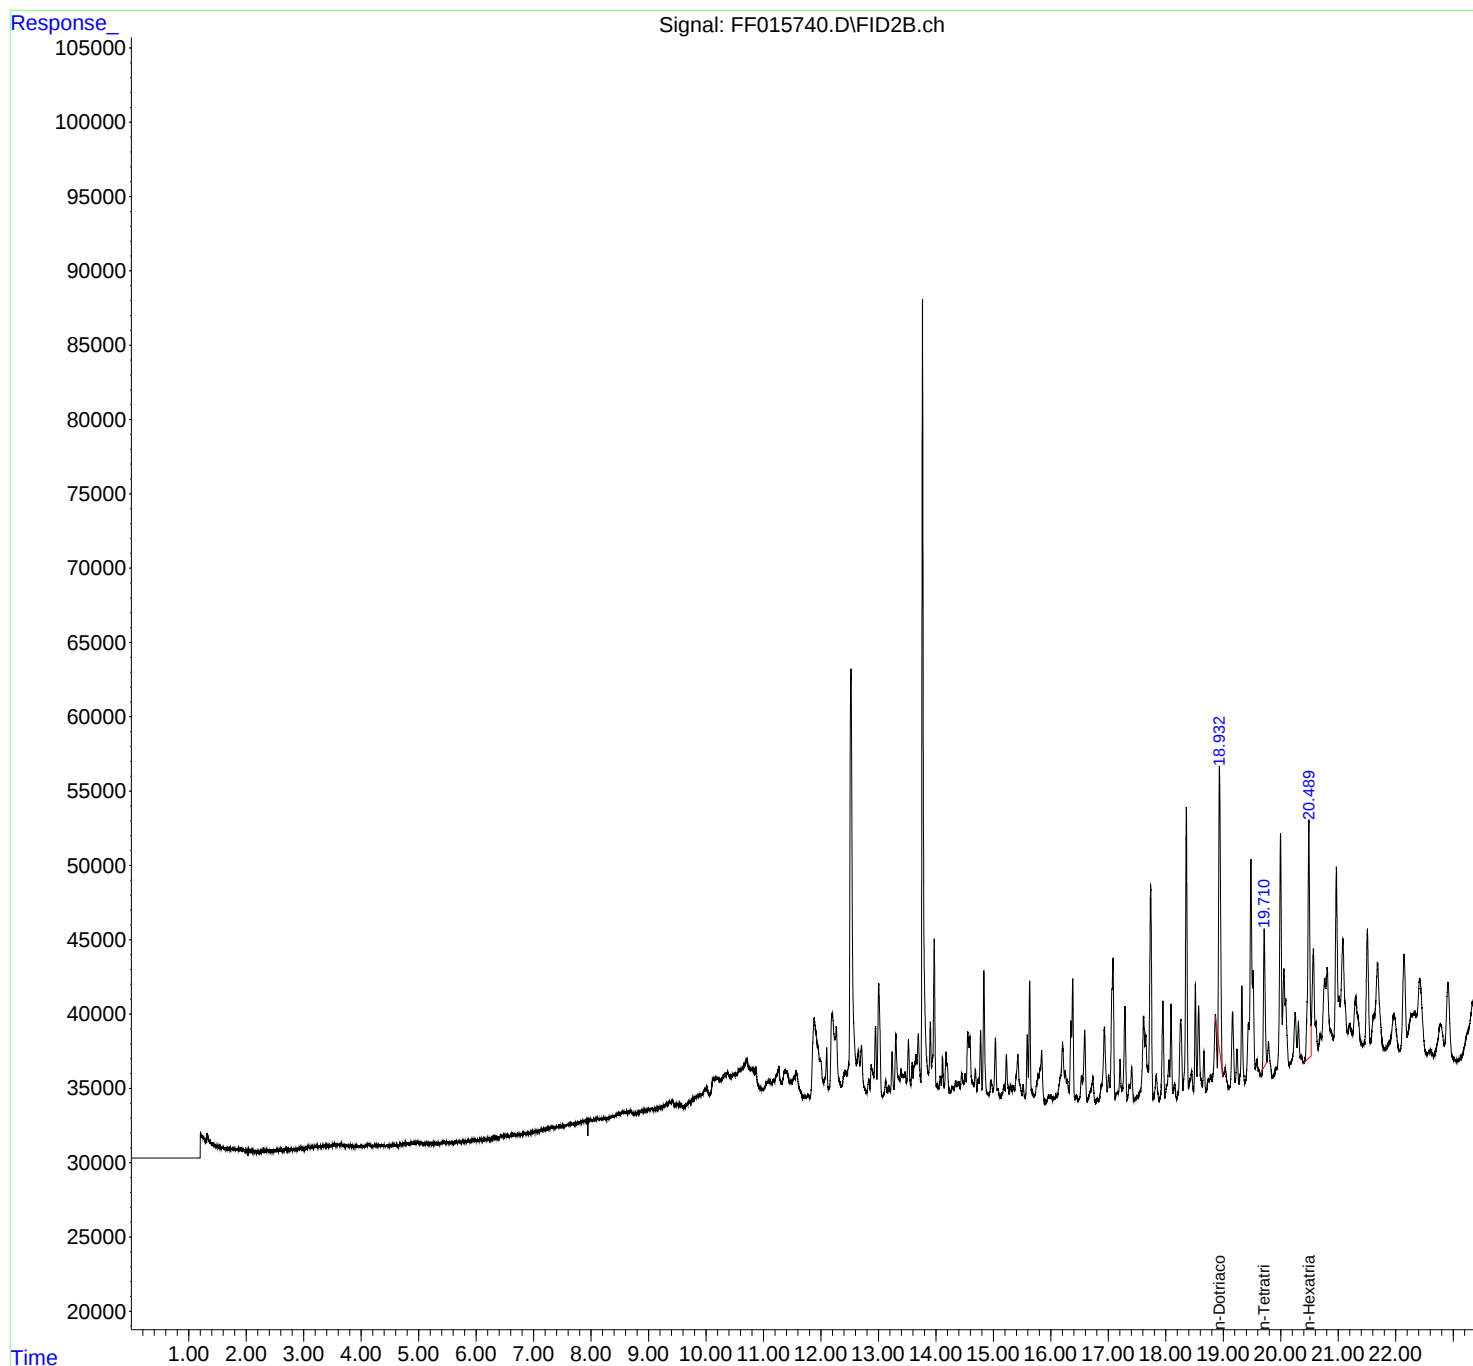


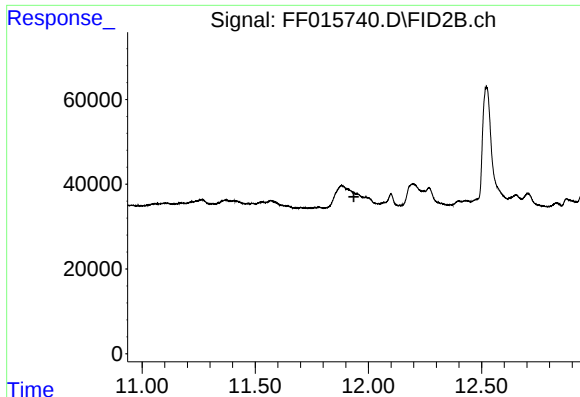

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.936 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

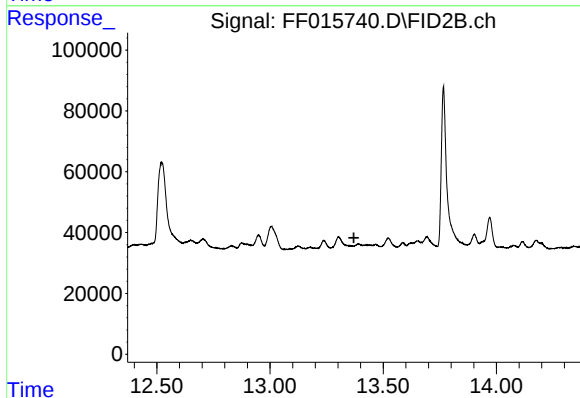


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.371 min
Response: 0
Conc: N.D.

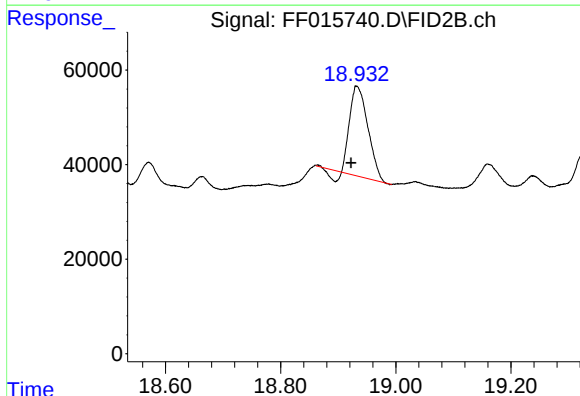


#18 n-Dotriacontane (C32)

R.T.: 18.933 min
Delta R.T.: 0.010 min
Response: 400485
Conc: 3.07 ug/ml

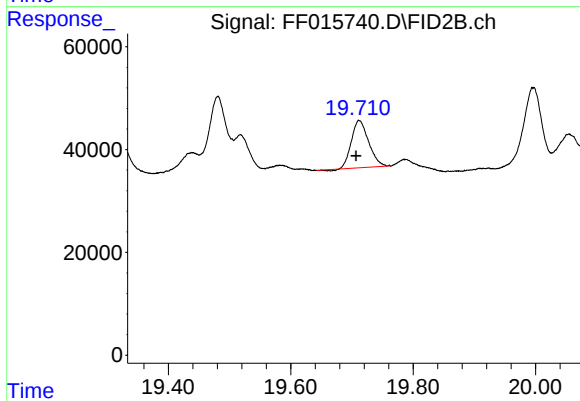

#19 n-Tetratriacontane (C34)

R.T.: 19.712 min
Delta R.T.: 0.005 min
Response: 178539
Conc: 1.53 ug/ml

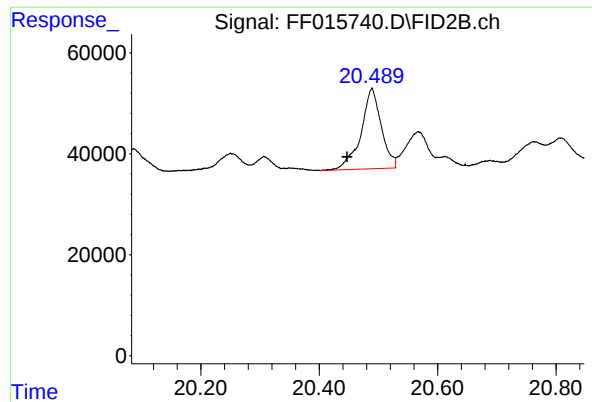

#20 n-Hexatriacontane (C36)

R.T.: 20.489 min
Delta R.T.: 0.042 min
Response: 378876
Conc: 3.82 ug/ml

Instrument :

FID_F

ClientSampleId :