

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032919\
 Data File : FF004037.D
 Signal(s) : FID2B.ch
 Acq On : 29 Mar 2019 10:49
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Mar 30 00:49:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.318	2872879	18.408 ug/ml
12) N-OCTACOSANE	16.739	2800859	18.535 ug/ml
13) N-TRIACONTANE	17.627	157029	1.067 ug/ml
14) N-DOTRIACONTANE	18.459	186426	1.311 ug/ml
15) N-TETRATRIACONTANE	19.244	132648	0.991 ug/ml
16) N-HEXATRIACONTANE	19.989	52342	0.401 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032919\
Data File : FF004037.D
Signal(s) : FID2B.ch
Acq On : 29 Mar 2019 10:49
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 30 00:49:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

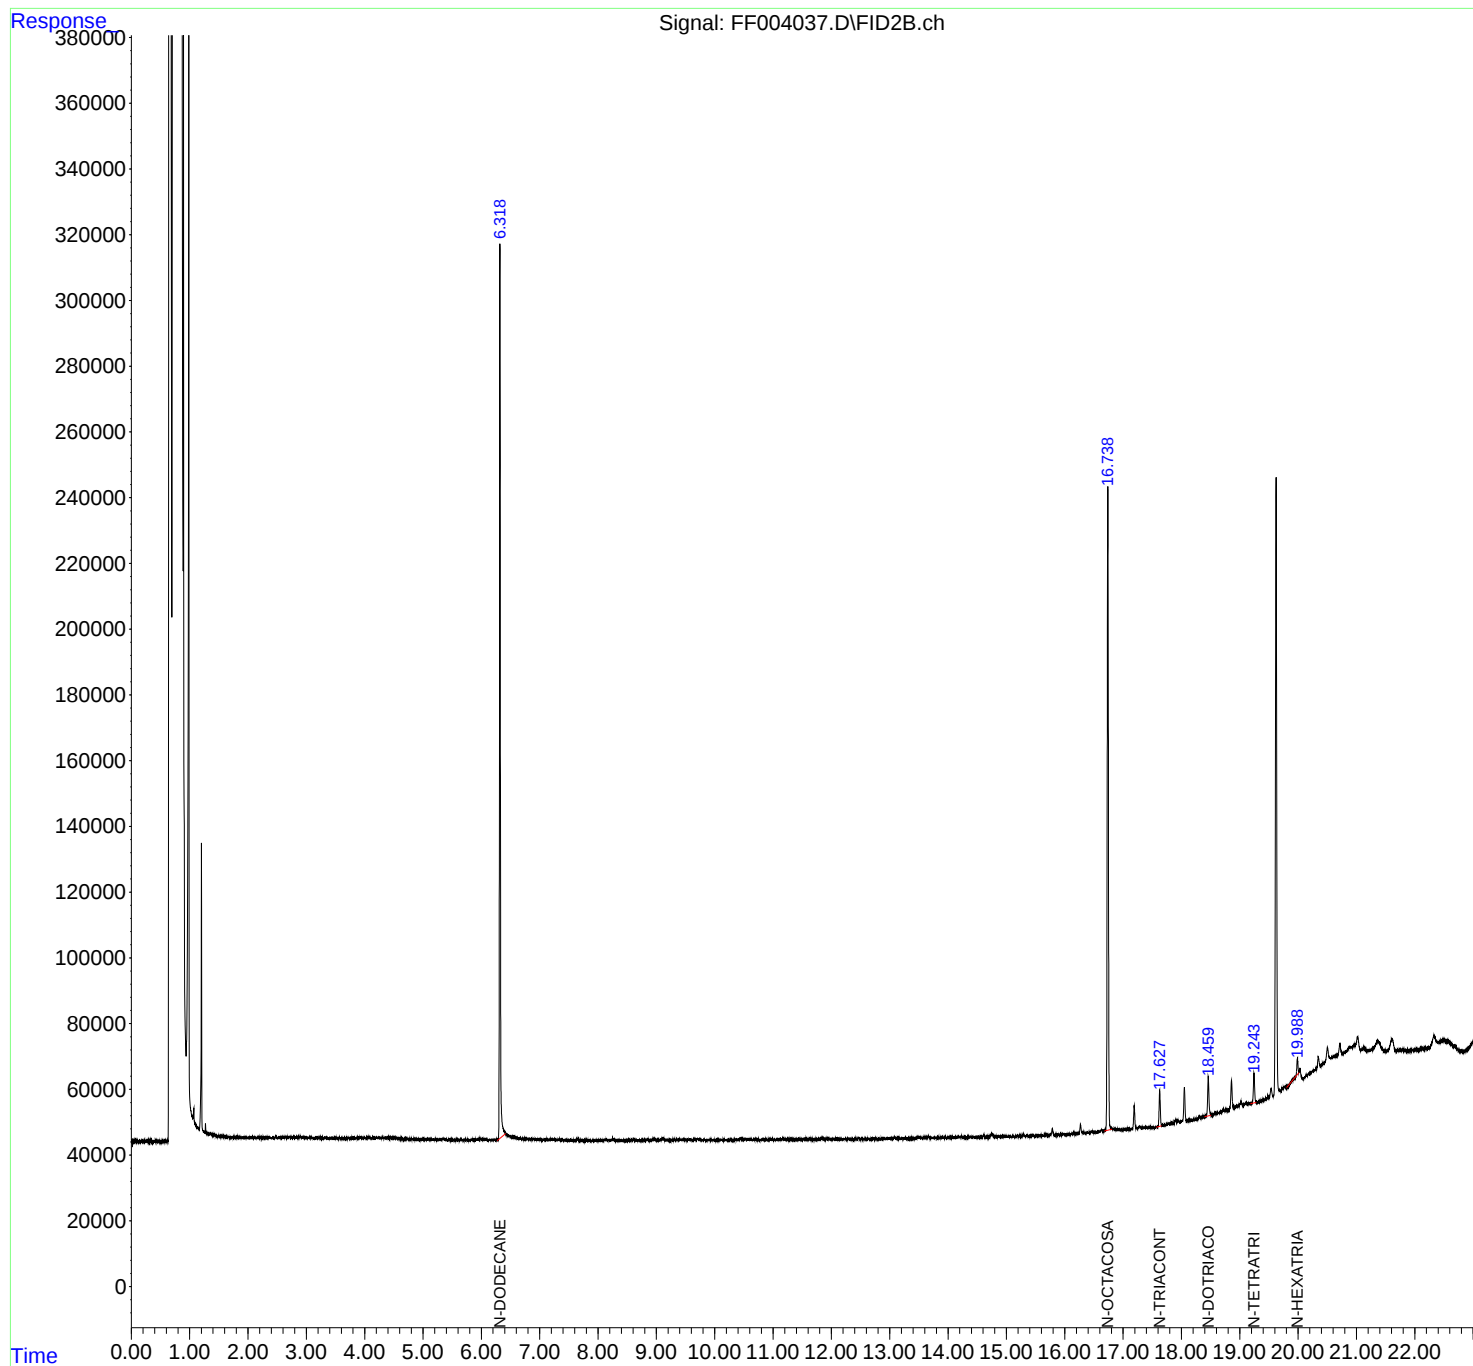


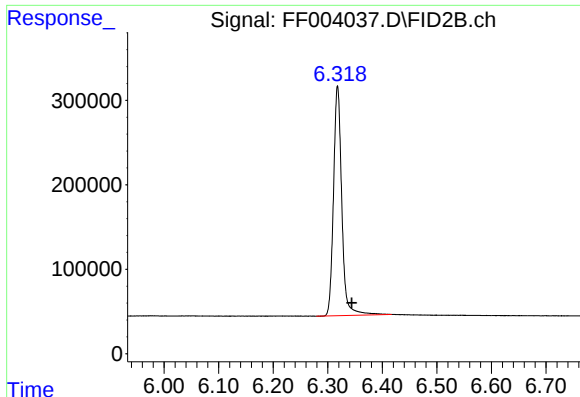

#3 N-DODECANE


R.T.: 6.318 min
Delta R.T.: -0.026 min
Response: 2872879
Conc: 18.41 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

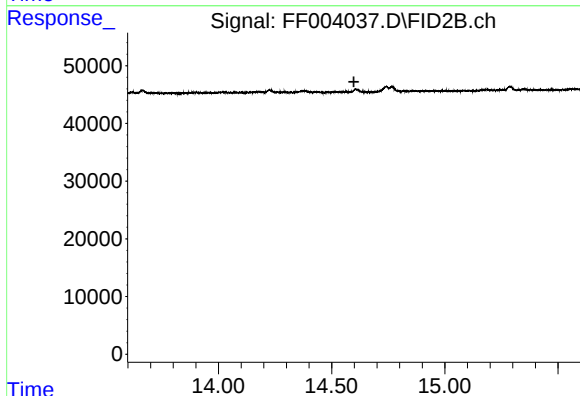


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

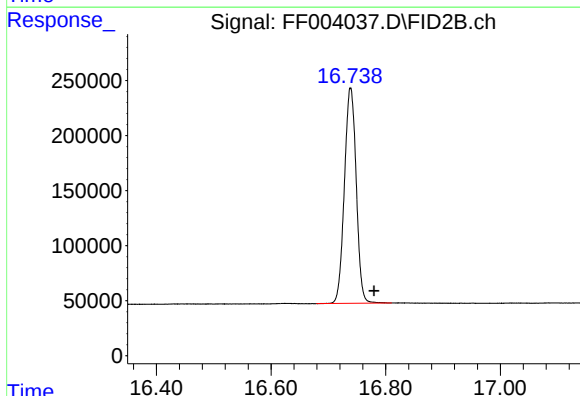


#12 N-OCTACOSANE

R.T.: 16.739 min
Delta R.T.: -0.041 min
Response: 2800859
Conc: 18.53 ug/ml

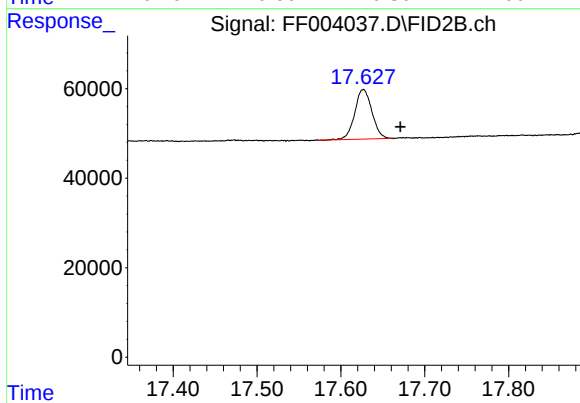

#13 N-TRIACONTANE


R.T.: 17.627 min
Delta R.T.: -0.044 min
Response: 157029
Conc: 1.07 ug/ml

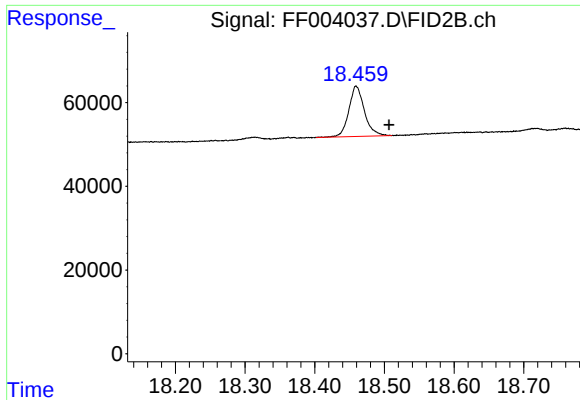

#14 N-DOTRIACONTANE


R.T.: 18.459 min
Delta R.T.: -0.047 min
Response: 186426
Conc: 1.31 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

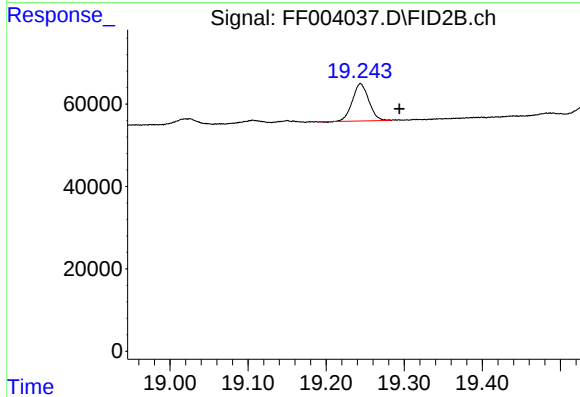

#15 N-TETRATRIACONTANE

R.T.: 19.244 min
Delta R.T.: -0.050 min
Response: 132648
Conc: 0.99 ug/ml

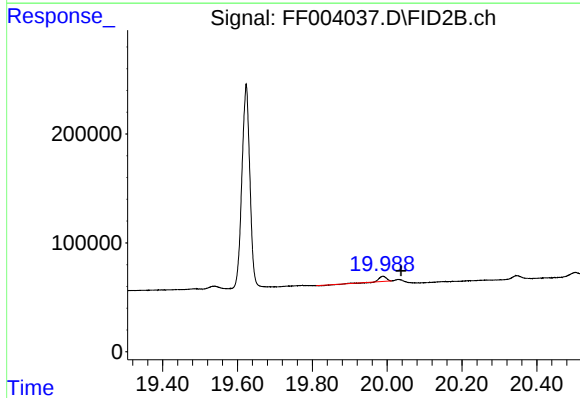

#16 N-HEXATRIACONTANE

R.T.: 19.989 min
Delta R.T.: -0.049 min
Response: 52342
Conc: 0.40 ug/ml