

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032922\
Data File : FF010199.D
Signal(s) : FID2B.ch
Acq On : 29 Mar 2022 10:27
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 30 01:55:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.382	4402028	31.838 ug/ml
12)	N-OCTACOSANE	16.812	3788173	28.797 ug/ml
13)	N-TRIACONTANE	17.698	118952	0.928 ug/ml
14)	N-DOTRIACONTANE	18.531	150826	1.207 ug/ml
15)	N-TETRATRIACONTANE	19.314	131397	1.216 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032922\
Data File : FF010199.D
Signal(s) : FID2B.ch
Acq On : 29 Mar 2022 10:27
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 30 01:55:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

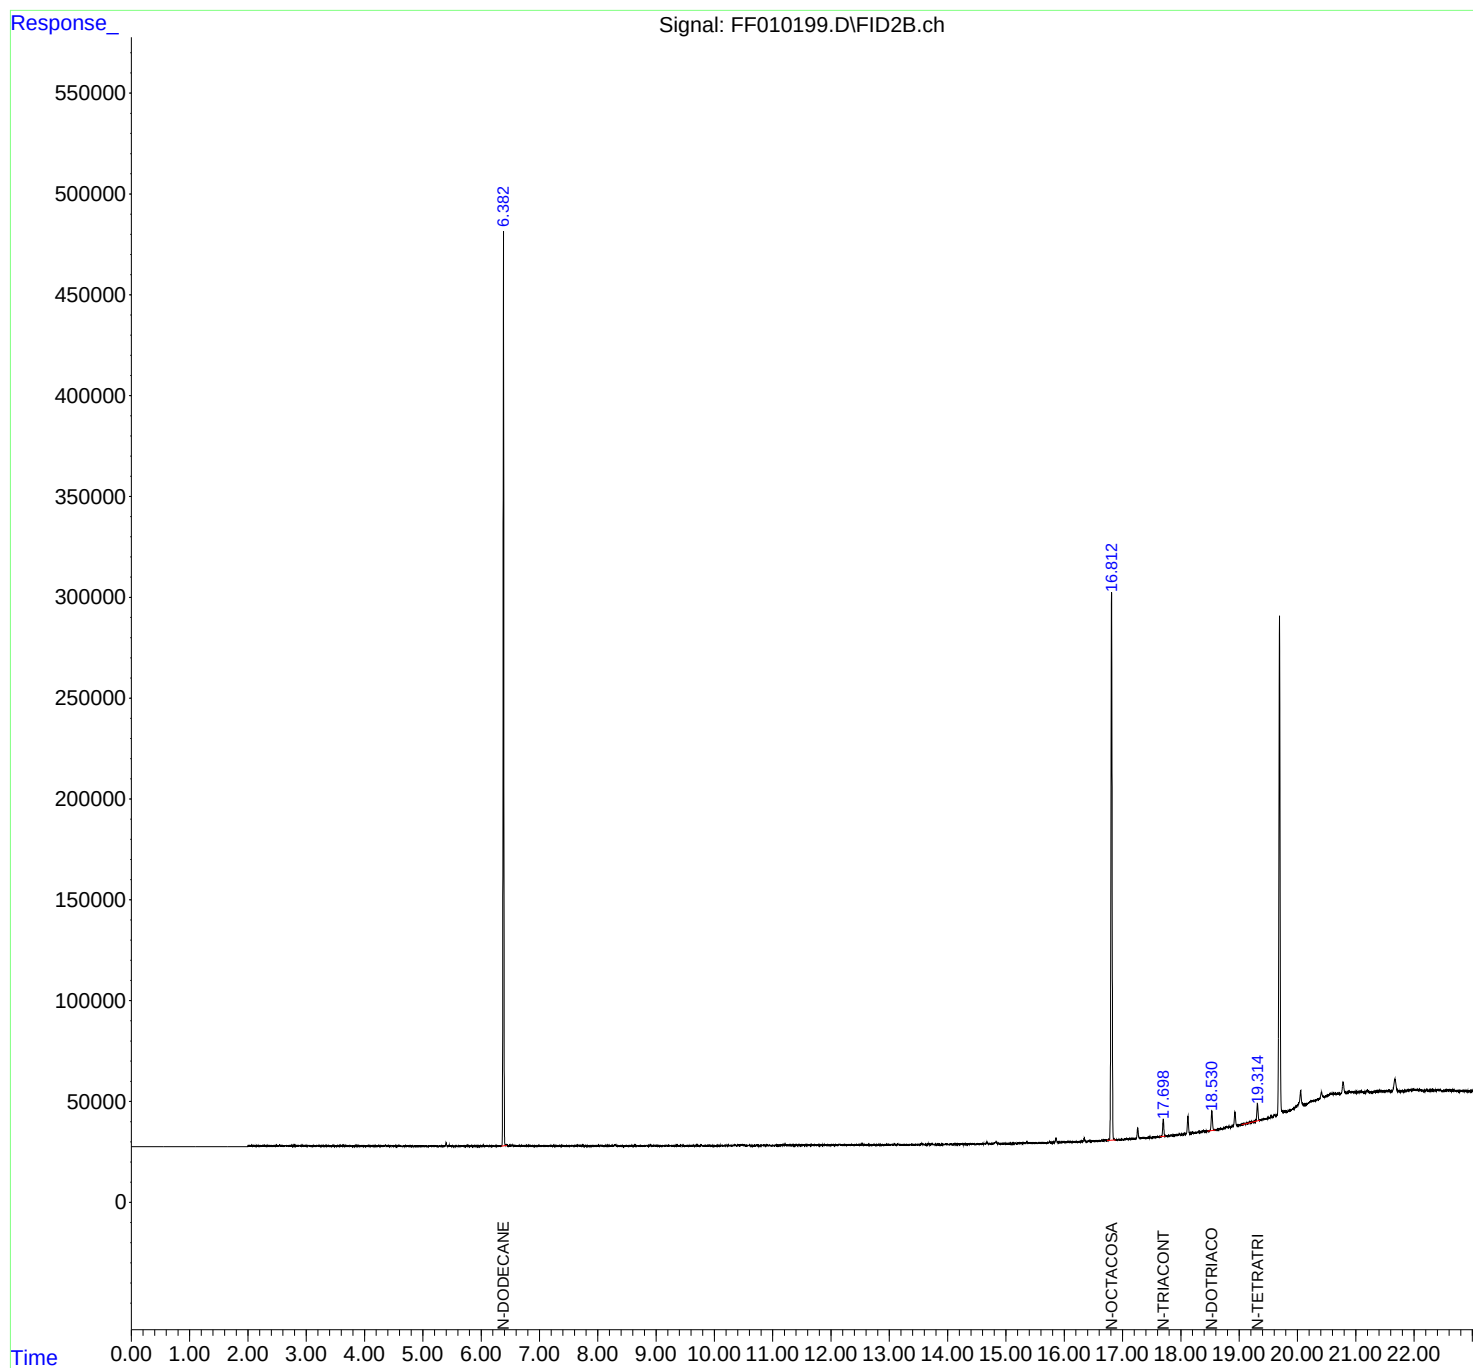

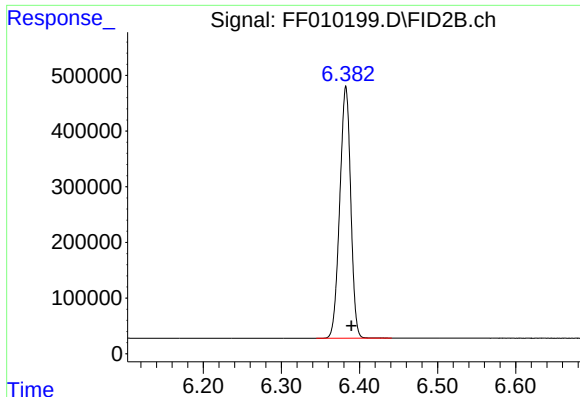


#3 N-DODECANE

R.T.: 6.382 min
Delta R.T.: -0.007 min
Response: 4402028
Conc: 31.84 ug/ml

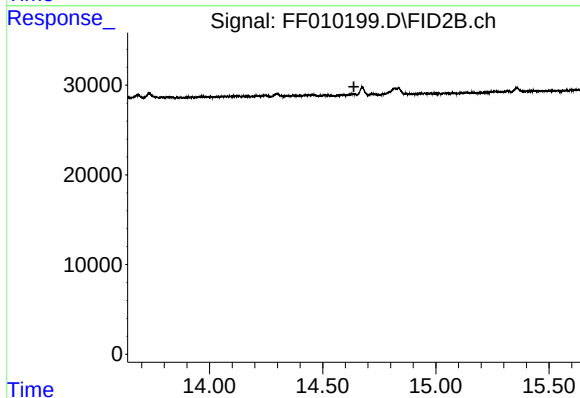


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.638 min
Response: 0
Conc: N.D.

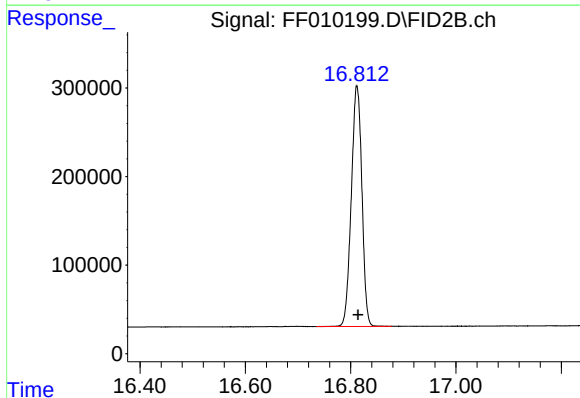


#12 N-OCTACOSANE

R.T.: 16.812 min
Delta R.T.: -0.002 min
Response: 3788173
Conc: 28.80 ug/ml

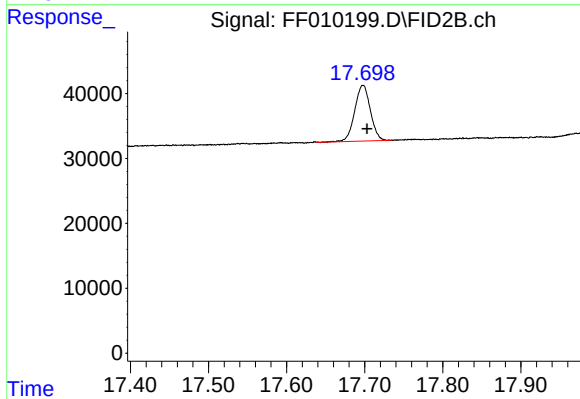


#13 N-TRIACONTANE

R.T.: 17.698 min
Delta R.T.: -0.005 min
Response: 118952
Conc: 0.93 ug/ml

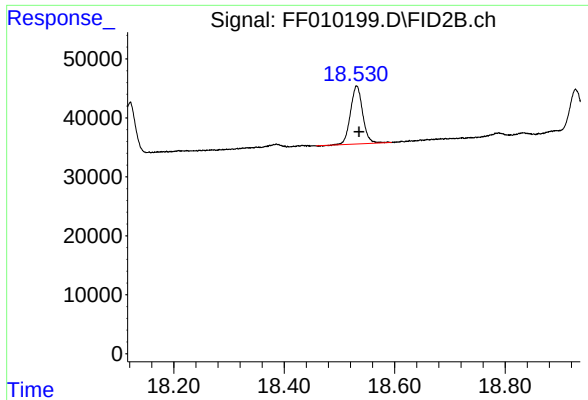

#14 N-DOTRIACONTANE

R.T.: 18.531 min
Delta R.T.: -0.004 min
Response: 150826
Conc: 1.21 ug/ml

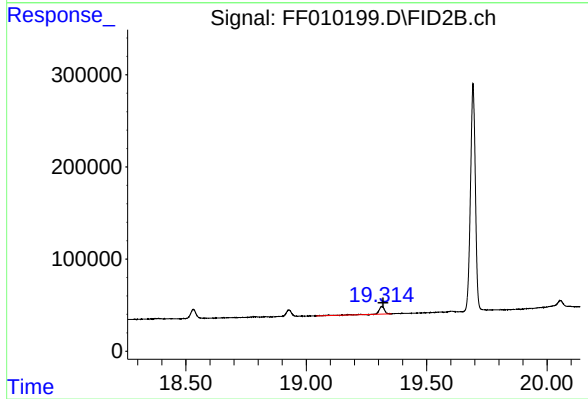

#15 N-TETRATRIACONTANE

R.T.: 19.314 min
Delta R.T.: -0.005 min
Response: 131397
Conc: 1.22 ug/ml