

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032924\
Data File : FF014093.D
Signal(s) : FID2B.ch
Acq On : 29 Mar 2024 16:15
Operator : YP\AJ
Sample : P1908-19
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Mar 29 23:05:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031524.M
Quant Title :
QLast Update : Fri Mar 15 13:52:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.948	2224119	18.559 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032924\
Data File : FF014093.D
Signal(s) : FID2B.ch
Acq On : 29 Mar 2024 16:15
Operator : YP\AJ
Sample : P1908-19
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Mar 29 23:05:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031524.M
Quant Title :
QLast Update : Fri Mar 15 13:52:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

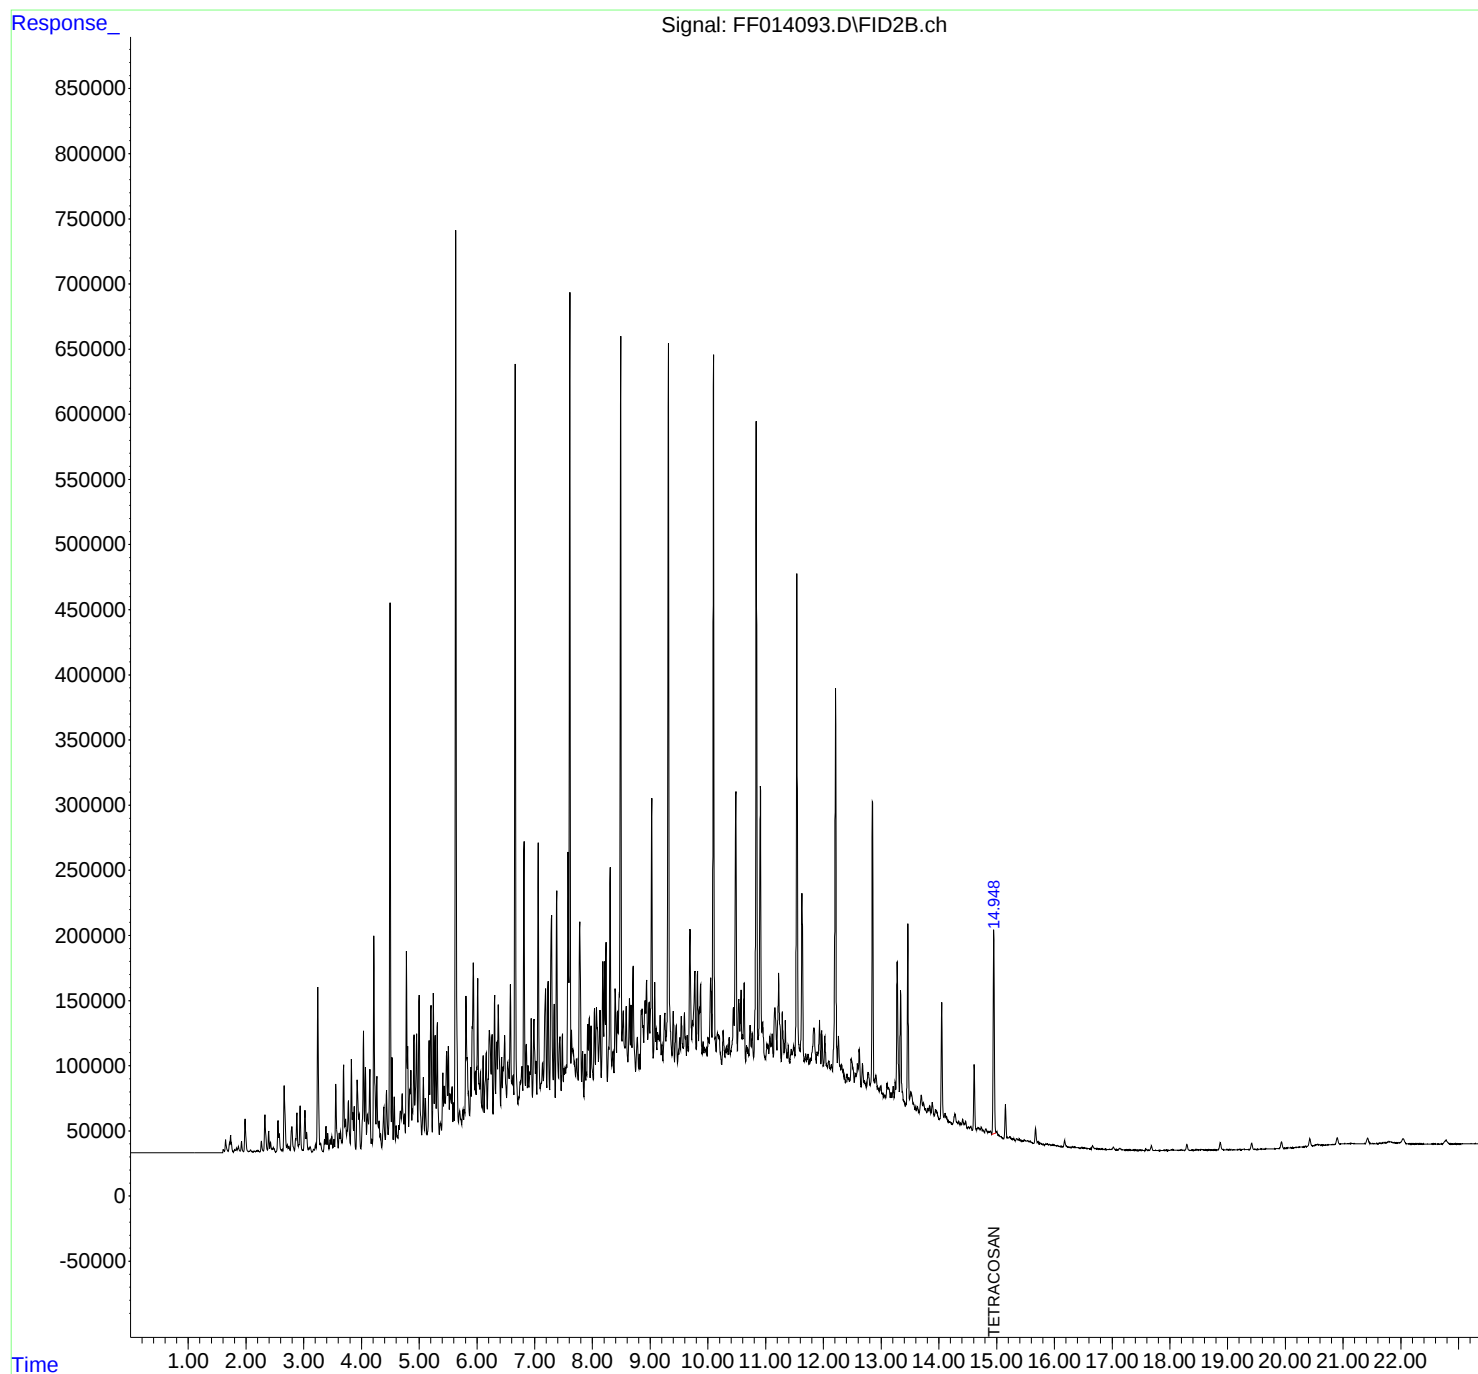

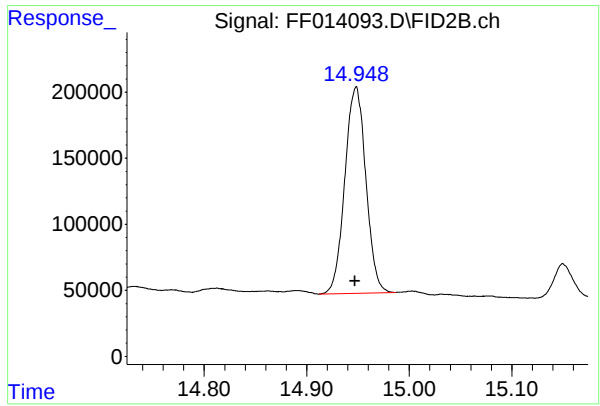

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.948 min
Delta R.T.: 0.001 min
Response: 2224119
Conc: 18.56 ug/ml

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP