

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF033023\
 Data File : FF012369.D
 Signal(s) : FID2B.ch
 Acq On : 30 Mar 2023 10:10
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 30 17:25:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
7) N-EICOSANE	12.871f	52024	0.391 ug/ml
8) N-DOCOSANE	14.109	115145	0.906 ug/ml
10) N-TETRACOSANE	15.196	465147	3.730 ug/ml
11) N-HEXACOSANE	16.237	60478	0.505 ug/ml
12) N-OCTACOSANE	17.186	49337	0.429 ug/ml
13) N-TRIACONTANE	18.072	73390	0.667 ug/ml
14) N-DOTRIACONTANE	18.910	143217	1.380 ug/ml
16) N-HEXATRIACONTANE	20.463	76820	0.877 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF033023\
Data File : FF012369.D
Signal(s) : FID2B.ch
Acq On : 30 Mar 2023 10:10
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 30 17:25:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

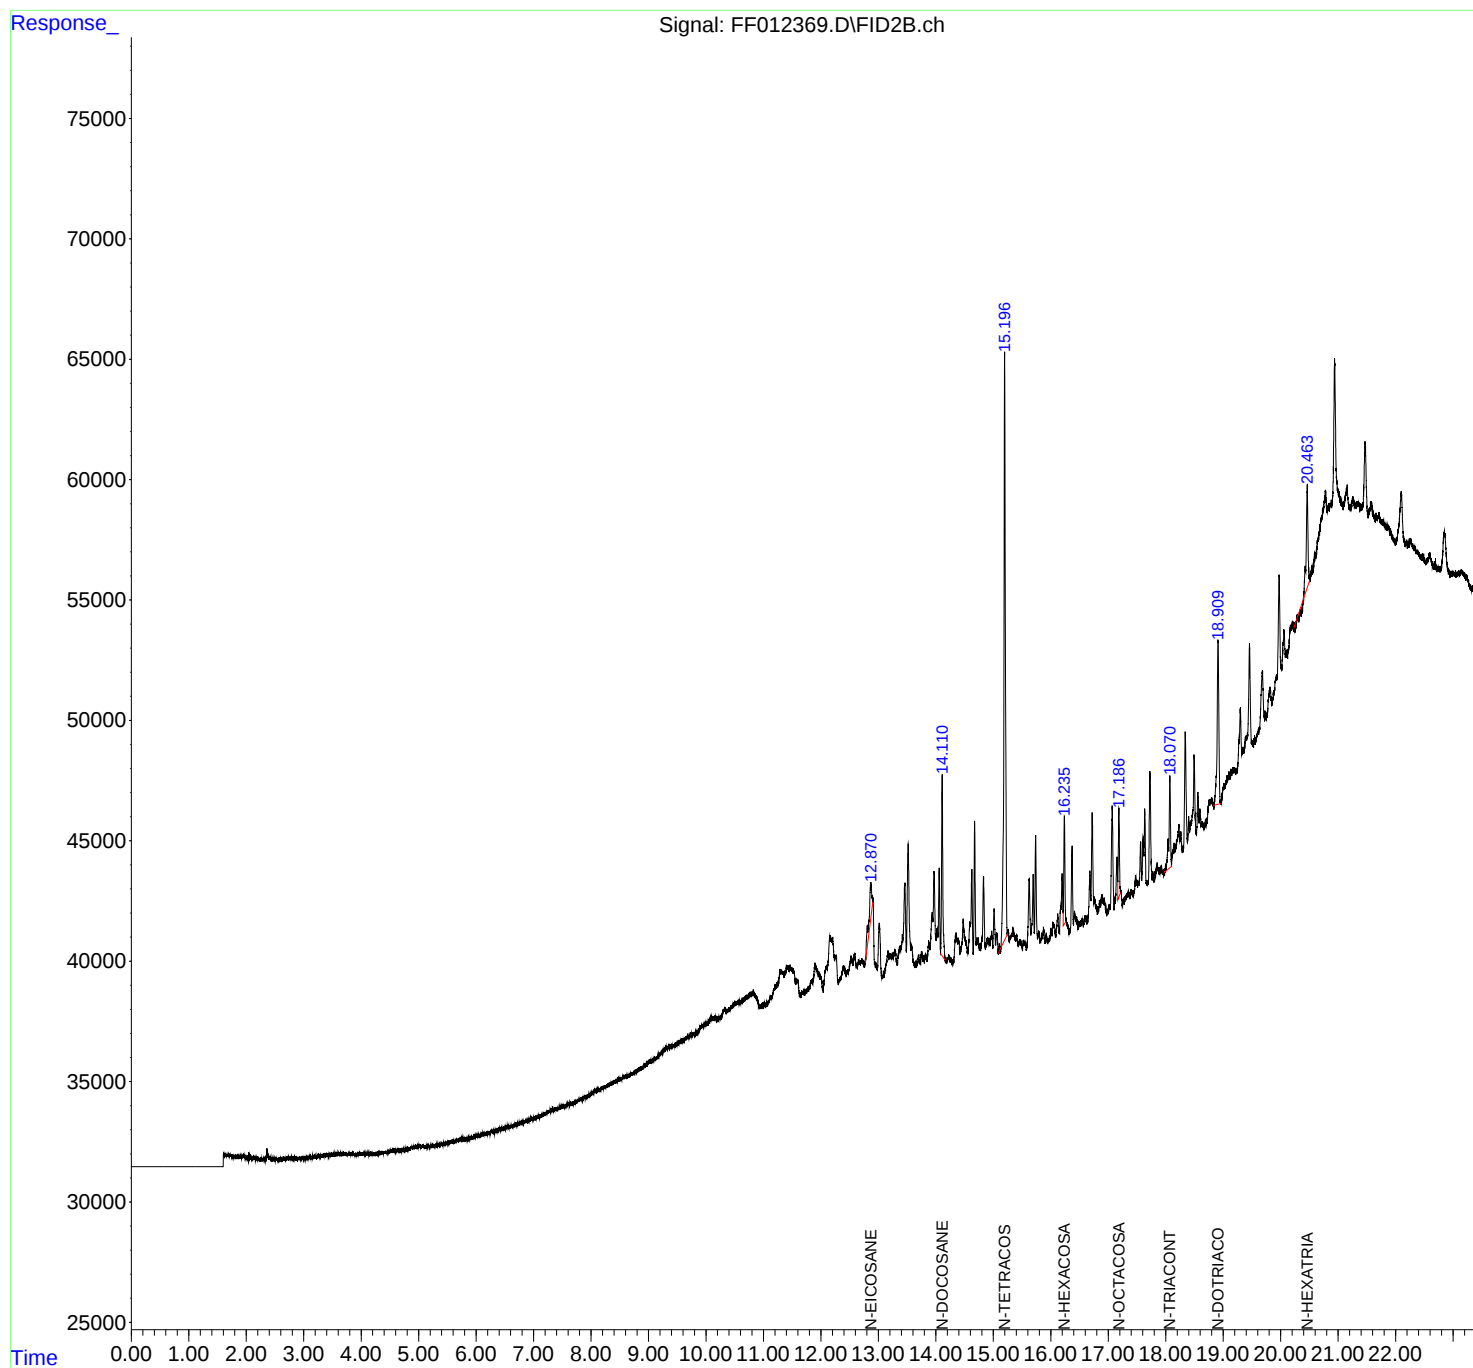


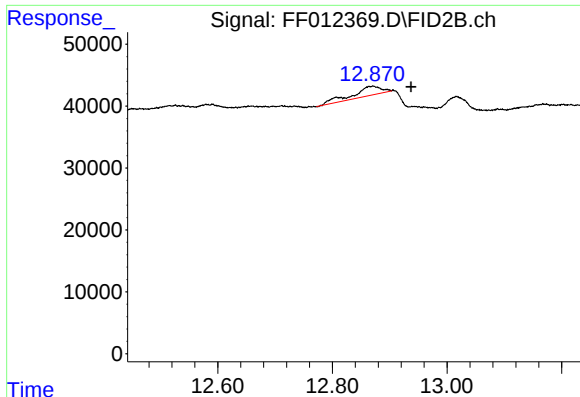

#7 N-EICOSANE


R.T.: 12.871 min
Delta R.T.: -0.066 min
Response: 52024
Conc: 0.39 ug/ml

Instrument :
FID_F
ClientSampleId :

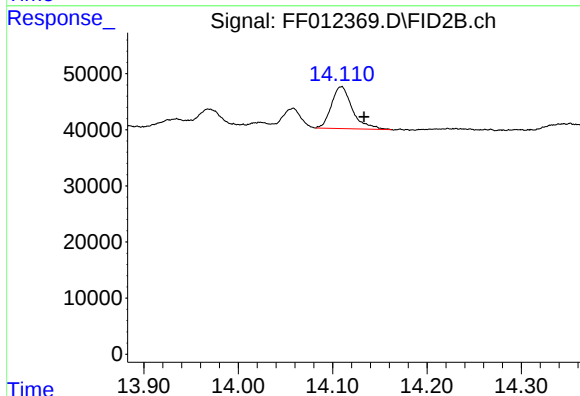


#8 N-DOCOSANE

R.T.: 14.109 min
Delta R.T.: -0.024 min
Response: 115145
Conc: 0.91 ug/ml

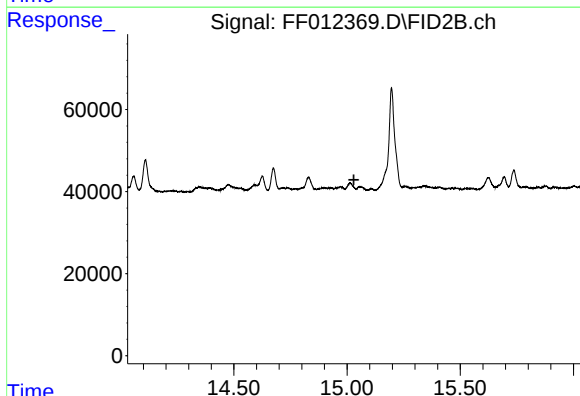


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.030 min
Response: 0
Conc: N.D.

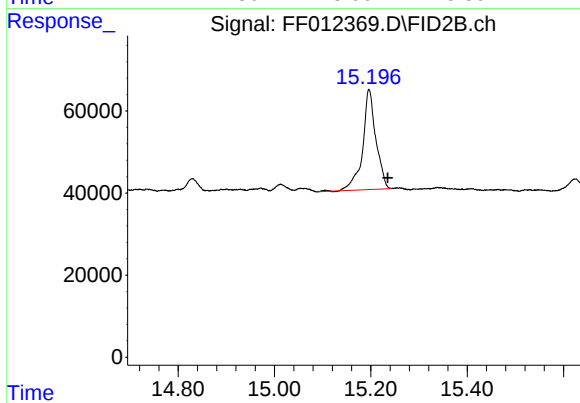

#10 N-TETRACOSANE


R.T.: 15.196 min
Delta R.T.: -0.039 min
Response: 465147
Conc: 3.73 ug/ml

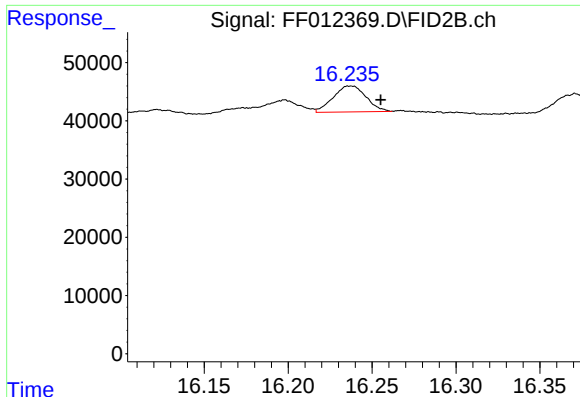

#11 N-HEXACOSANE


R.T.: 16.237 min
Delta R.T.: -0.018 min
Response: 60478
Conc: 0.51 ug/ml

Instrument :
FID_F
ClientSampleId :

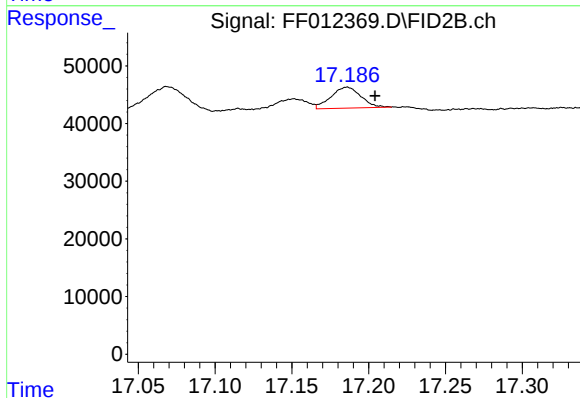


#12 N-OCTACOSANE

R.T.: 17.186 min
Delta R.T.: -0.018 min
Response: 49337
Conc: 0.43 ug/ml

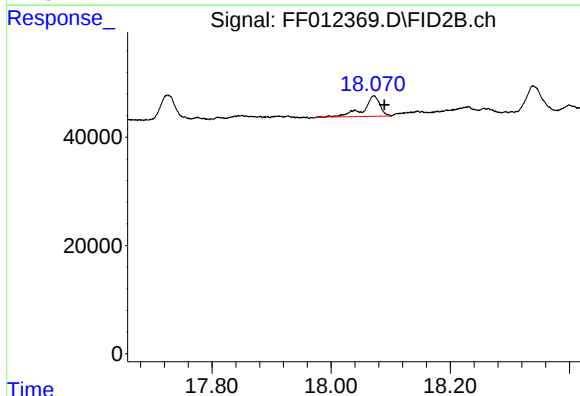


#13 N-TRIACONTANE

R.T.: 18.072 min
Delta R.T.: -0.017 min
Response: 73390
Conc: 0.67 ug/ml

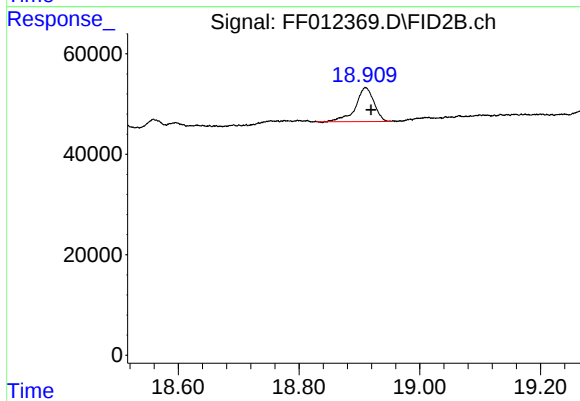

#14 N-DOTRIACONTANE

R.T.: 18.910 min
Delta R.T.: -0.009 min
Response: 143217
Conc: 1.38 ug/ml

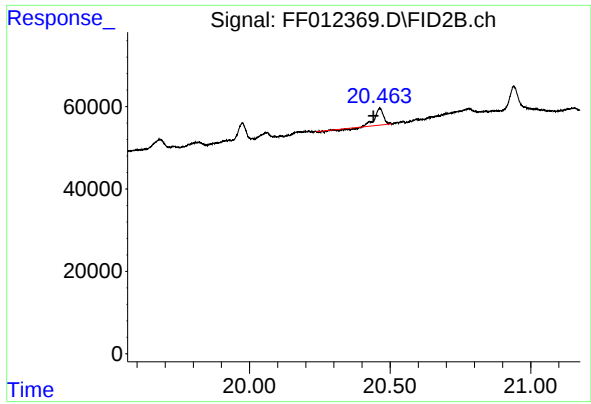

#16 N-HEXATRIACONTANE

R.T.: 20.463 min
Delta R.T.: 0.024 min
Response: 76820
Conc: 0.88 ug/ml

Instrument :

FID_F

ClientSampleId :