

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF033023\  
 Data File : FF012370.D  
 Signal(s) : FID2B.ch  
 Acq On : 30 Mar 2023 10:39  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Mar 30 17:25:50 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF031623.M  
 Quant Title :  
 QLast Update : Wed Mar 15 18:07:23 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.018 | 2394245  | 21.394 ug/ml |
| Target Compounds              |        |          |              |
| 13) N-TRIACONTANE             | 18.076 | 64833    | 0.589 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.907 | 92101    | 0.887 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.688 | 68074    | 0.720 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.428 | 45104    | 0.515 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF033023\  
Data File : FF012370.D  
Signal(s) : FID2B.ch  
Acq On : 30 Mar 2023 10:39  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Mar 30 17:25:50 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF031623.M  
Quant Title :  
QLast Update : Wed Mar 15 18:07:23 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

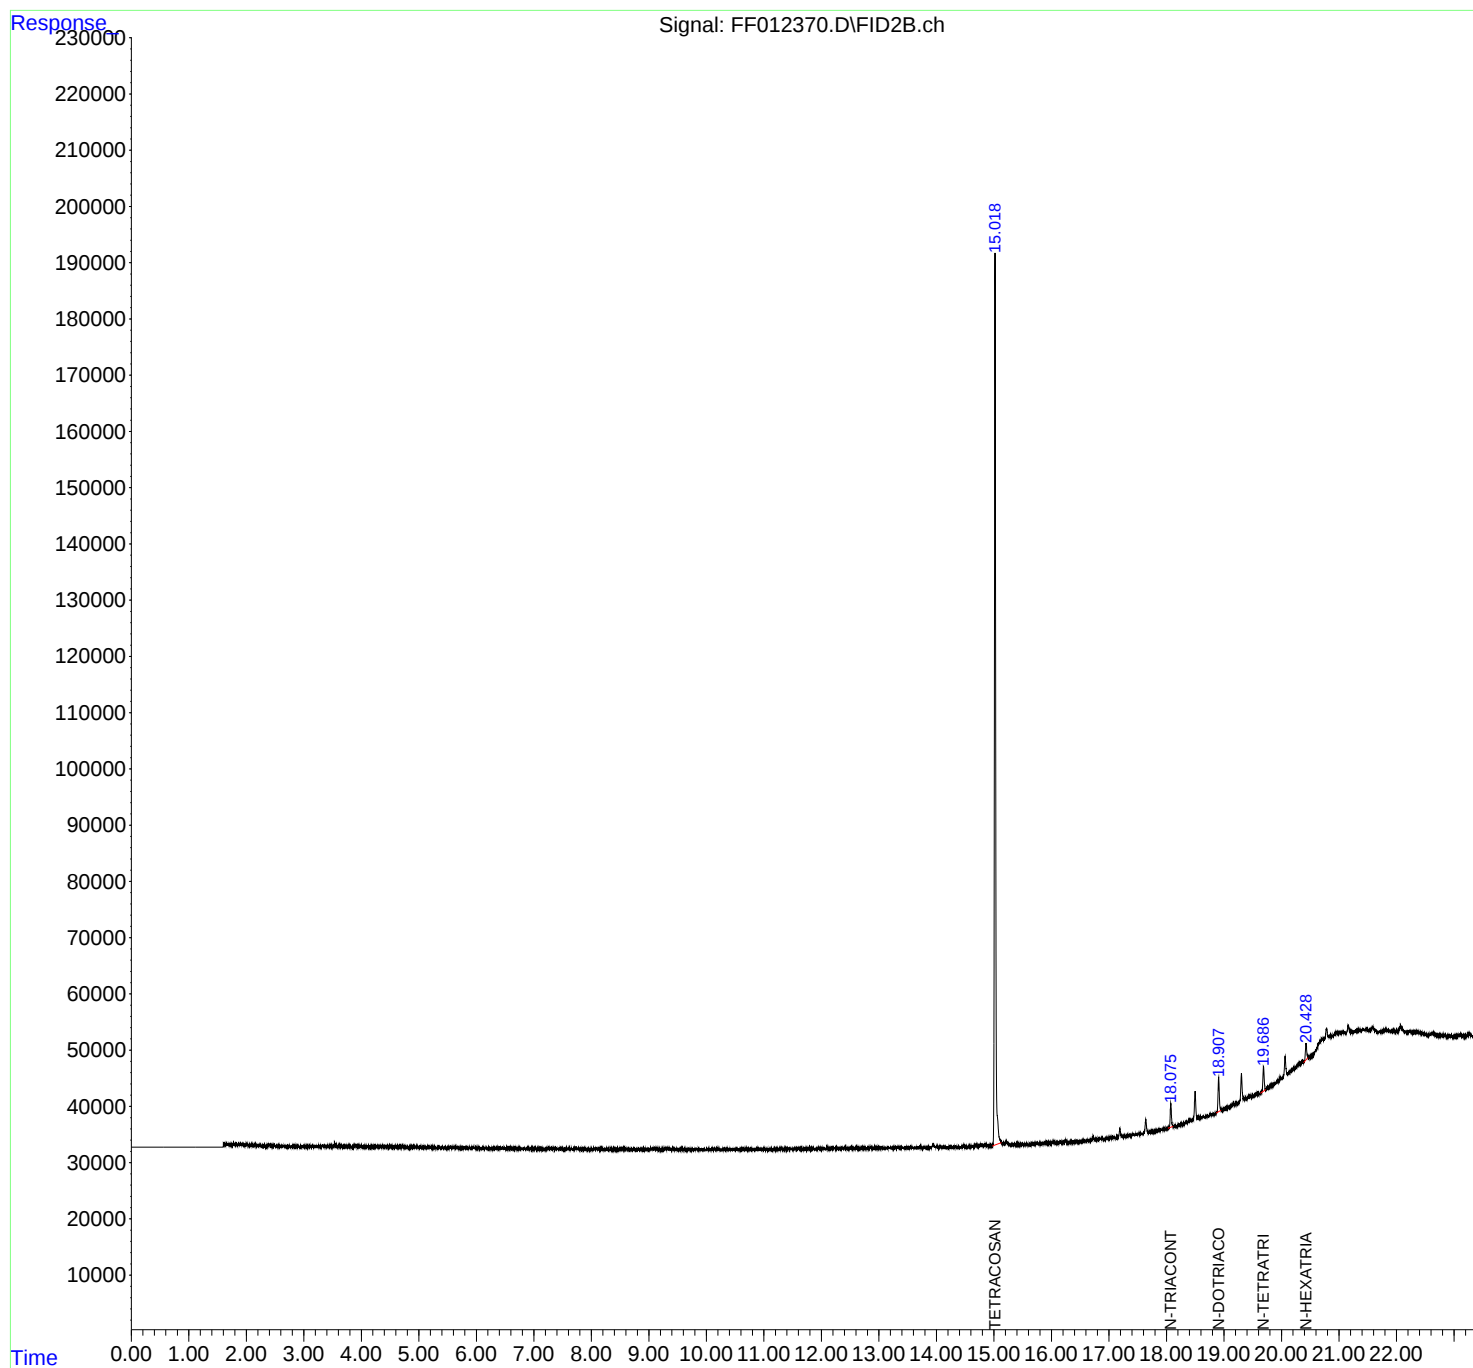


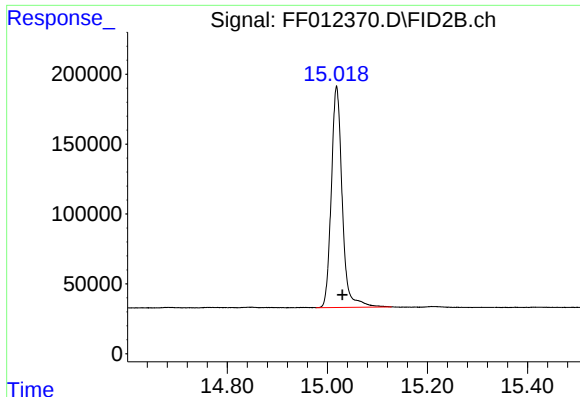

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.018 min  
Delta R.T.: -0.012 min  
Response: 2394245  
Conc: 21.39 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

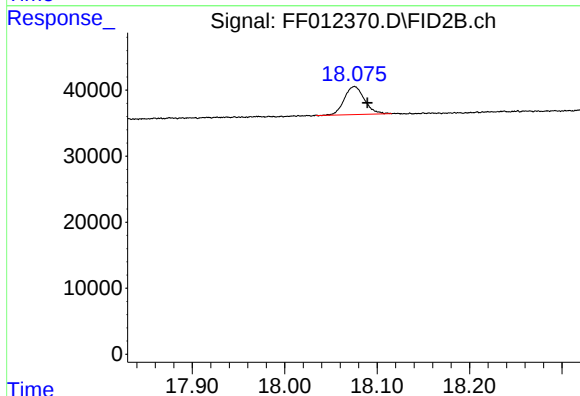


#13 N-TRIACONTANE

R.T.: 18.076 min  
Delta R.T.: -0.014 min  
Response: 64833  
Conc: 0.59 ug/ml

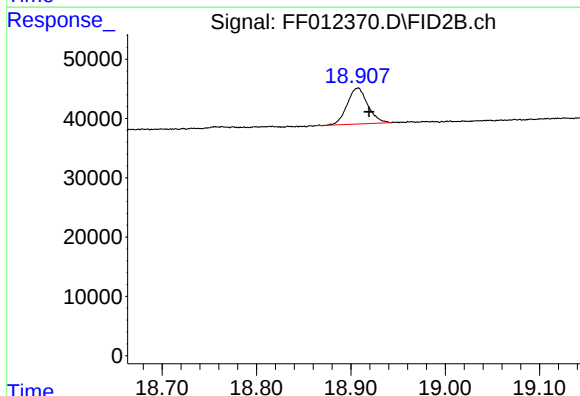


#14 N-DOTRIACONTANE

R.T.: 18.907 min  
Delta R.T.: -0.012 min  
Response: 92101  
Conc: 0.89 ug/ml

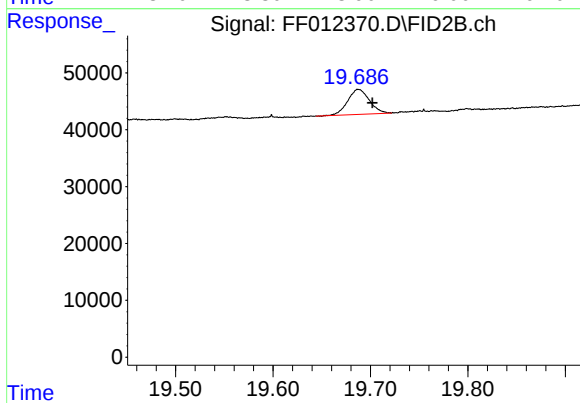

#15 N-TETRATRIACONTANE

R.T.: 19.688 min  
Delta R.T.: -0.014 min  
Response: 68074  
Conc: 0.72 ug/ml

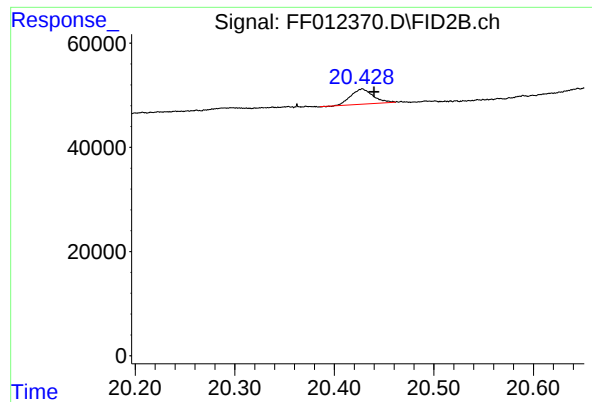

#16 N-HEXATRIACONTANE

R.T.: 20.428 min  
Delta R.T.: -0.012 min  
Response: 45104  
Conc: 0.51 ug/ml

Instrument :

FID\_F

ClientSampleId :