

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF033023\
 Data File : FF012372.D
 Signal(s) : FID2B.ch
 Acq On : 30 Mar 2023 11:37
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 30 17:26:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.749	2458879	19.835 ug/ml
12) N-OCTACOSANE	17.191	2457710	21.366 ug/ml
13) N-TRIACONTANE	18.075	108240	0.984 ug/ml
14) N-DOTRIACONTANE	18.906	155690	1.500 ug/ml
15) N-TETRATRIACONTANE	19.687	125667	1.328 ug/ml
16) N-HEXATRIACONTANE	20.428	94325	1.077 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF033023\
Data File : FF012372.D
Signal(s) : FID2B.ch
Acq On : 30 Mar 2023 11:37
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 30 17:26:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

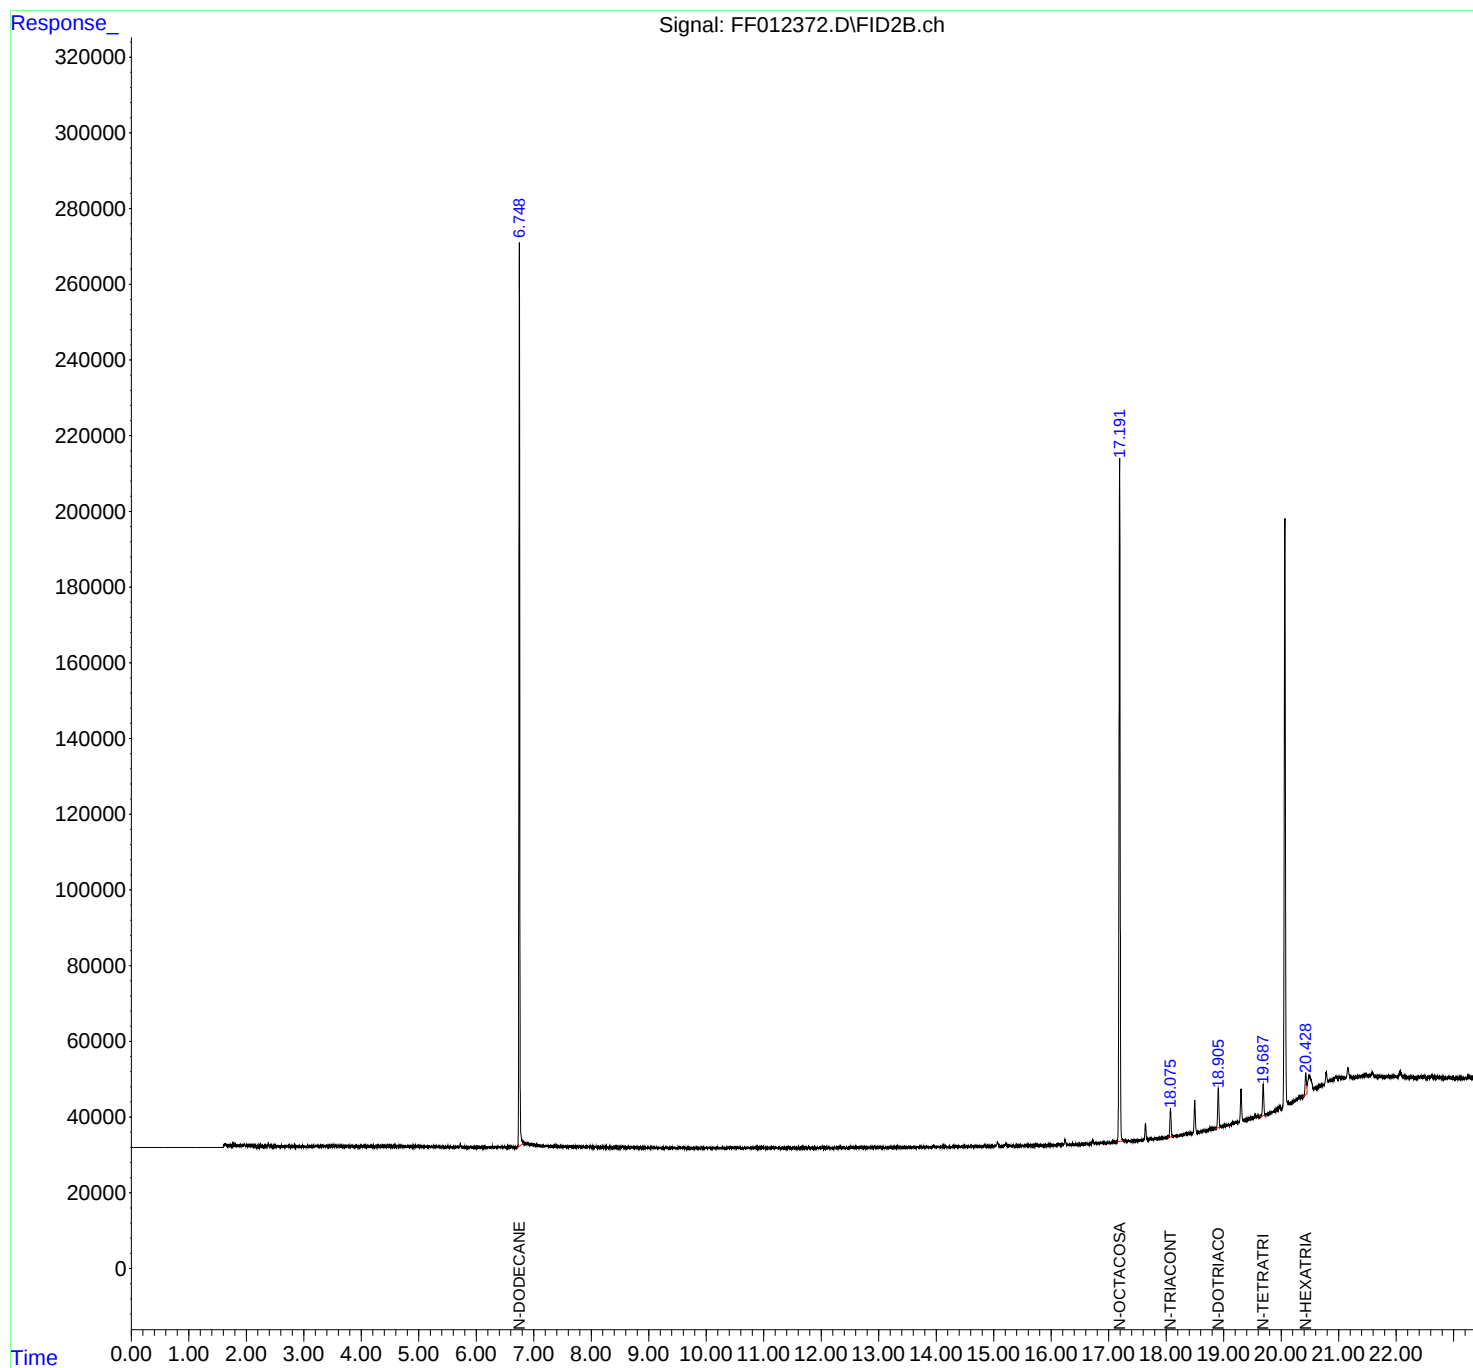


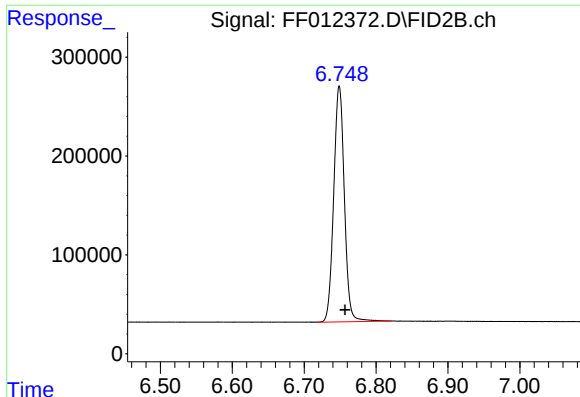

#3 N-DODECANE


R.T.: 6.749 min
Delta R.T.: -0.008 min
Response: 2458879
Conc: 19.83 ug/ml

Instrument :
FID_F
ClientSampleId :

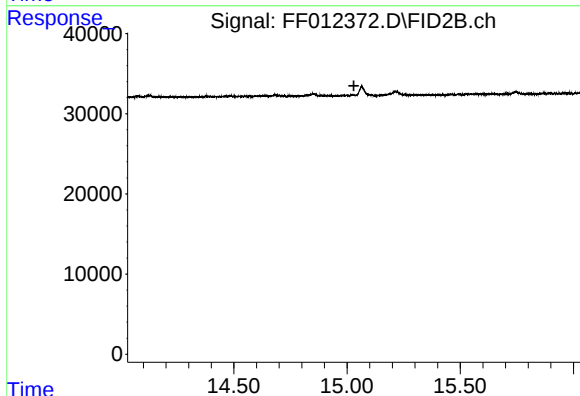


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.030 min
Response: 0
Conc: N.D.

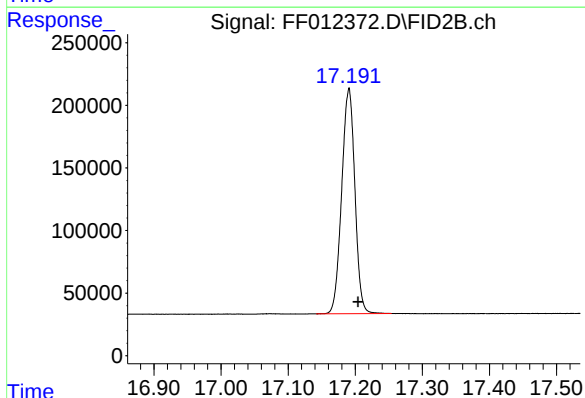


#12 N-OCTACOSANE

R.T.: 17.191 min
Delta R.T.: -0.013 min
Response: 2457710
Conc: 21.37 ug/ml

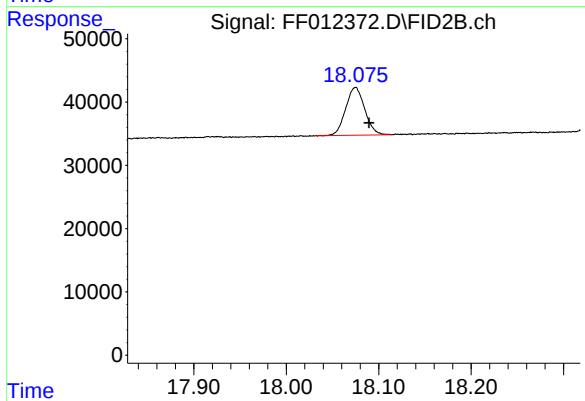

#13 N-TRIACONTANE


R.T.: 18.075 min
Delta R.T.: -0.014 min
Response: 108240
Conc: 0.98 ug/ml

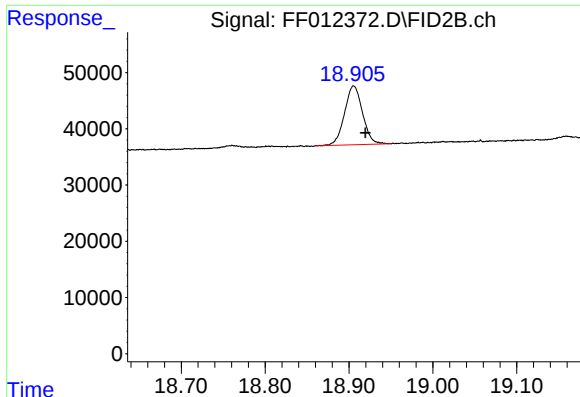

#14 N-DOTRIACONTANE


R.T.: 18.906 min
Delta R.T.: -0.014 min
Response: 155690
Conc: 1.50 ug/ml

Instrument :
FID_F
ClientSampleId :

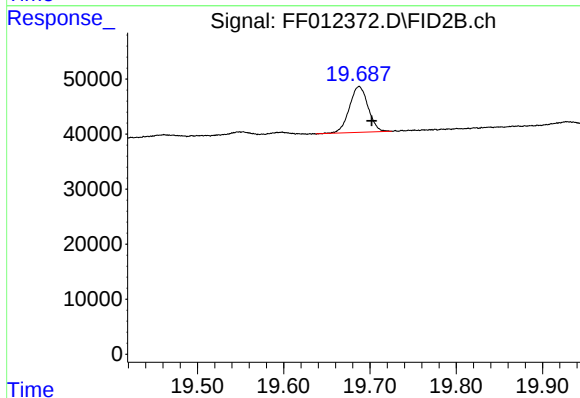

#15 N-TETRATRIACONTANE

R.T.: 19.687 min
Delta R.T.: -0.015 min
Response: 125667
Conc: 1.33 ug/ml

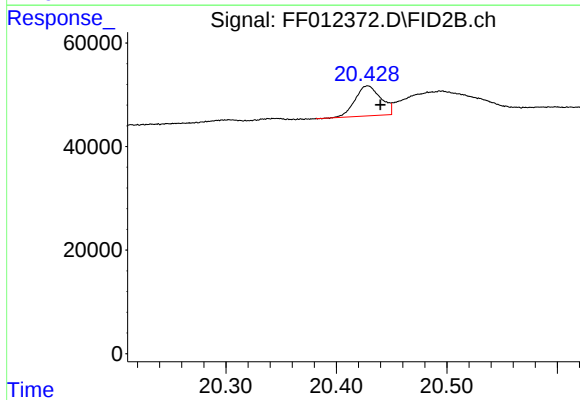

#16 N-HEXATRIACONTANE

R.T.: 20.428 min
Delta R.T.: -0.012 min
Response: 94325
Conc: 1.08 ug/ml