

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040120\
Data File : FF006710.D
Signal(s) : FID2B.ch
Acq On : 01 Apr 2020 10:23
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 01 15:14:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13)	N-TRIACONTANE	17.631	135001	0.954 ug/ml
14)	N-DOTRIACONTANE	18.460	376789	2.795 ug/ml
15)	N-TETRATRIACONTANE	19.238	137003	1.213 ug/ml
16)	N-HEXATRIACONTANE	19.975	147440	1.605 ug/ml
17)	N-OCTATRIACONTANE	20.691	140824	2.039 ug/ml
18)	N-TETRACONTANE	21.576	451610	6.526 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040120\
Data File : FF006710.D
Signal(s) : FID2B.ch
Acq On : 01 Apr 2020 10:23
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 01 15:14:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

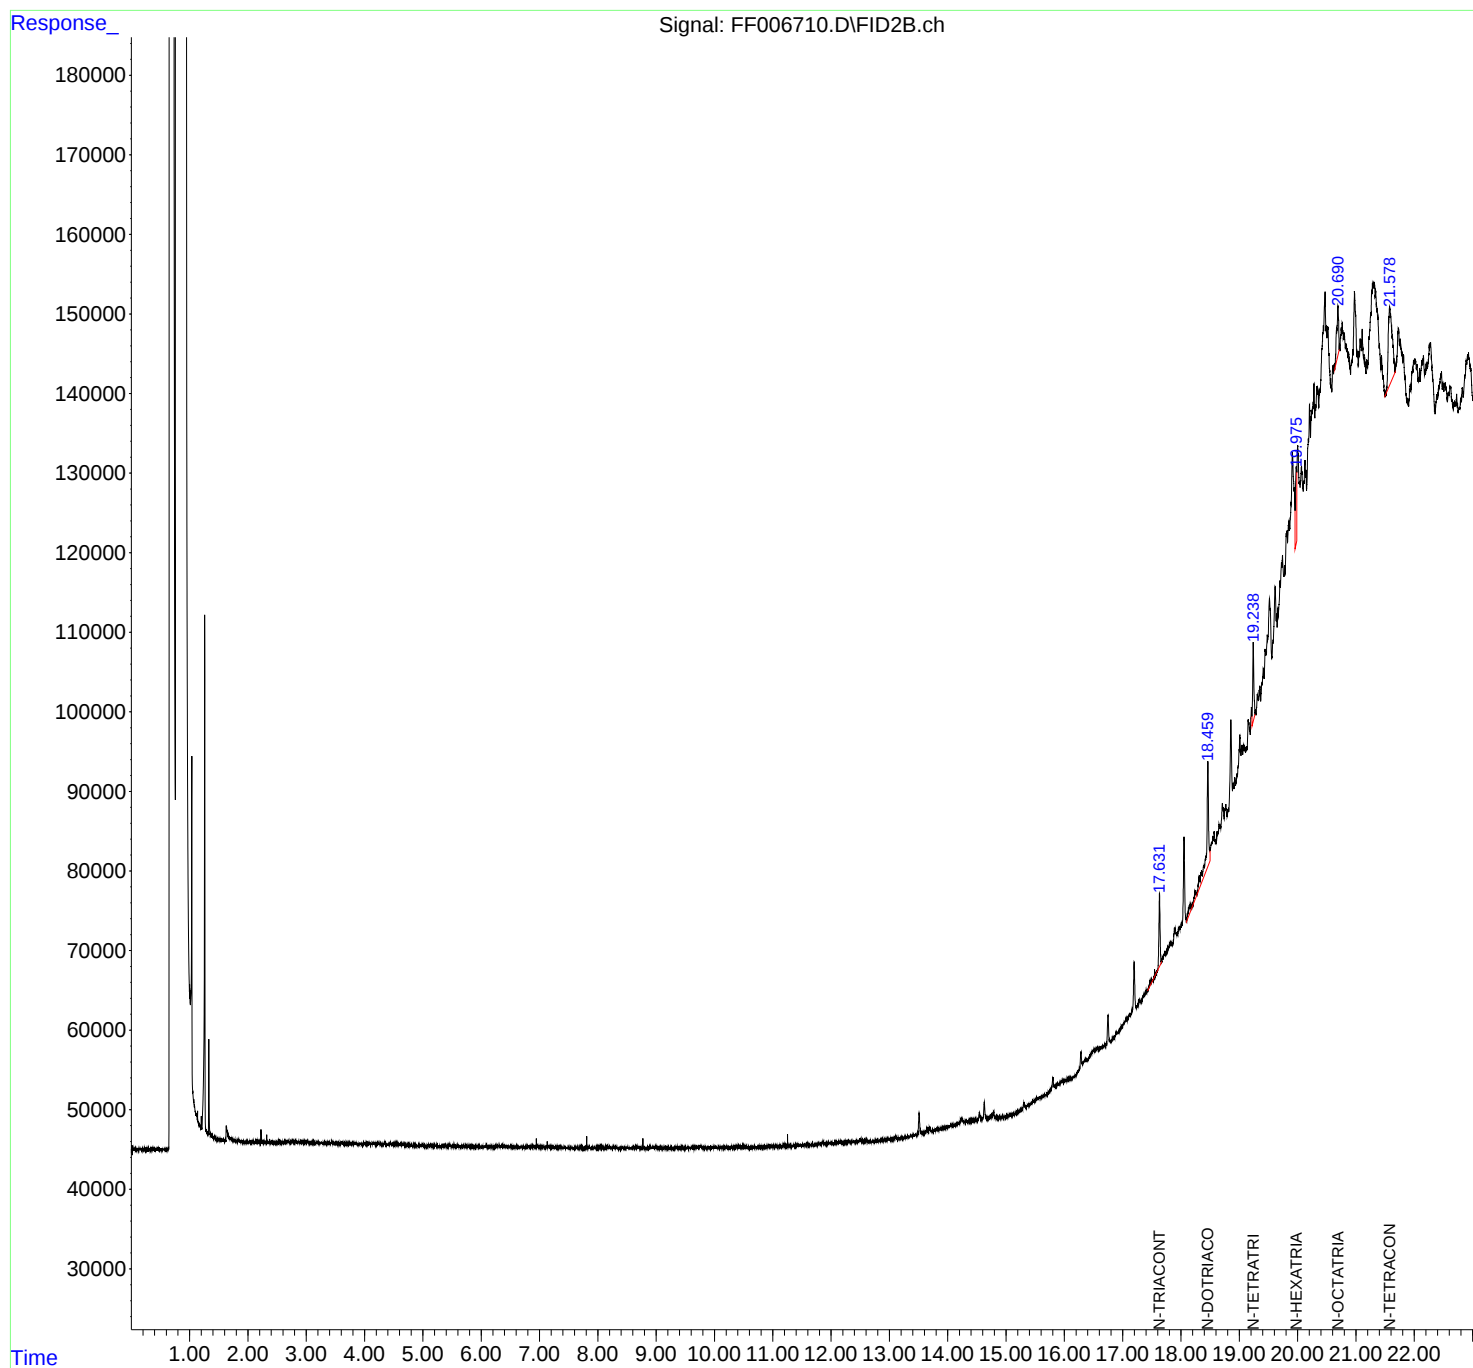


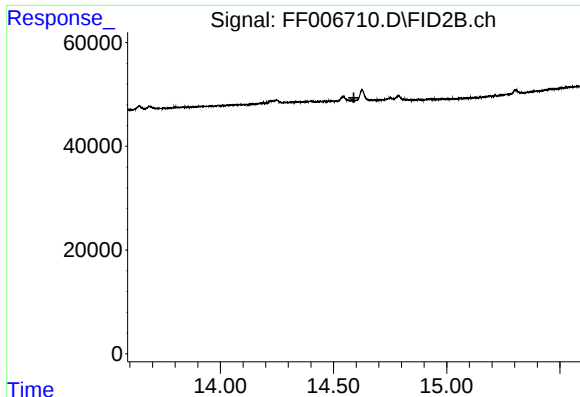

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.590 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

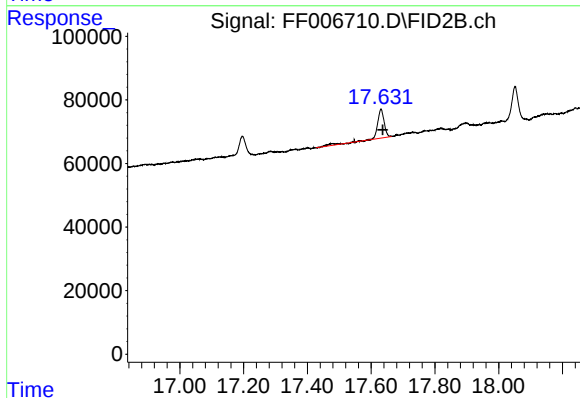


#13 N-TRIACONTANE

R.T.: 17.631 min
Delta R.T.: -0.005 min
Response: 135001
Conc: 0.95 ug/ml

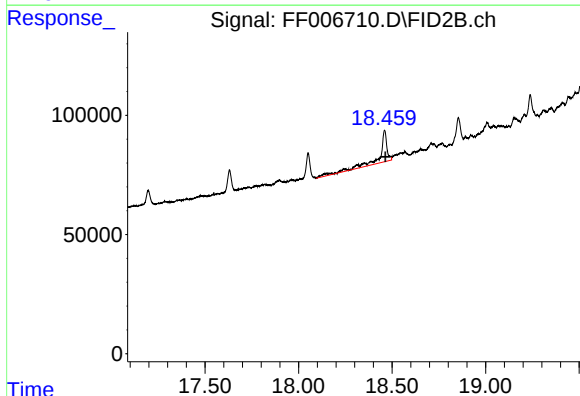


#14 N-DOTRIACONTANE

R.T.: 18.460 min
Delta R.T.: -0.004 min
Response: 376789
Conc: 2.80 ug/ml

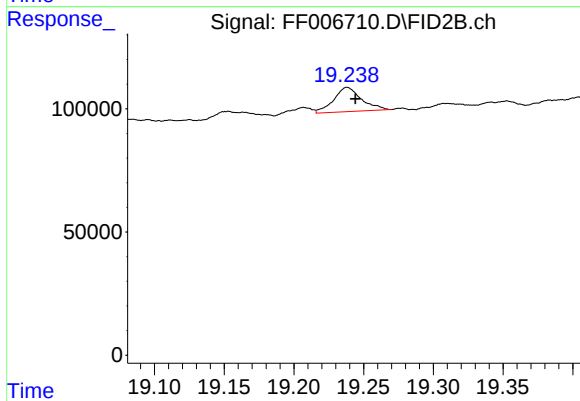

#15 N-TETRATRIACONTANE


R.T.: 19.238 min
Delta R.T.: -0.006 min
Response: 137003
Conc: 1.21 ug/ml

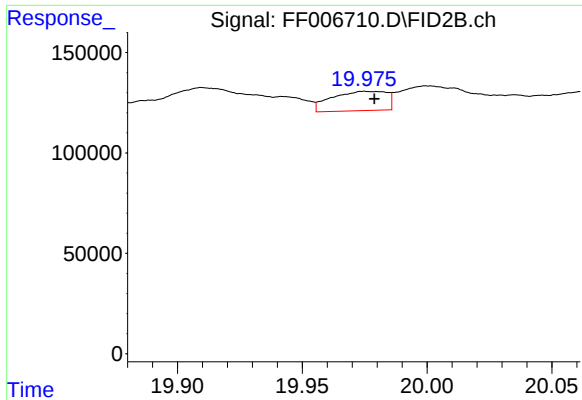

#16 N-HEXATRIACONTANE


R.T.: 19.975 min
Delta R.T.: -0.003 min
Response: 147440
Conc: 1.61 ug/ml

Instrument :
FID_F
ClientSampleId :

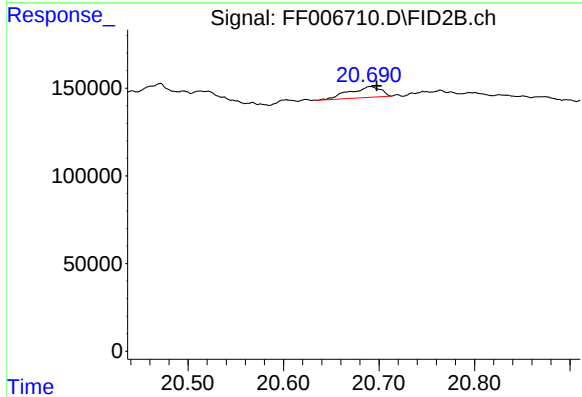

#17 N-OCTATRIACONTANE

R.T.: 20.691 min
Delta R.T.: -0.007 min
Response: 140824
Conc: 2.04 ug/ml

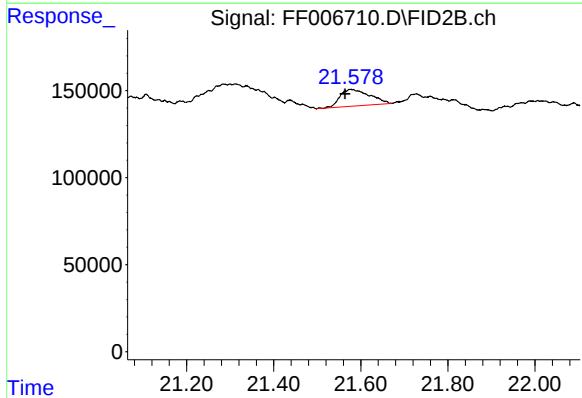

#18 N-TETRACONTANE

R.T.: 21.576 min
Delta R.T.: 0.012 min
Response: 451610
Conc: 6.53 ug/ml