

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040120\
 Data File : FF006716.D
 Signal(s) : FID2B.ch
 Acq On : 01 Apr 2020 13:33
 Operator : DD\AJ
 Sample : L1762-23 5X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 01 15:14:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.586	627527	4.876 ug/ml
Target Compounds			
4) N-TETRADECANE	8.219f	225462	1.576 ug/ml
5) N-HEXADECANE	9.772	52902	0.361 ug/ml
6) N-OCTADECANE	11.237	163453	1.106 ug/ml
7) N-EICOSANE	12.514	428776	2.885 ug/ml
8) N-DOCOSANE	13.688	227036	1.529 ug/ml
10) N-TETRACOSANE	14.784	3307375	22.378 ug/ml
11) N-HEXACOSANE	15.800	229609	1.584 ug/ml
12) N-OCTACOSANE	16.751	288738	2.016 ug/ml
13) N-TRIACONTANE	17.636	564671	3.990 ug/ml
14) N-DOTRIACONTANE	18.441	1053933	7.819 ug/ml
15) N-TETRATRIACONTANE	19.246	133716	1.184 ug/ml
16) N-HEXATRIACONTANE	19.985	309085	3.365 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040120\
Data File : FF006716.D
Signal(s) : FID2B.ch
Acq On : 01 Apr 2020 13:33
Operator : DD\AJ
Sample : L1762-23 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 01 15:14:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

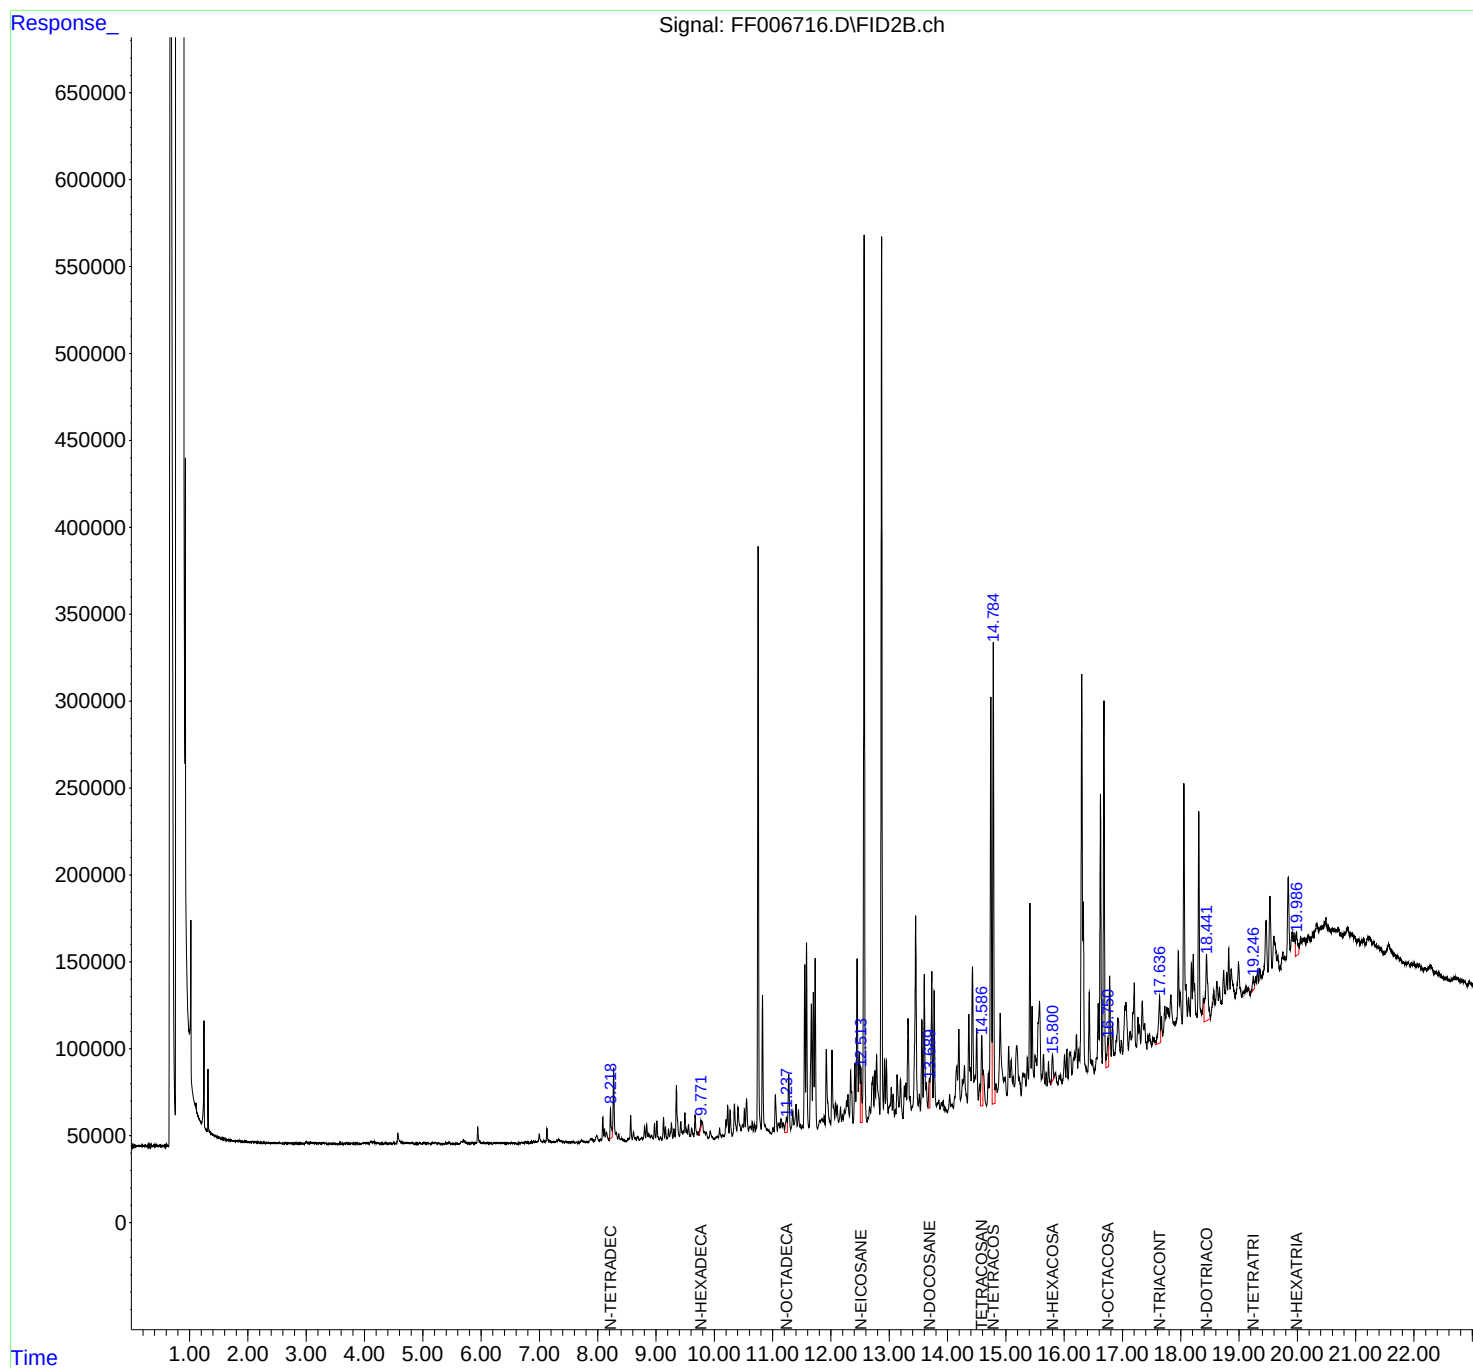


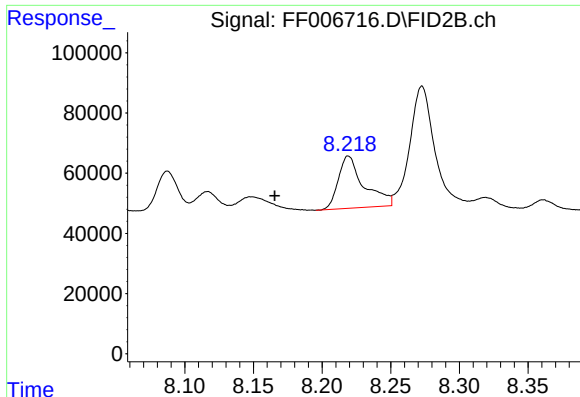

#4 N-TETRADECANE


R.T.: 8.219 min
Delta R.T.: 0.054 min
Response: 225462
Conc: 1.58 ug/ml

Instrument :
FID_F
ClientSampleId :

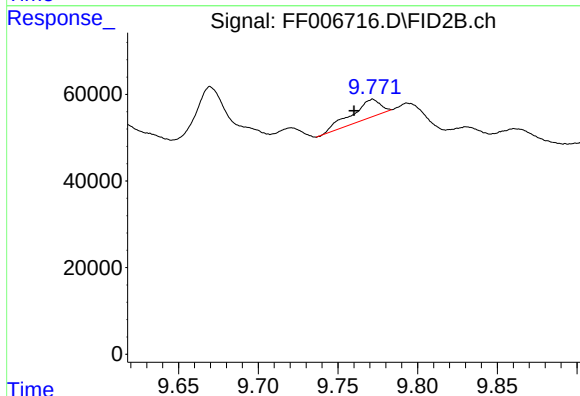


#5 N-HEXADECANE

R.T.: 9.772 min
Delta R.T.: 0.012 min
Response: 52902
Conc: 0.36 ug/ml

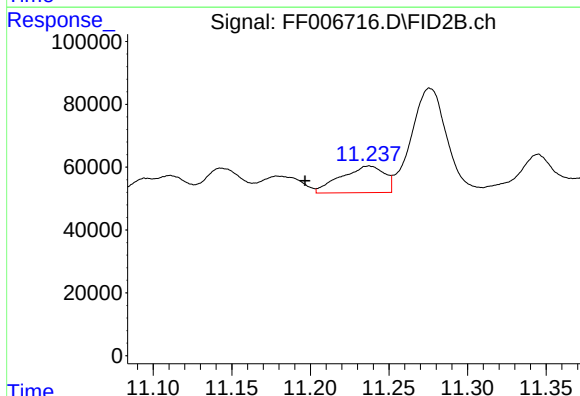


#6 N-OCTADECANE

R.T.: 11.237 min
Delta R.T.: 0.041 min
Response: 163453
Conc: 1.11 ug/ml

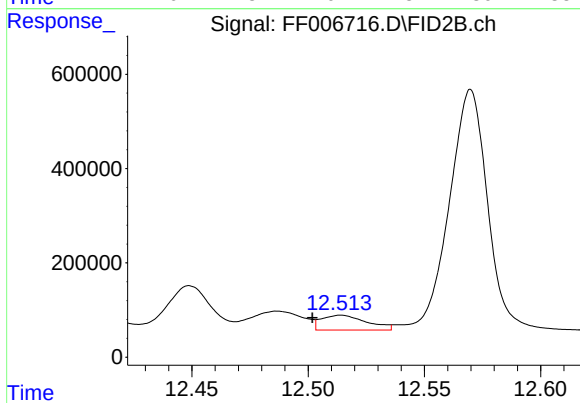

#7 N-EICOSANE


R.T.: 12.514 min
Delta R.T.: 0.012 min
Response: 428776
Conc: 2.88 ug/ml

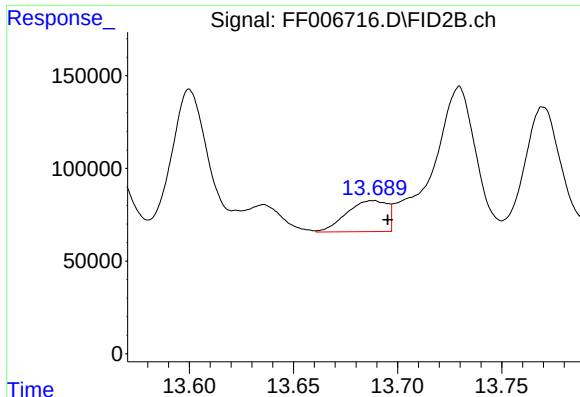

#8 N-DOCOSANE


R.T.: 13.688 min
Delta R.T.: -0.007 min
Response: 227036
Conc: 1.53 ug/ml

Instrument :
FID_F
ClientSampleId :

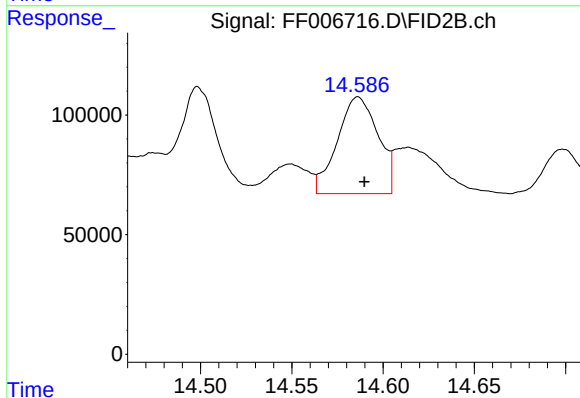


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.586 min
Delta R.T.: -0.004 min
Response: 627527
Conc: 4.88 ug/ml

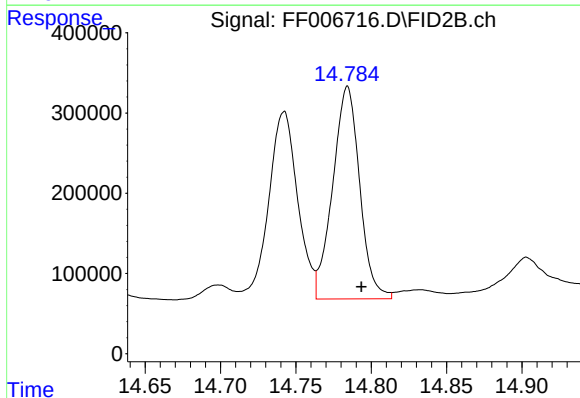


#10 N-TETRACOSANE

R.T.: 14.784 min
Delta R.T.: -0.009 min
Response: 3307375
Conc: 22.38 ug/ml

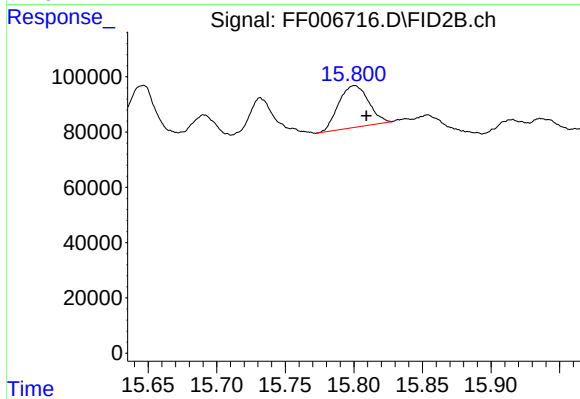

#11 N-HEXACOSANE


R.T.: 15.800 min
Delta R.T.: -0.009 min
Response: 229609
Conc: 1.58 ug/ml

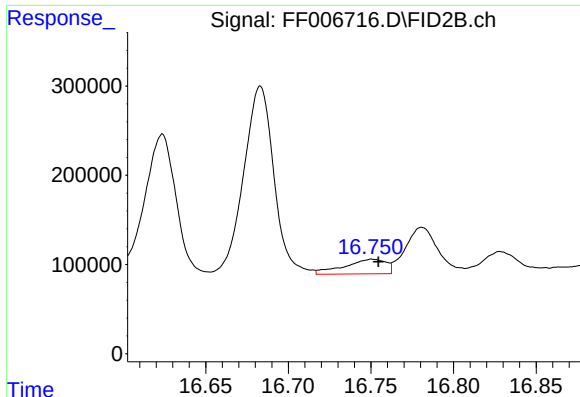

#12 N-OCTACOSANE


R.T.: 16.751 min
Delta R.T.: -0.004 min
Response: 288738
Conc: 2.02 ug/ml

Instrument :
FID_F
ClientSampleId :

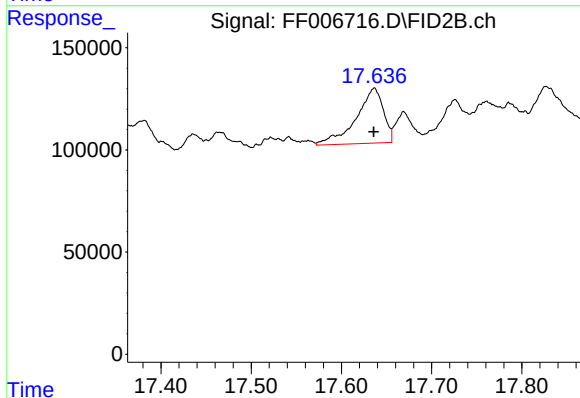


#13 N-TRIACONTANE

R.T.: 17.636 min
Delta R.T.: 0.000 min
Response: 564671
Conc: 3.99 ug/ml

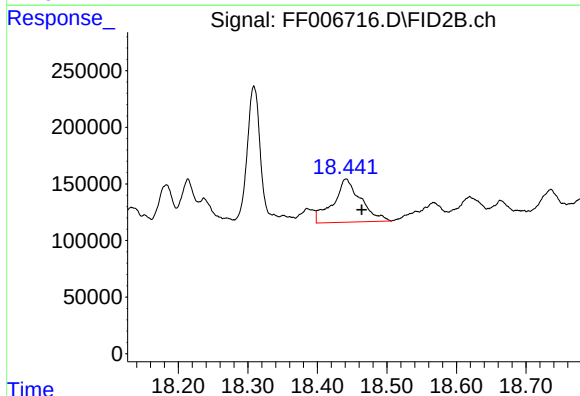


#14 N-DOTRIACONTANE

R.T.: 18.441 min
Delta R.T.: -0.023 min
Response: 1053933
Conc: 7.82 ug/ml

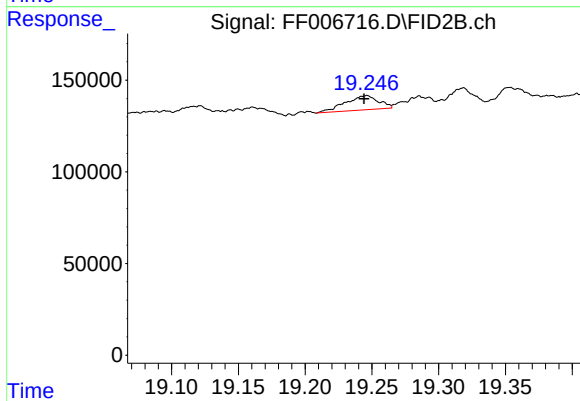

#15 N-TETRATRIACONTANE

R.T.: 19.246 min
Delta R.T.: 0.002 min
Response: 133716
Conc: 1.18 ug/ml

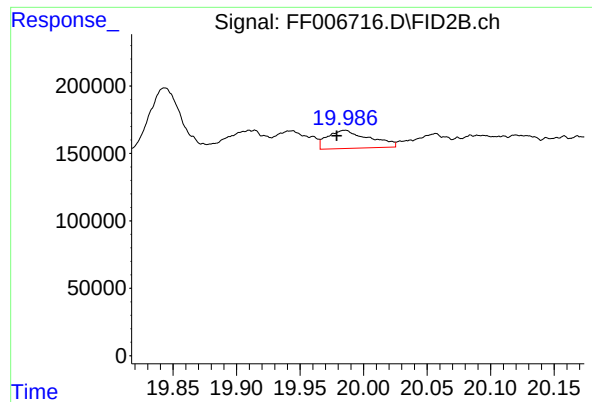

#16 N-HEXATRIACONTANE

R.T.: 19.985 min
Delta R.T.: 0.006 min
Response: 309085
Conc: 3.37 ug/ml

Instrument :
FID_F
ClientSampleId :