

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040120\
 Data File : FF006721.D
 Signal(s) : FID2B.ch
 Acq On : 01 Apr 2020 16:05
 Operator : DD\AJ
 Sample : L2055-02
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 02 00:57:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.587	1567123	12.176 ug/ml
Target Compounds			
4) N-TETRADECANE	8.123	101114	0.707 ug/ml
7) N-EICOSANE	12.566f	318326	2.142 ug/ml
8) N-DOCOSANE	13.691	82018	0.552 ug/ml
10) N-TETRACOSANE	14.783	291115	1.970 ug/ml
11) N-HEXACOSANE	15.808	215107	1.484 ug/ml
12) N-OCTACOSANE	16.754	442573	3.090 ug/ml
13) N-TRIACONTANE	17.641	1138948	8.047 ug/ml
14) N-DOTRIACONTANE	18.464	896986	6.654 ug/ml
15) N-TETRATRIACONTANE	19.248	439774	3.895 ug/ml
16) N-HEXATRIACONTANE	19.970	180775	1.968 ug/ml
17) N-OCTATRIACONTANE	20.701	142572	2.065 ug/ml
18) N-TETRACONTANE	21.566	113143	1.635 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040120\
Data File : FF006721.D
Signal(s) : FID2B.ch
Acq On : 01 Apr 2020 16:05
Operator : DD\AJ
Sample : L2055-02
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 02 00:57:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

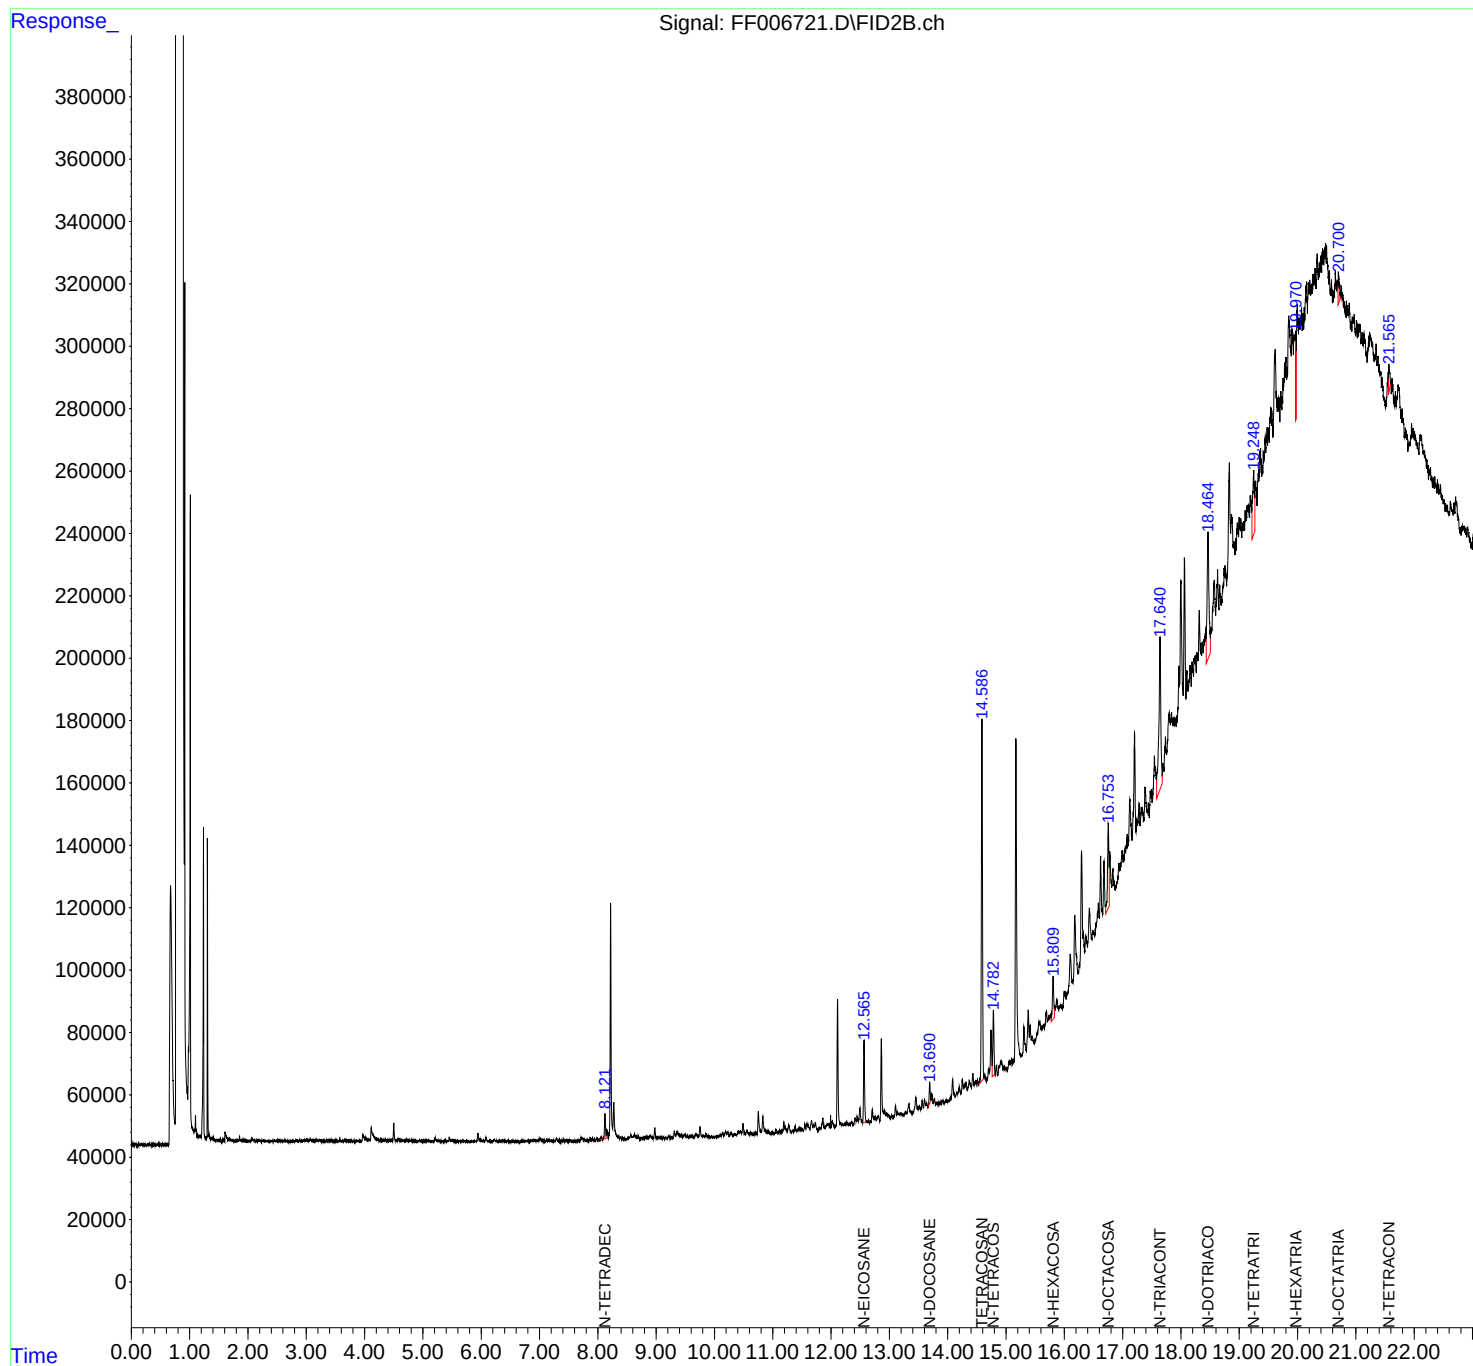


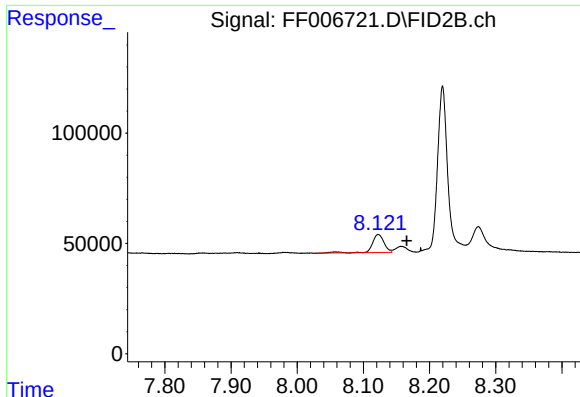

#4 N-TETRADECANE


R.T.: 8.123 min
Delta R.T.: -0.043 min
Response: 101114
Conc: 0.71 ug/ml

Instrument :
FID_F
ClientSampleId :

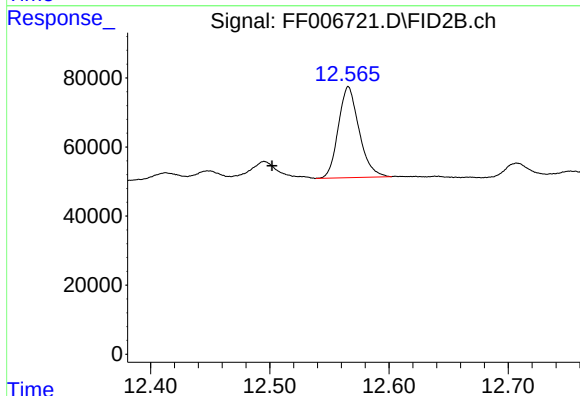


#7 N-EICOSANE

R.T.: 12.566 min
Delta R.T.: 0.064 min
Response: 318326
Conc: 2.14 ug/ml

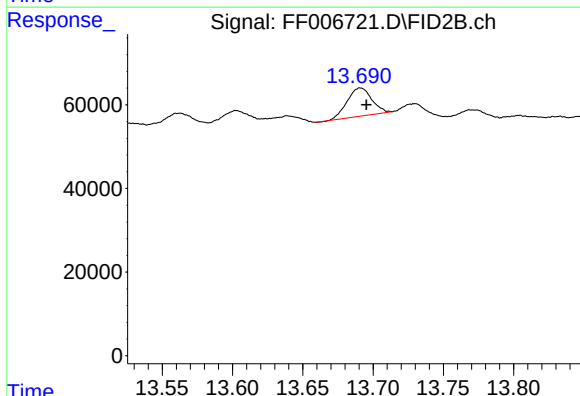


#8 N-DOCOSANE

R.T.: 13.691 min
Delta R.T.: -0.004 min
Response: 82018
Conc: 0.55 ug/ml

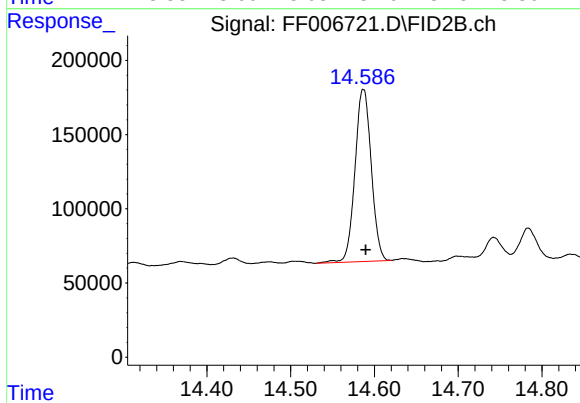

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.587 min
Delta R.T.: -0.003 min
Response: 1567123
Conc: 12.18 ug/ml

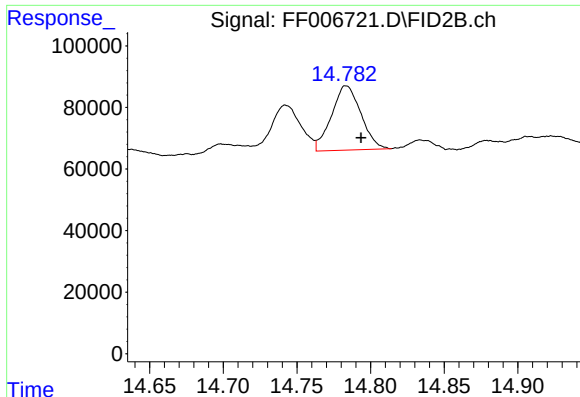

#10 N-TETRACOSANE


R.T.: 14.783 min
Delta R.T.: -0.010 min
Response: 291115
Conc: 1.97 ug/ml

Instrument :
FID_F
ClientSampleId :

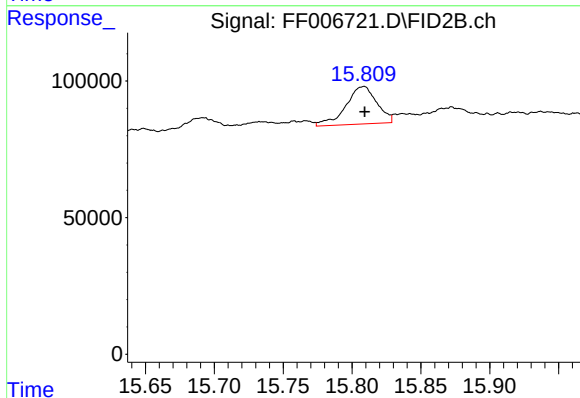


#11 N-HEXACOSANE

R.T.: 15.808 min
Delta R.T.: 0.000 min
Response: 215107
Conc: 1.48 ug/ml

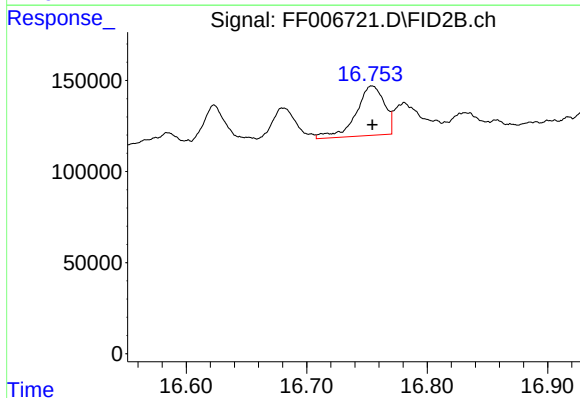


#12 N-OCTACOSANE

R.T.: 16.754 min
Delta R.T.: 0.000 min
Response: 442573
Conc: 3.09 ug/ml

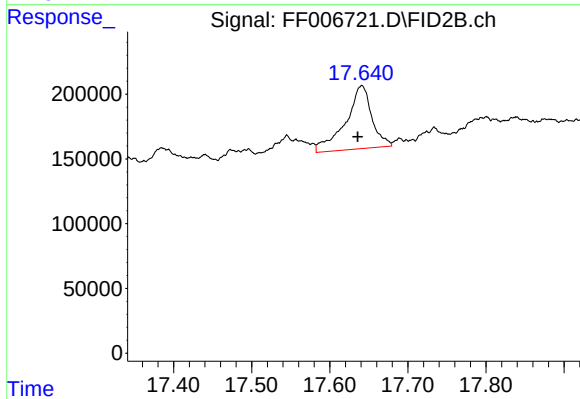

#13 N-TRIACONTANE


R.T.: 17.641 min
Delta R.T.: 0.005 min
Response: 1138948
Conc: 8.05 ug/ml

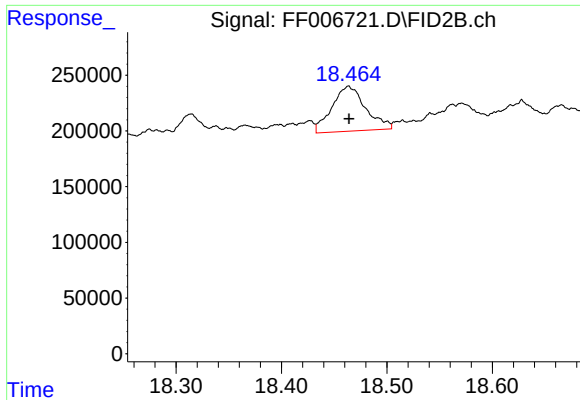

#14 N-DOTRIACONTANE


R.T.: 18.464 min
Delta R.T.: 0.000 min
Response: 896986
Conc: 6.65 ug/ml

Instrument :
FID_F
ClientSampleId :

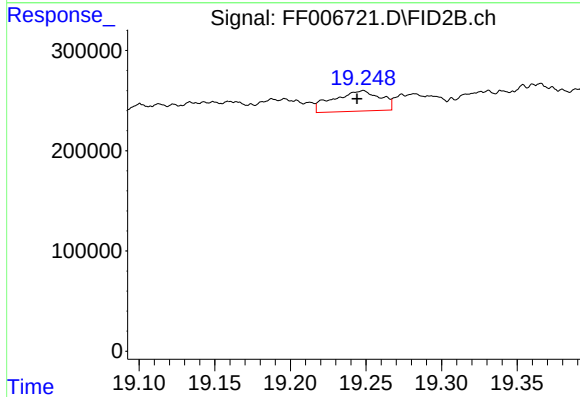


#15 N-TETRATRIACONTANE

R.T.: 19.248 min
Delta R.T.: 0.004 min
Response: 439774
Conc: 3.89 ug/ml

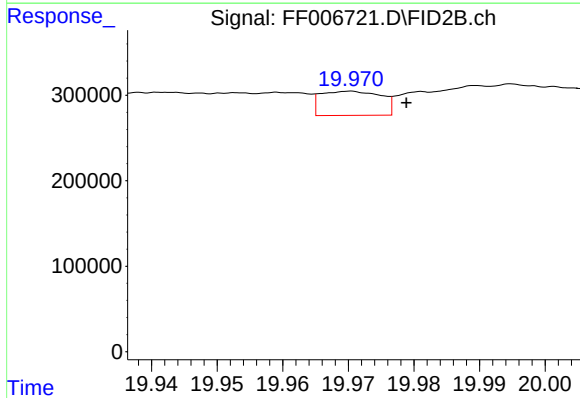


#16 N-HEXATRIACONTANE

R.T.: 19.970 min
Delta R.T.: -0.009 min
Response: 180775
Conc: 1.97 ug/ml

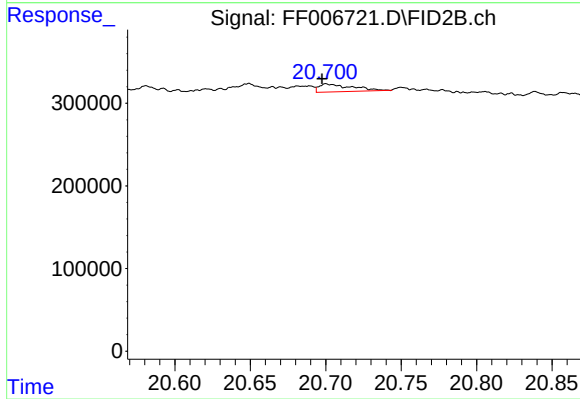

#17 N-OCTATRIACONTANE

R.T.: 20.701 min
Delta R.T.: 0.003 min
Response: 142572
Conc: 2.06 ug/ml

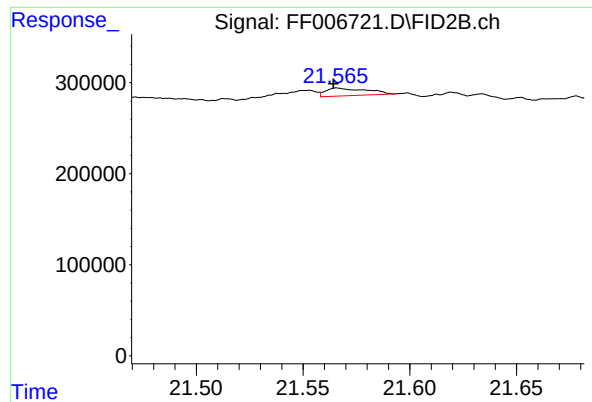

#18 N-TETRACONTANE

R.T.: 21.566 min
Delta R.T.: 0.002 min
Response: 113143
Conc: 1.64 ug/ml

Instrument :
FID_F
ClientSampleId :