

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040122\
Data File : FF010240.D
Signal(s) : FID2B.ch
Acq On : 01 Apr 2022 16:42
Operator : AJ\MA
Sample : N1870-19 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Apr 01 17:12:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.624	480673	4.021 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040122\
Data File : FF010240.D
Signal(s) : FID2B.ch
Acq On : 01 Apr 2022 16:42
Operator : AJ\MA
Sample : N1870-19 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Apr 01 17:12:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

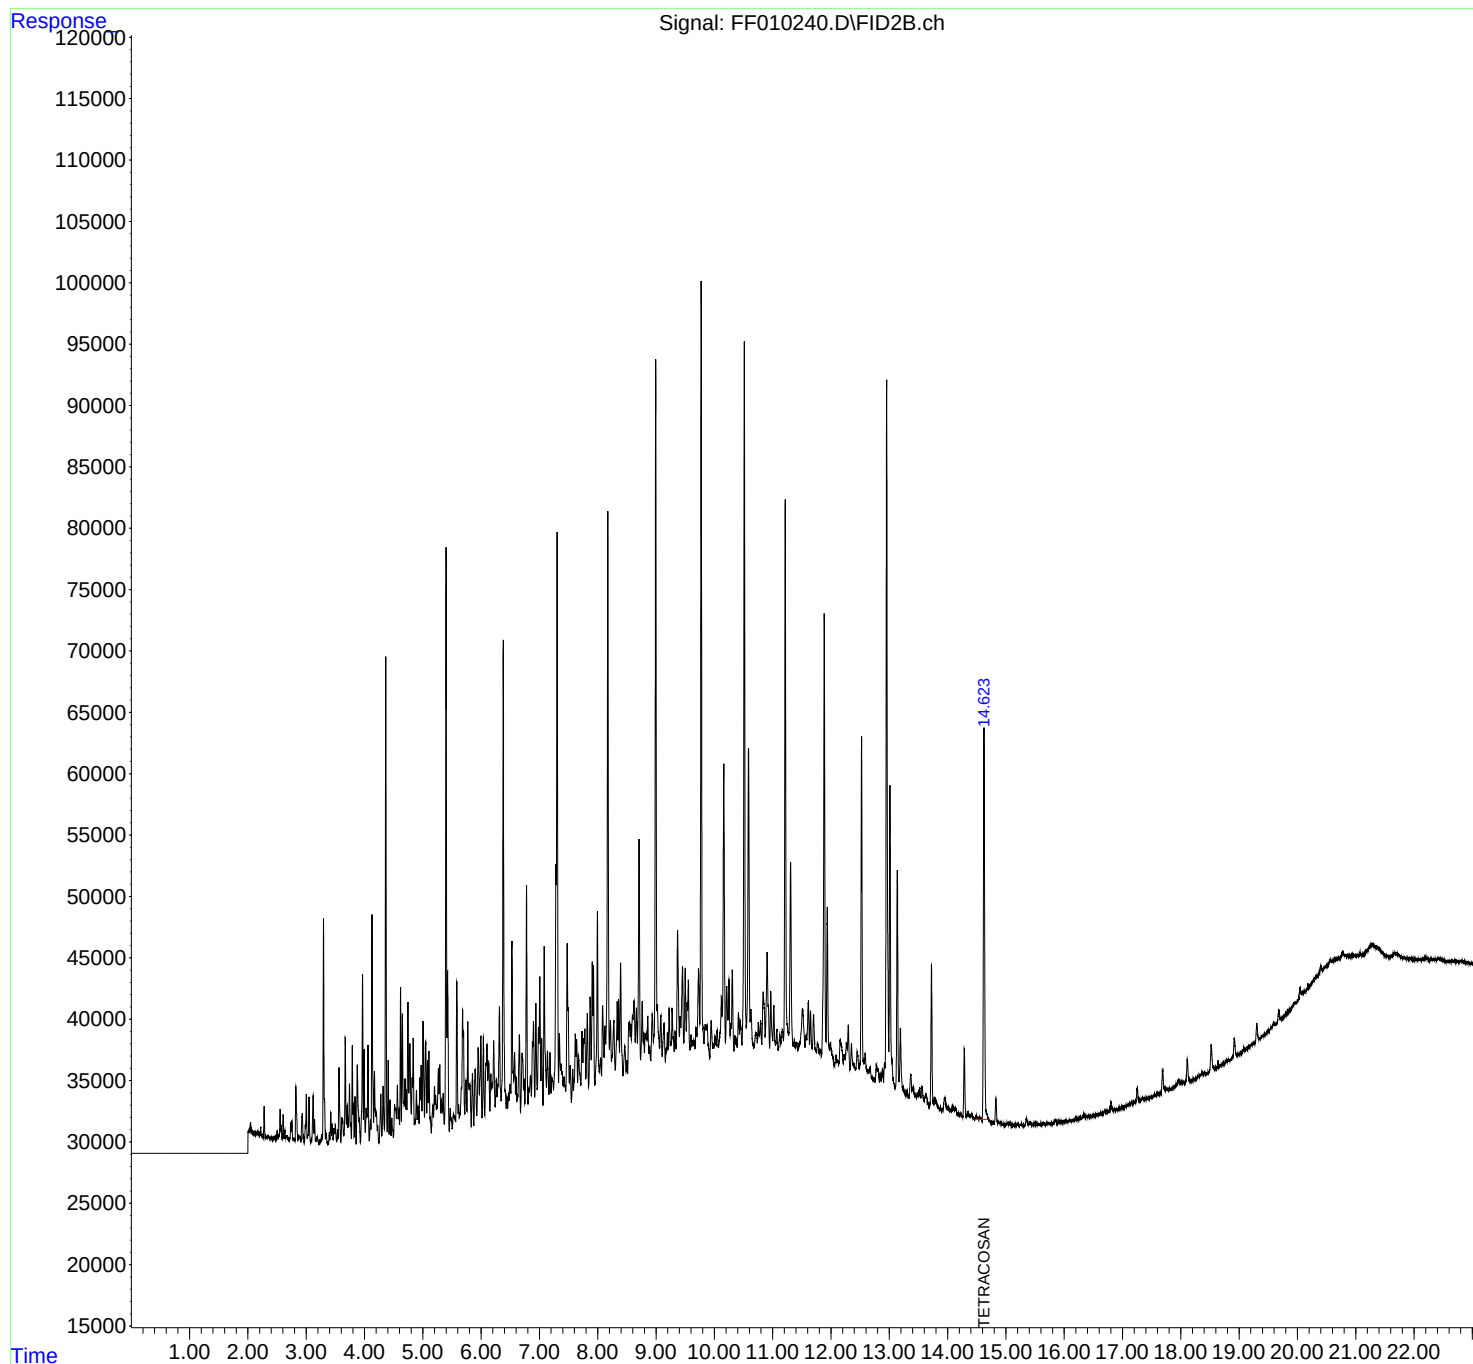

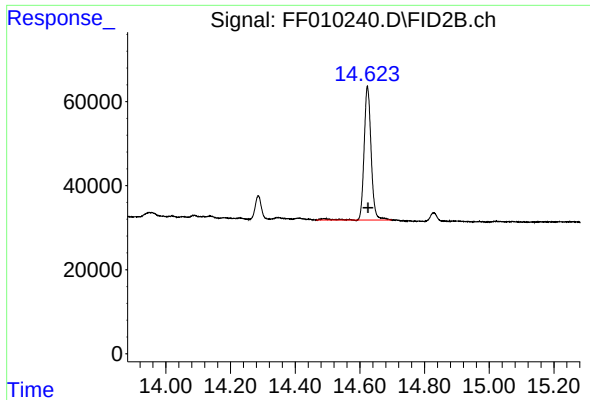

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.624 min
Delta R.T.: -0.002 min
Response: 480673
Conc: 4.02 ug/ml

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP