

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040219\
 Data File : FF004052.D
 Signal(s) : FID2B.ch
 Acq On : 02 Apr 2019 10:01
 Operator : AJ\SJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 TRPH STD

Integration File: autoint1.e
 Quant Time: Apr 02 10:59:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 10:58:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.553	6160388	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.206	6871857	50.000 ug/ml
2) N-DECANE	4.294	6918944	50.000 ug/ml
3) N-DODECANE	6.314	7116500	50.000 ug/ml
4) N-TETRADECANE	8.106	7202785	50.000 ug/ml
5) N-HEXADECANE	9.704	7289248	50.000 ug/ml
6) N-OCTADECANE	11.146	7287000	50.000 ug/ml
7) N-EICOSANE	12.456	7194240	50.000 ug/ml
8) N-DOCOSANE	13.654	7104711	50.000 ug/ml
10) N-TETRACOSANE	14.758	6967579	50.000 ug/ml
11) N-HEXACOSANE	15.778	6848505	50.000 ug/ml
12) N-OCTACOSANE	16.730	6745590	50.000 ug/ml
13) N-TRIACONTANE	17.616	6642093	50.000 ug/ml
14) N-DOTRIACONTANE	18.450	6414345	50.000 ug/ml
15) N-TETRATRIACONTANE	19.234	6209532	50.000 ug/ml
16) N-HEXATRIACONTANE	19.977	6154886	50.000 ug/ml
17) N-OCTATRIACONTANE	20.700	5411902	50.000 ug/ml
18) N-TETRACONTANE	21.567	5506161	50.000 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040219\
Data File : FF004052.D
Signal(s) : FID2B.ch
Acq On : 02 Apr 2019 10:01
Operator : AJ\SJ
Sample : 50 TRPH STD
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

Integration File: autoint1.e
Quant Time: Apr 02 10:59:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 10:58:26 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

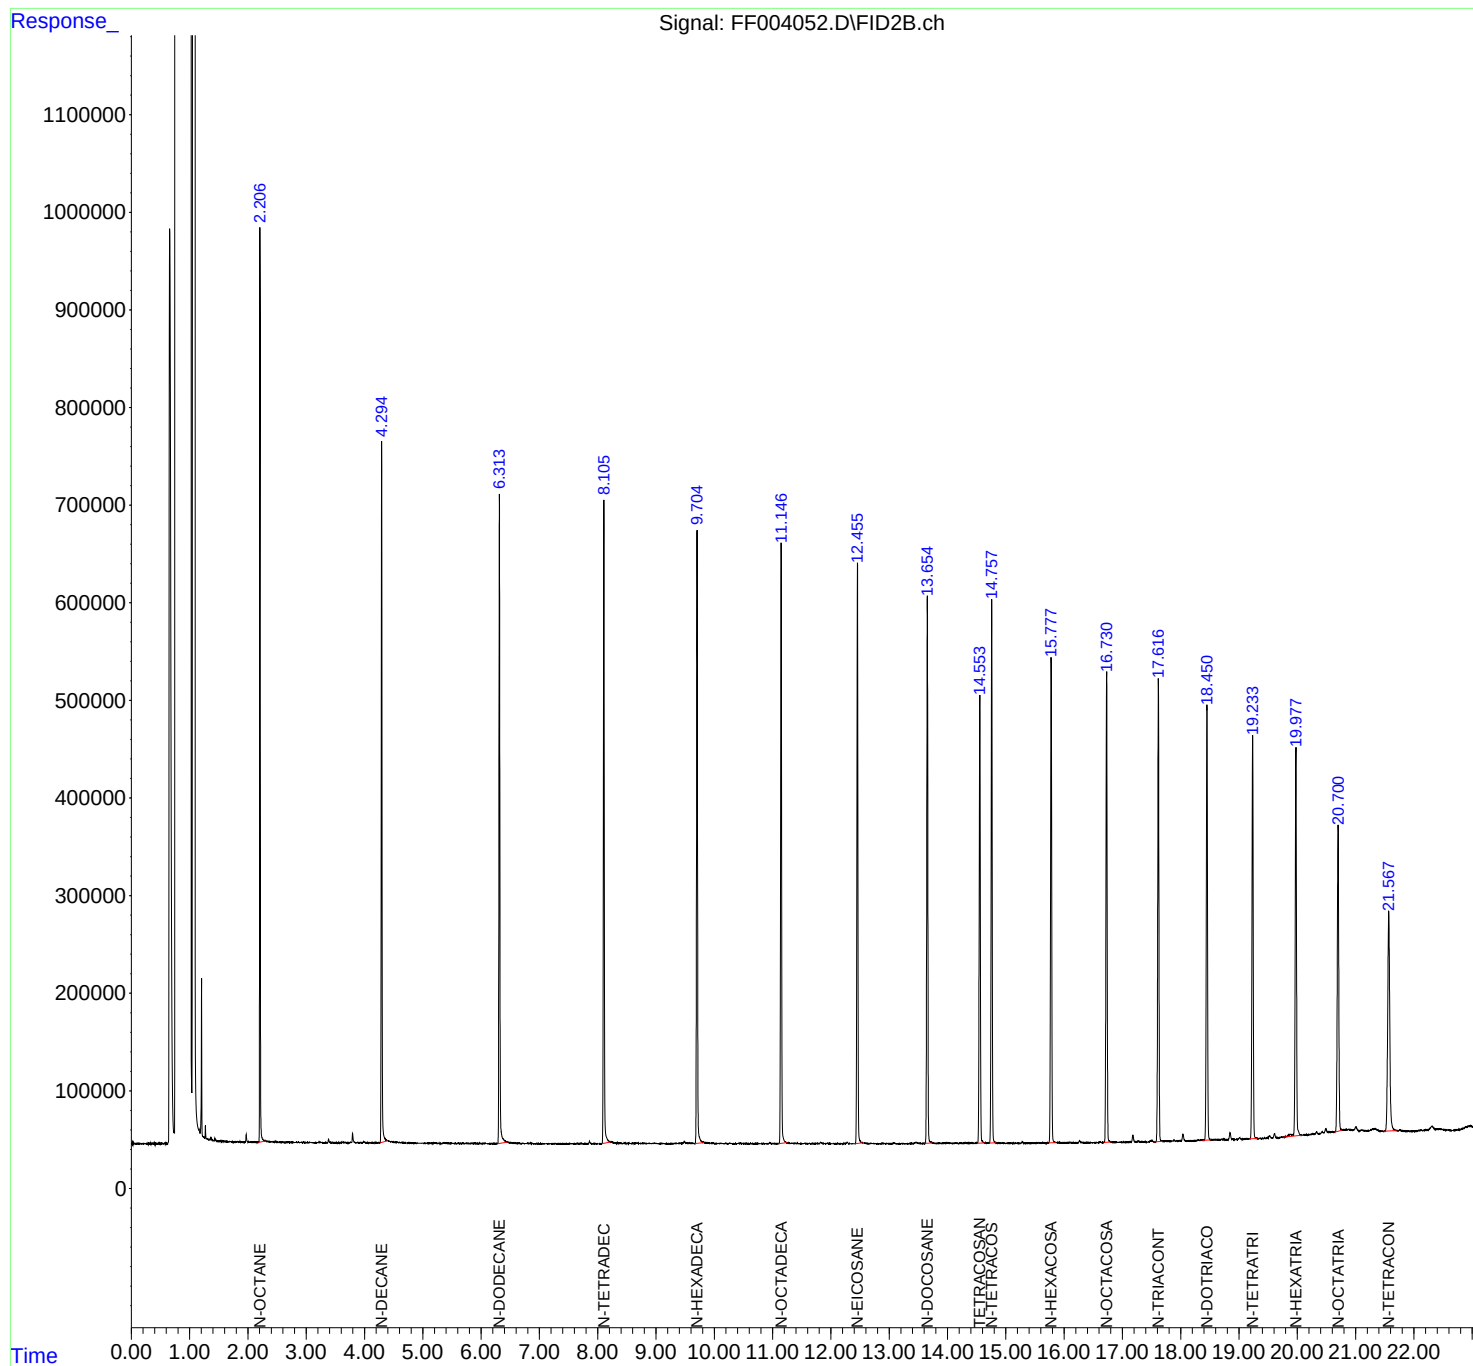


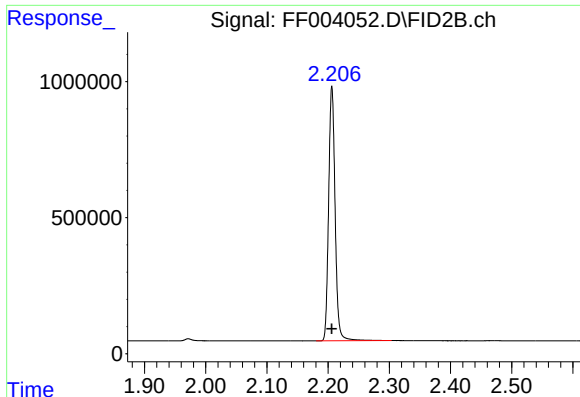

#1 N-OCTANE


R.T.: 2.206 min
Delta R.T.: 0.000 min
Response: 6871857
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

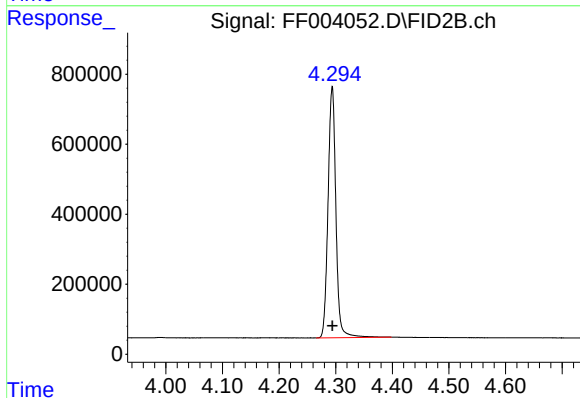


#2 N-DECANE

R.T.: 4.294 min
Delta R.T.: 0.000 min
Response: 6918944
Conc: 50.00 ug/ml

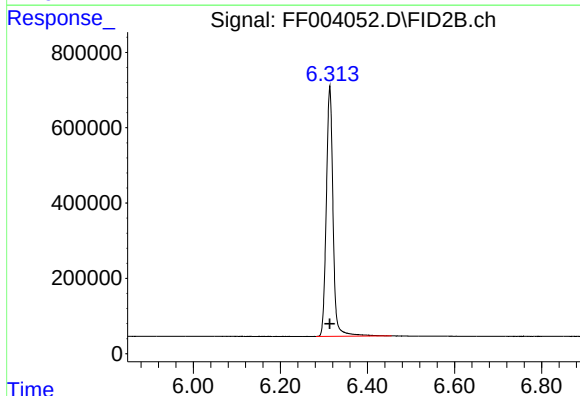


#3 N-DODECANE

R.T.: 6.314 min
Delta R.T.: 0.000 min
Response: 7116500
Conc: 50.00 ug/ml

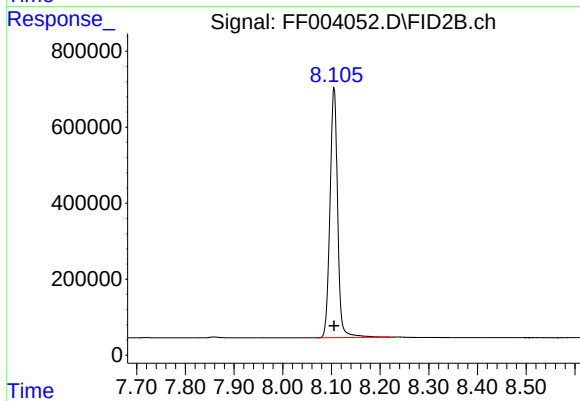

#4 N-TETRADECANE


R.T.: 8.106 min
Delta R.T.: 0.000 min
Response: 7202785
Conc: 50.00 ug/ml

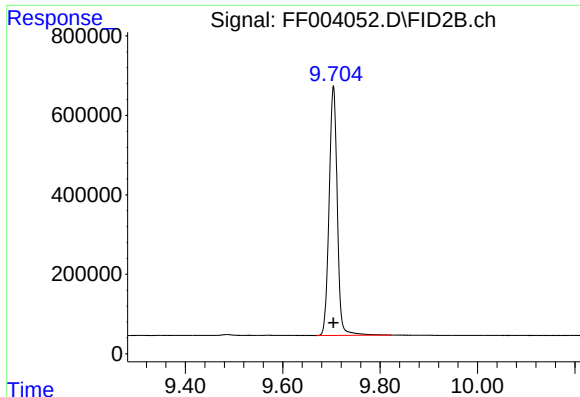

#5 N-HEXADECANE


R.T.: 9.704 min
Delta R.T.: 0.000 min
Response: 7289248
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

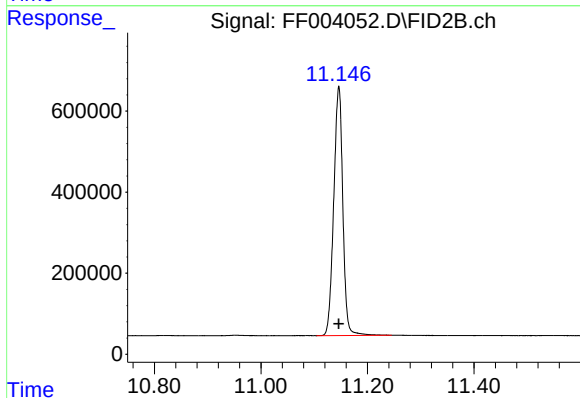


#6 N-OCTADECANE

R.T.: 11.146 min
Delta R.T.: 0.000 min
Response: 7287000
Conc: 50.00 ug/ml

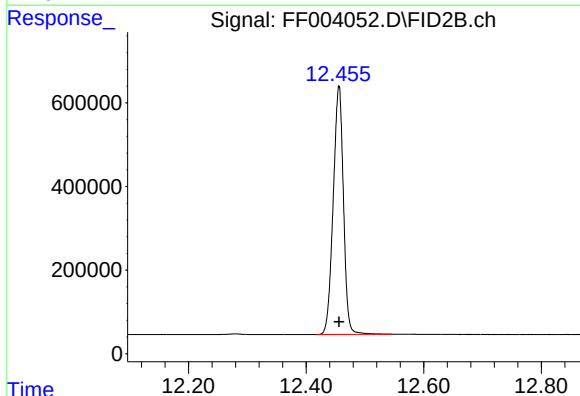


#7 N-EICOSANE

R.T.: 12.456 min
Delta R.T.: 0.000 min
Response: 7194240
Conc: 50.00 ug/ml

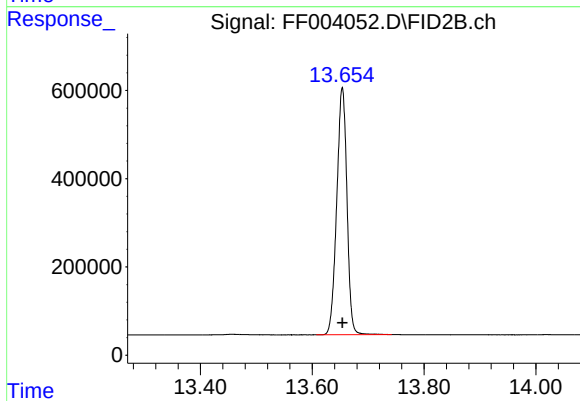

#8 N-DOCOSANE


R.T.: 13.654 min
Delta R.T.: 0.000 min
Response: 7104711
Conc: 50.00 ug/ml

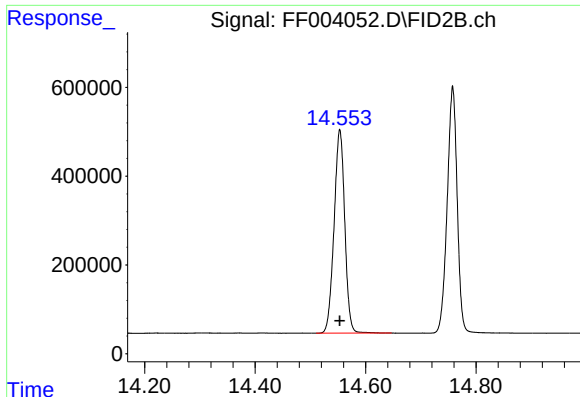

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.553 min
Delta R.T.: 0.000 min
Response: 6160388
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

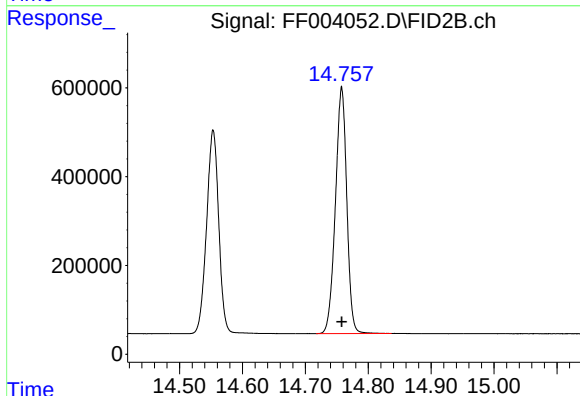


#10 N-TETRACOSANE

R.T.: 14.758 min
Delta R.T.: 0.000 min
Response: 6967579
Conc: 50.00 ug/ml

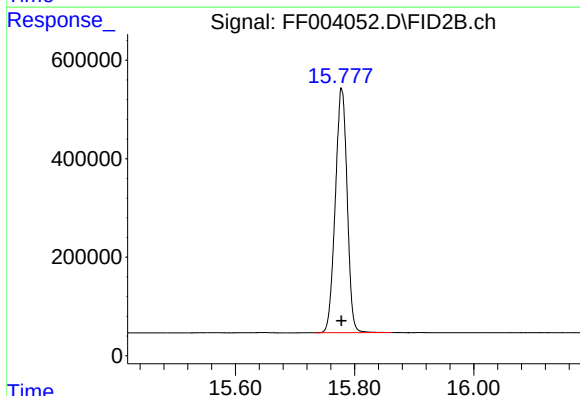


#11 N-HEXACOSANE

R.T.: 15.778 min
Delta R.T.: 0.000 min
Response: 6848505
Conc: 50.00 ug/ml

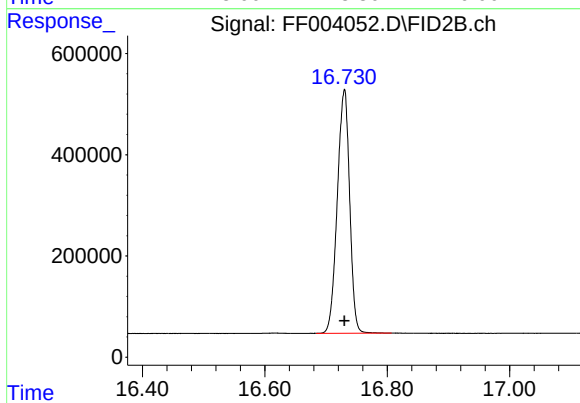

#12 N-OCTACOSANE


R.T.: 16.730 min
Delta R.T.: 0.000 min
Response: 6745590
Conc: 50.00 ug/ml

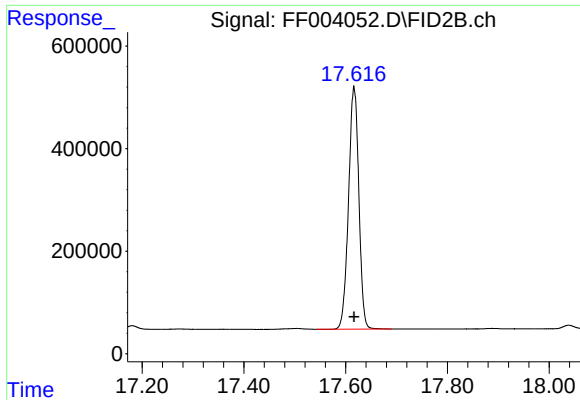

#13 N-TRIACONTANE


R.T.: 17.616 min
Delta R.T.: 0.000 min
Response: 6642093
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

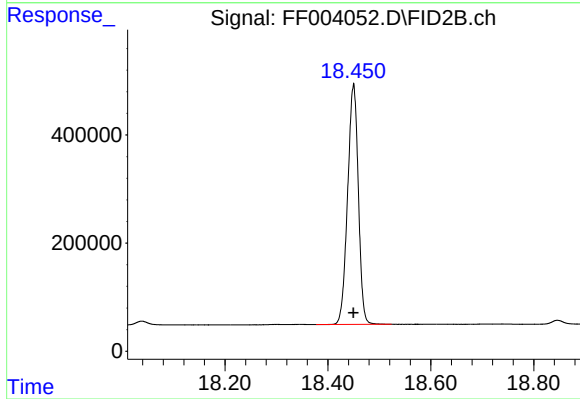


#14 N-DOTRIACONTANE

R.T.: 18.450 min
Delta R.T.: 0.000 min
Response: 6414345
Conc: 50.00 ug/ml

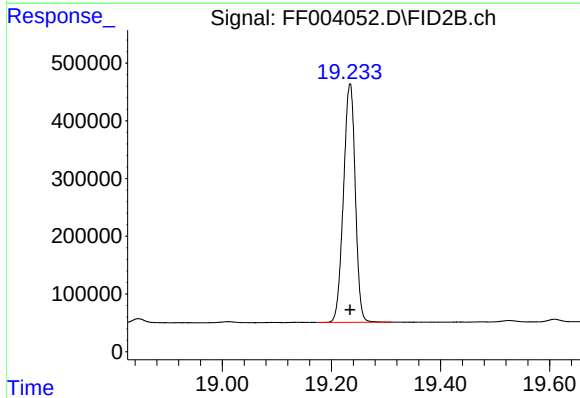


#15 N-TETRATRIACONTANE

R.T.: 19.234 min
Delta R.T.: 0.000 min
Response: 6209532
Conc: 50.00 ug/ml

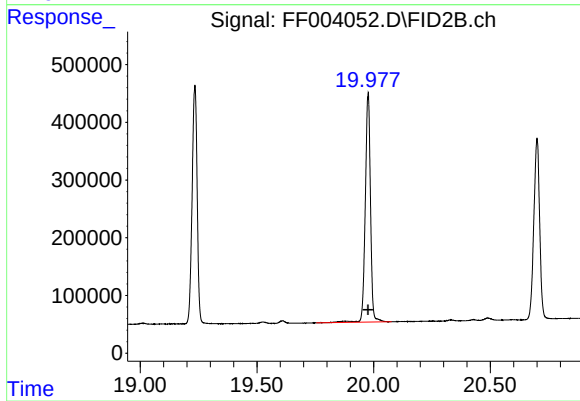

#16 N-HEXATRIACONTANE


R.T.: 19.977 min
Delta R.T.: 0.000 min
Response: 6154886
Conc: 50.00 ug/ml

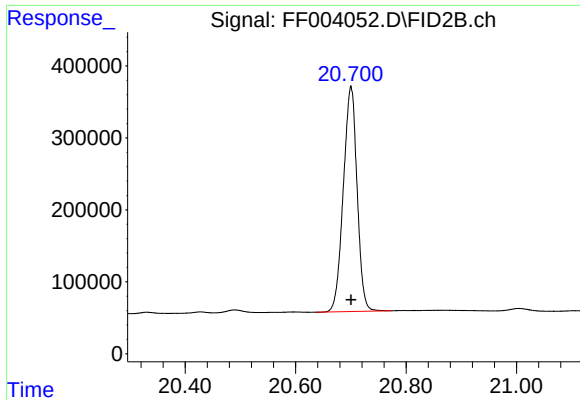

#17 N-OCTATRIACONTANE

R.T.: 20.700 min
Delta R.T.: 0.000 min
Response: 5411902
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

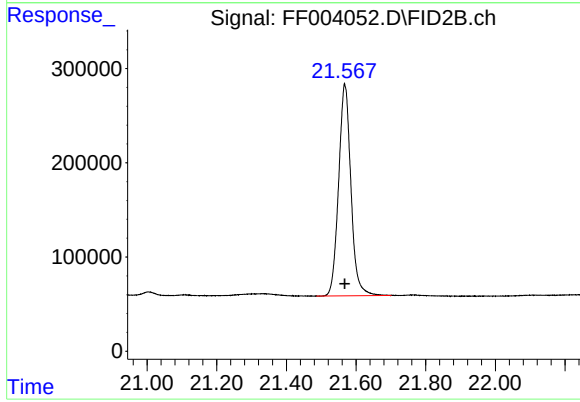

#18 N-TETRACONTANE

R.T.: 21.567 min
Delta R.T.: 0.000 min
Response: 5506161
Conc: 50.00 ug/ml