

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040219\
Data File : FF004059.D
Signal(s) : FID2B.ch
Acq On : 02 Apr 2019 15:26
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 02 23:56:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.313	3416031	24.348 ug/ml
12)	N-OCTACOSANE	16.726	3861540	26.856 ug/ml
13)	N-TRIACONTANE	17.614	287673	2.014 ug/ml
14)	N-DOTRIACONTANE	18.446	338277	2.396 ug/ml
15)	N-TETRATRIACONTANE	19.232	243487	1.826 ug/ml
16)	N-HEXATRIACONTANE	19.981	306399	2.415 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040219\
Data File : FF004059.D
Signal(s) : FID2B.ch
Acq On : 02 Apr 2019 15:26
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 02 23:56:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

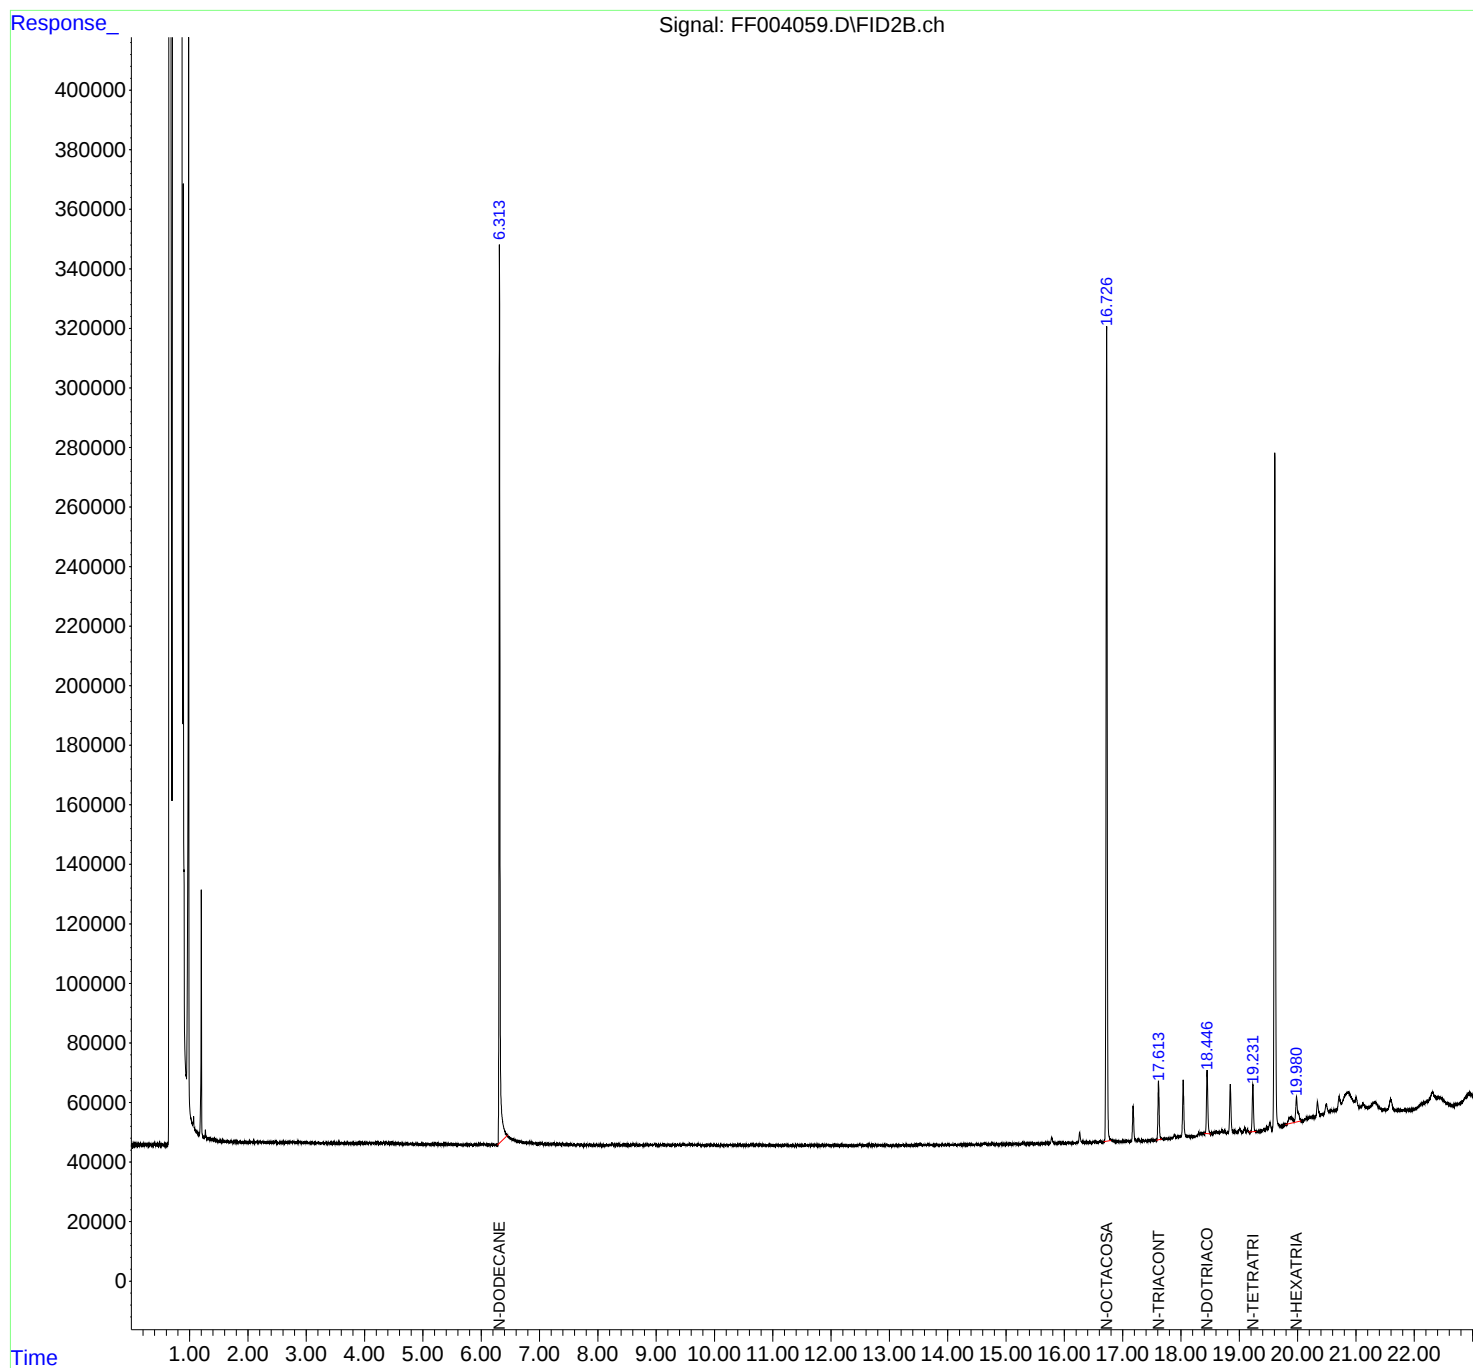


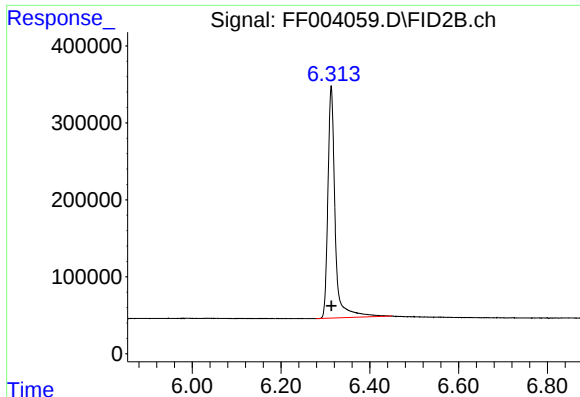

#3 N-DODECANE


R.T.: 6.313 min
Delta R.T.: 0.000 min
Response: 3416031
Conc: 24.35 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

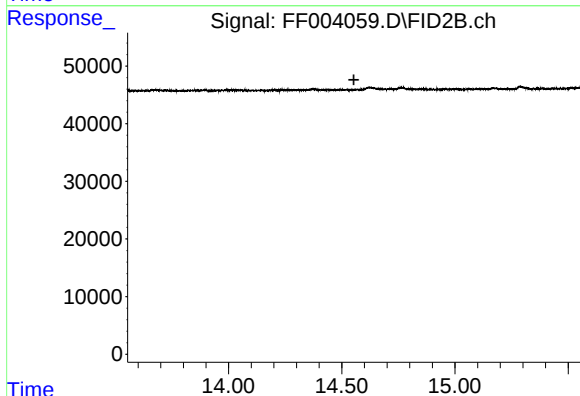


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.553 min
Response: 0
Conc: N.D.

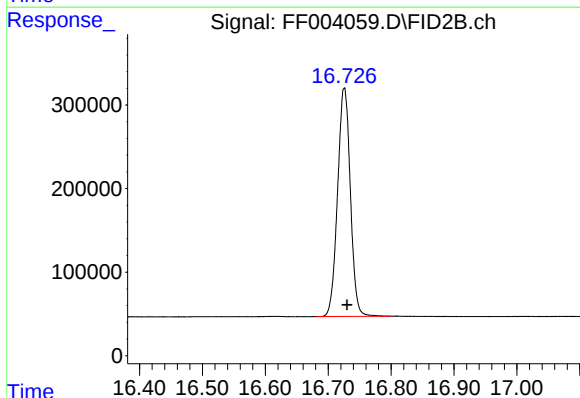


#12 N-OCTACOSANE

R.T.: 16.726 min
Delta R.T.: -0.005 min
Response: 3861540
Conc: 26.86 ug/ml

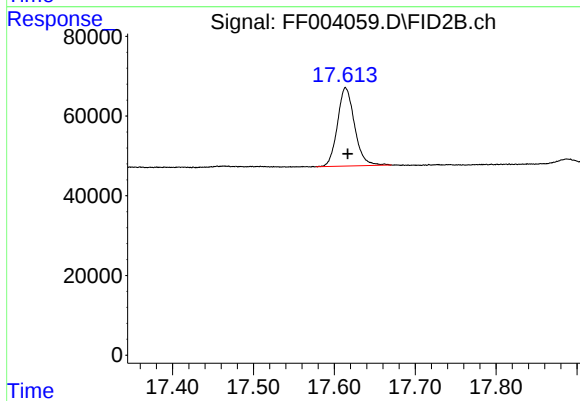

#13 N-TRIACONTANE


R.T.: 17.614 min
Delta R.T.: -0.003 min
Response: 287673
Conc: 2.01 ug/ml

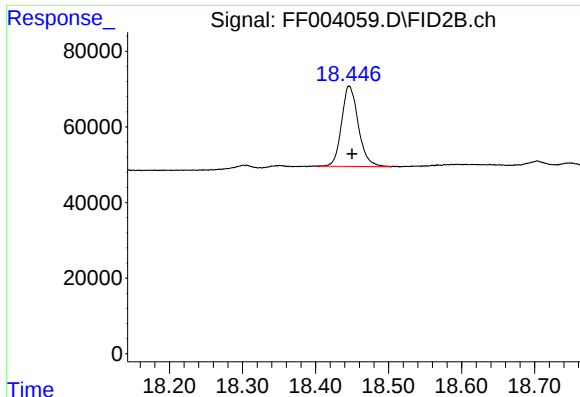

#14 N-DOTRIACONTANE


R.T.: 18.446 min
Delta R.T.: -0.004 min
Response: 338277
Conc: 2.40 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

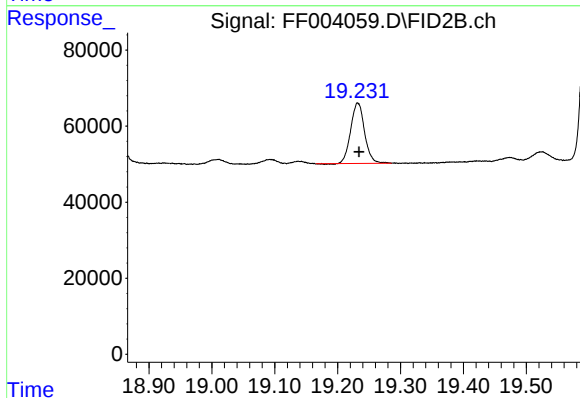

#15 N-TETRATRIACONTANE

R.T.: 19.232 min
Delta R.T.: -0.002 min
Response: 243487
Conc: 1.83 ug/ml

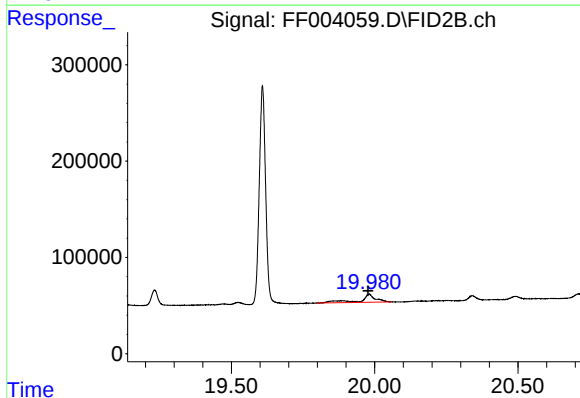

#16 N-HEXATRIACONTANE

R.T.: 19.981 min
Delta R.T.: 0.004 min
Response: 306399
Conc: 2.41 ug/ml