

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040219\
 Data File : FF004065.D
 Signal(s) : FID2B.ch
 Acq On : 02 Apr 2019 18:31
 Operator : AJ\SJ
 Sample : K2186-21
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 TP-TRACK-78-79

Integration File: autoint1.e
 Quant Time: Apr 02 23:57:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.565	1812746	13.944 ug/ml
Target Compounds			
4) N-TETRADECANE	8.174f	200676	1.411 ug/ml
12) N-OCTACOSANE	16.743	175618	1.221 ug/ml
13) N-TRIACONTANE	17.636	244982	1.715 ug/ml
14) N-DOTRIACONTANE	18.426	412430	2.922 ug/ml
15) N-TETRATRIACONTANE	19.219	646096	4.845 ug/ml
16) N-HEXATRIACONTANE	19.985	2240552	17.658 ug/ml
17) N-OCTATRIACONTANE	20.680	986243	8.664 ug/ml
18) N-TETRACONTANE	21.563	319084	2.631 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040219\
Data File : FF004065.D
Signal(s) : FID2B.ch
Acq On : 02 Apr 2019 18:31
Operator : AJ\SJ
Sample : K2186-21
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TP-TRACK-78-79

Integration File: autoint1.e
Quant Time: Apr 02 23:57:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

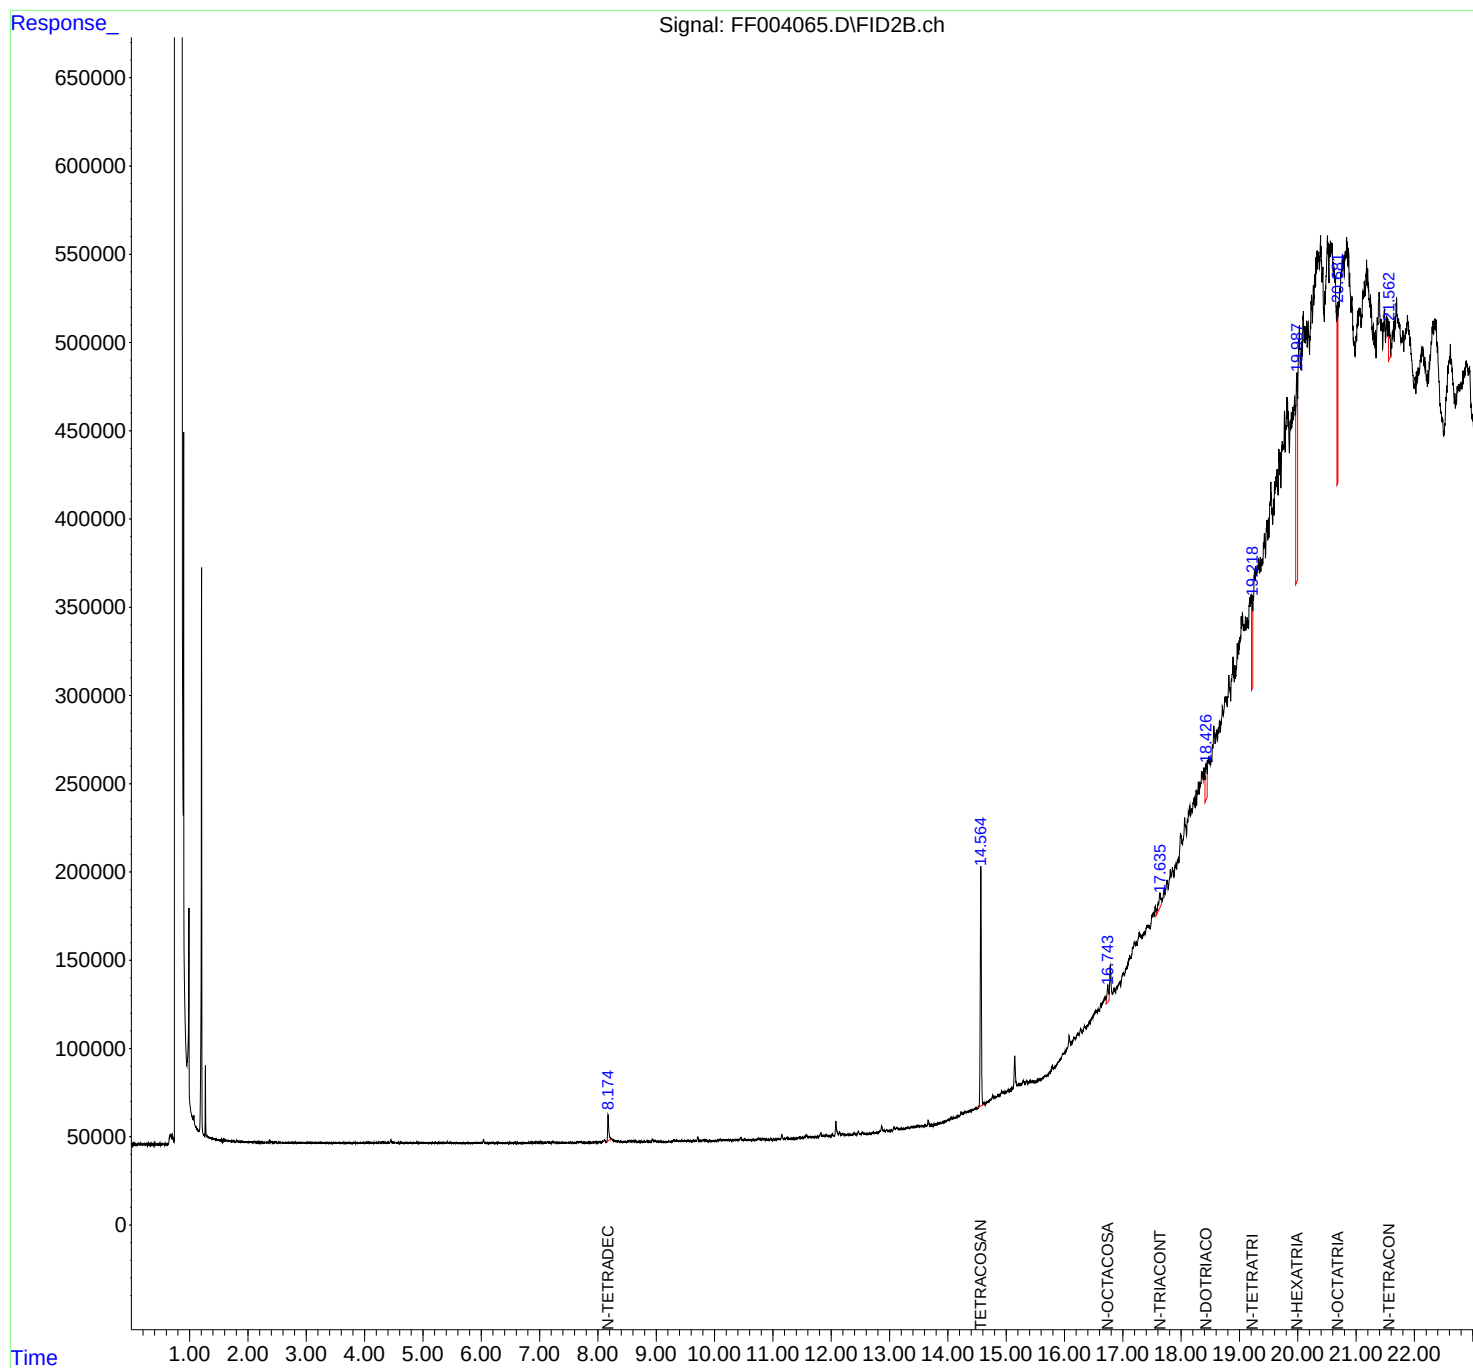


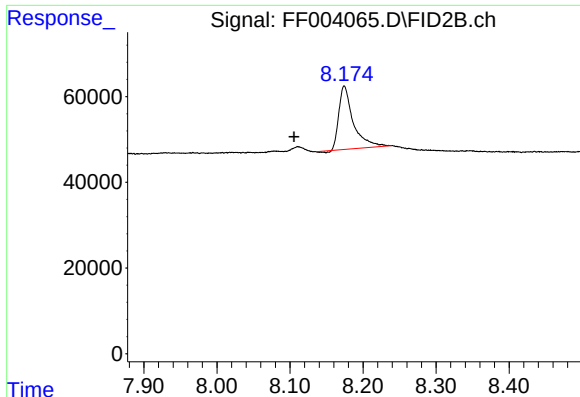

#4 N-TETRADECANE


R.T.: 8.174 min
Delta R.T.: 0.069 min
Response: 200676
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-TRACK-78-79

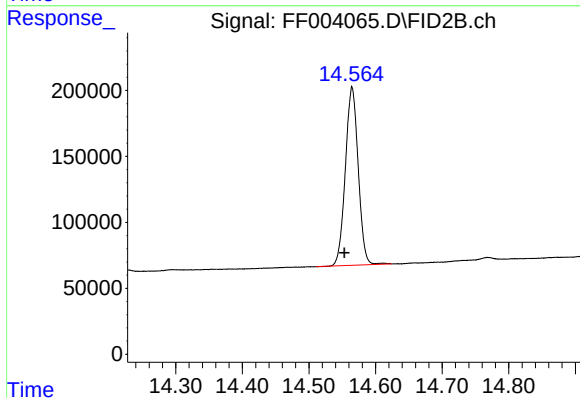


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.565 min
Delta R.T.: 0.011 min
Response: 1812746
Conc: 13.94 ug/ml

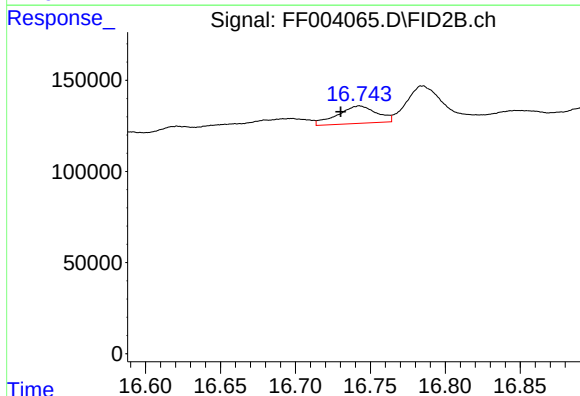


#12 N-OCTACOSANE

R.T.: 16.743 min
Delta R.T.: 0.013 min
Response: 175618
Conc: 1.22 ug/ml

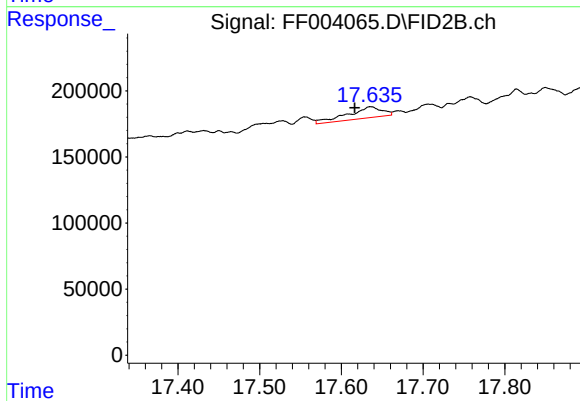

#13 N-TRIACONTANE


R.T.: 17.636 min
Delta R.T.: 0.019 min
Response: 244982
Conc: 1.72 ug/ml

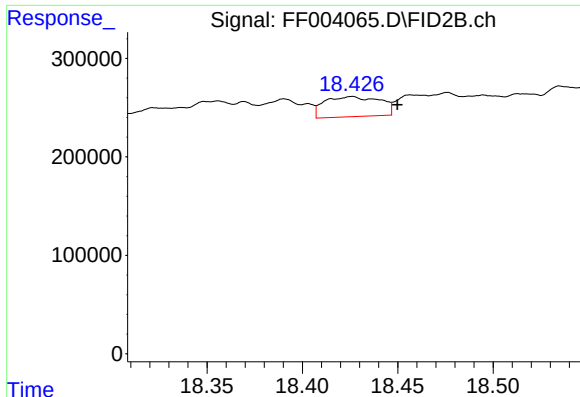

#14 N-DOTRIACONTANE


R.T.: 18.426 min
Delta R.T.: -0.024 min
Response: 412430
Conc: 2.92 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-TRACK-78-79

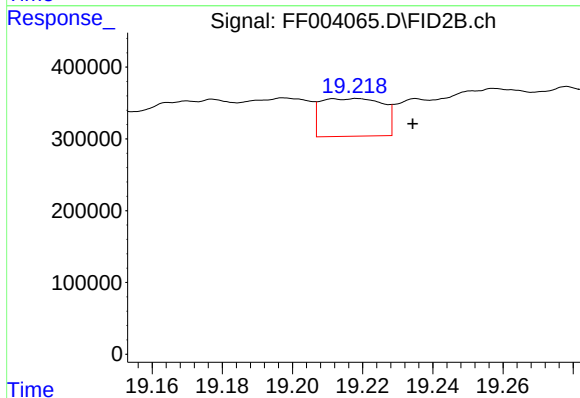


#15 N-TETRATRIACONTANE

R.T.: 19.219 min
Delta R.T.: -0.016 min
Response: 646096
Conc: 4.84 ug/ml

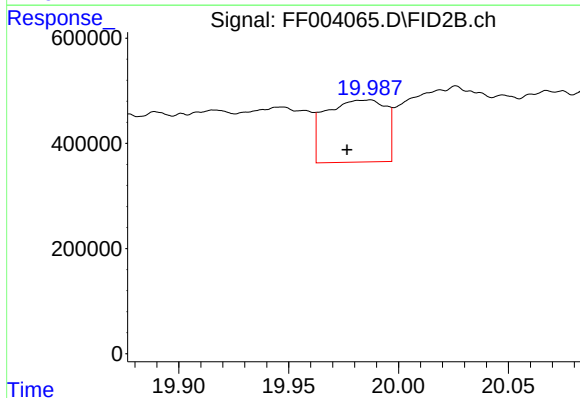


#16 N-HEXATRIACONTANE

R.T.: 19.985 min
Delta R.T.: 0.008 min
Response: 2240552
Conc: 17.66 ug/ml

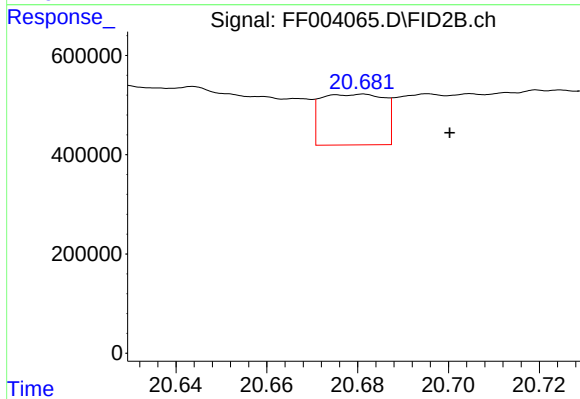

#17 N-OCTATRIACONTANE

R.T.: 20.680 min
Delta R.T.: -0.021 min
Response: 986243
Conc: 8.66 ug/ml

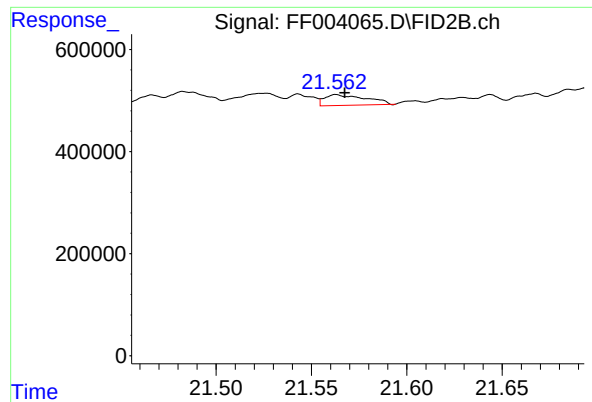

#18 N-TETRACONTANE

R.T.: 21.563 min
Delta R.T.: -0.004 min
Response: 319084
Conc: 2.63 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-TRACK-78-79