

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040219\
Data File : FF004072.D
Signal(s) : FID2B.ch
Acq On : 02 Apr 2019 22:38
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Apr 02 23:59:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.565	2091992	16.092 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.631	105590	0.739 ug/ml
15) N-TETRATRIACONTANE	19.248	36690	0.275 ug/ml
16) N-HEXATRIACONTANE	19.990	1058204	8.340 ug/ml
17) N-OCTATRIACONTANE	20.686	96292	0.846 ug/ml
18) N-TETRACONTANE	21.600	164158	1.353 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040219\
Data File : FF004072.D
Signal(s) : FID2B.ch
Acq On : 02 Apr 2019 22:38
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Apr 02 23:59:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

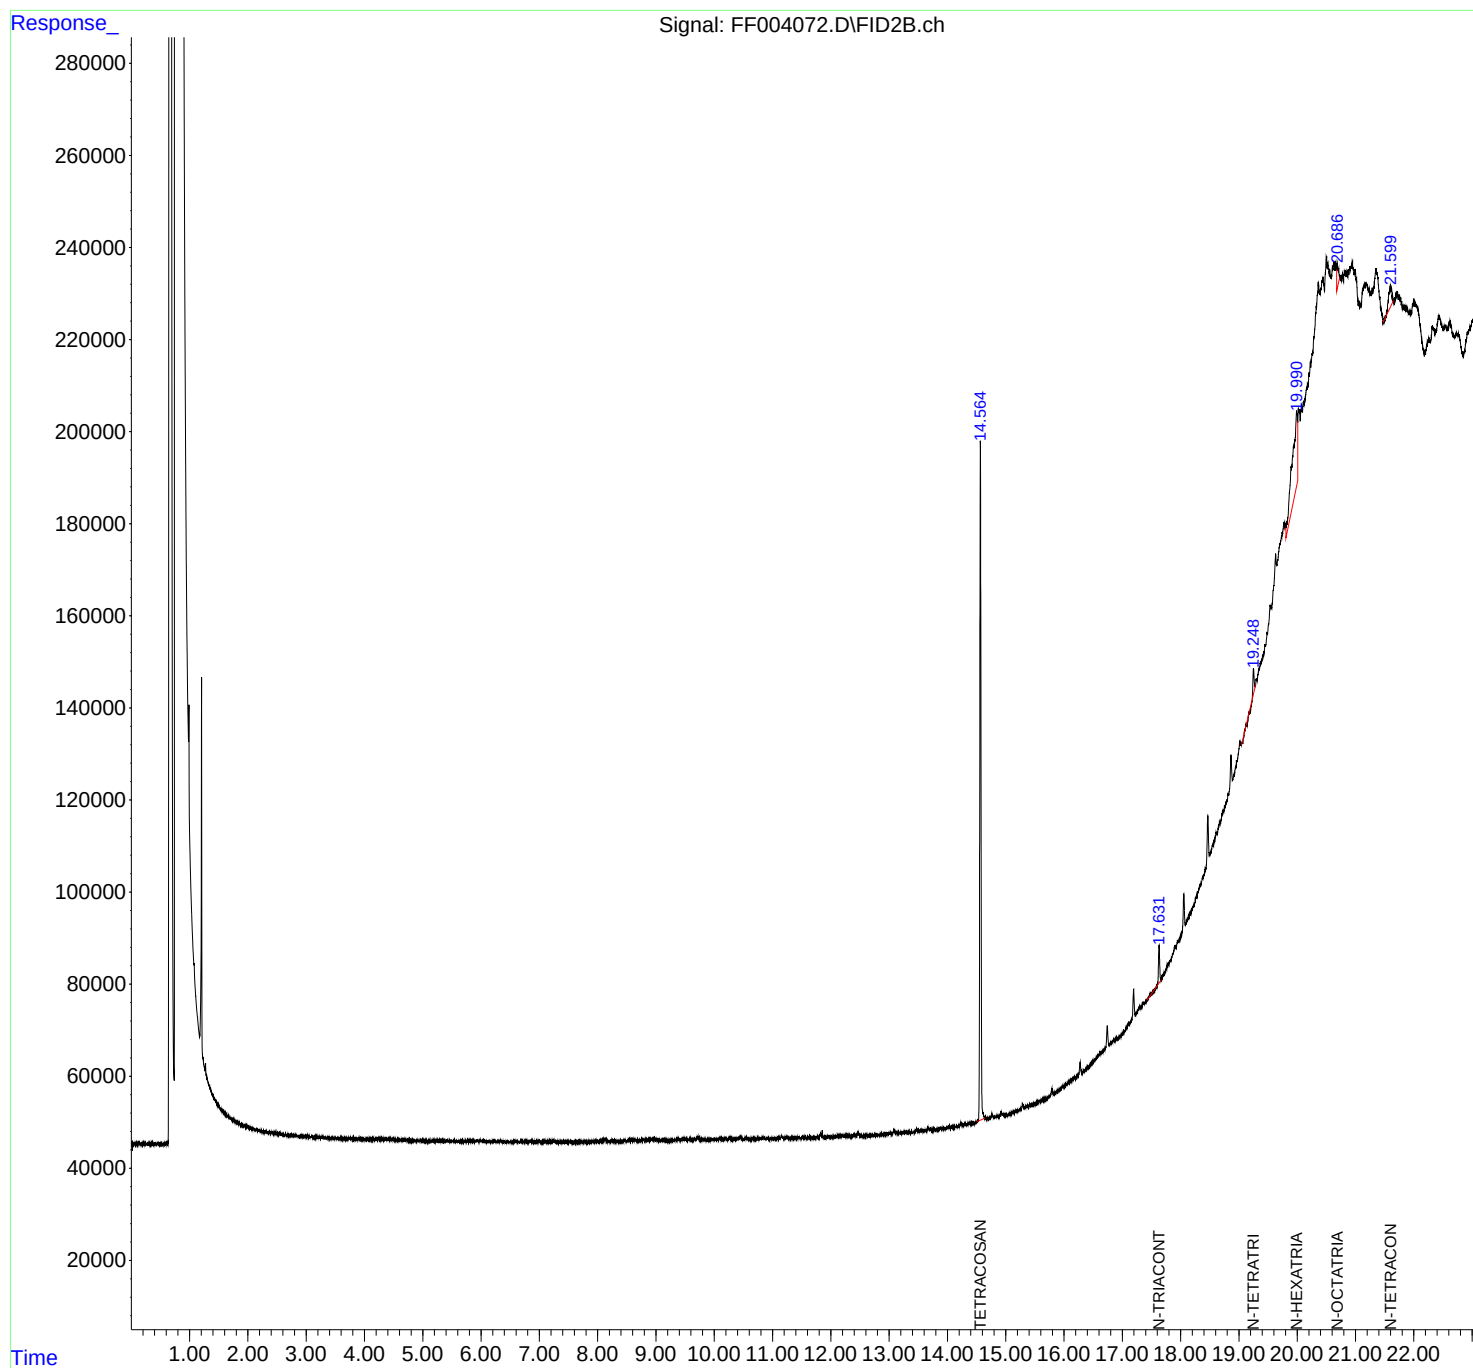


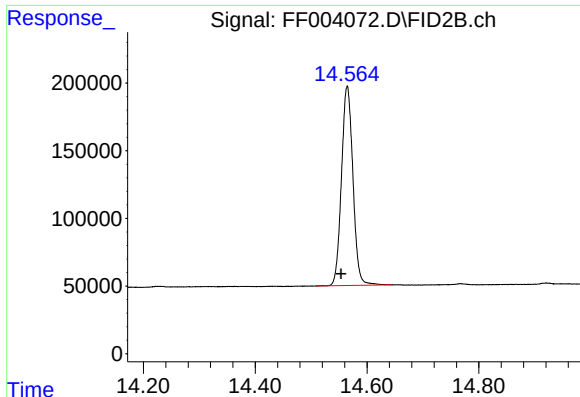

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.565 min
Delta R.T.: 0.011 min
Response: 2091992
Conc: 16.09 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

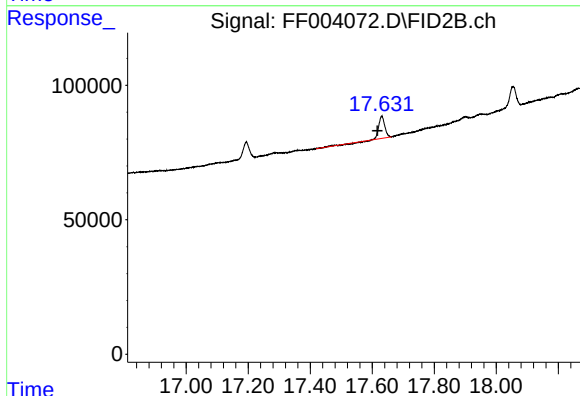


#13 N-TRIACONTANE

R.T.: 17.631 min
Delta R.T.: 0.014 min
Response: 105590
Conc: 0.74 ug/ml

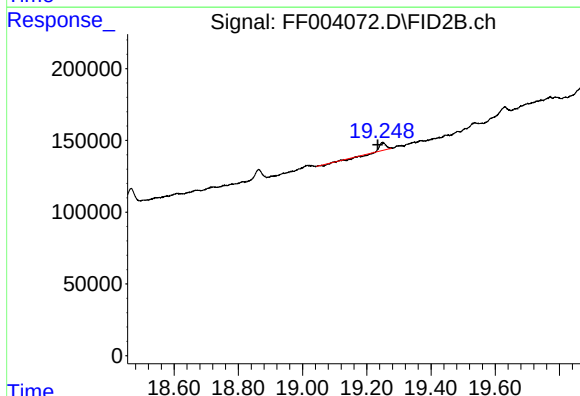


#15 N-TETRATRIACONTANE

R.T.: 19.248 min
Delta R.T.: 0.014 min
Response: 36690
Conc: 0.28 ug/ml

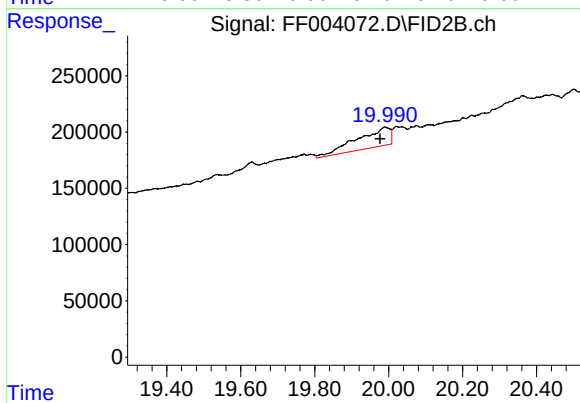

#16 N-HEXATRIACONTANE


R.T.: 19.990 min
Delta R.T.: 0.013 min
Response: 1058204
Conc: 8.34 ug/ml

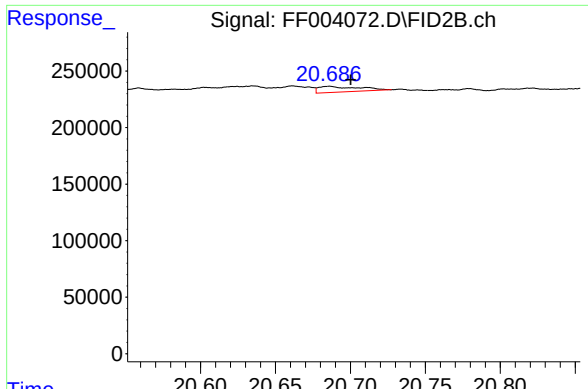

#17 N-OCTATRIACONTANE

R.T.: 20.686 min
Delta R.T.: -0.014 min
Response: 96292
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

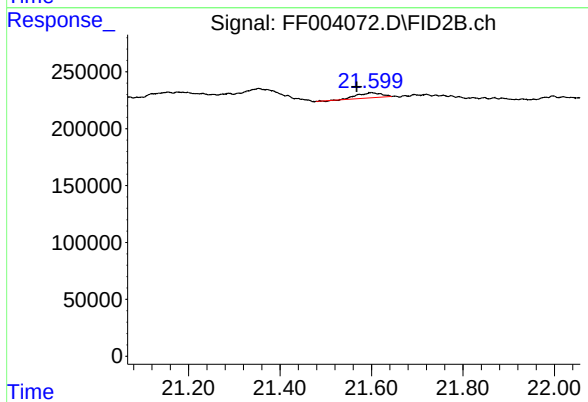

#18 N-TETRACONTANE

R.T.: 21.600 min
Delta R.T.: 0.033 min
Response: 164158
Conc: 1.35 ug/ml