

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
Data File : FF006726.D
Signal(s) : FID2B.ch
Acq On : 02 Apr 2020 10:19
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 02 17:48:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.586	2372375	18.433 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.634	179900	1.271 ug/ml
14)	N-DOTRIACONTANE	18.462	234749	1.742 ug/ml
15)	N-TETRATRIACONTANE	19.243	175188	1.551 ug/ml
16)	N-HEXATRIACONTANE	19.980	211021	2.298 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
Data File : FF006726.D
Signal(s) : FID2B.ch
Acq On : 02 Apr 2020 10:19
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 02 17:48:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

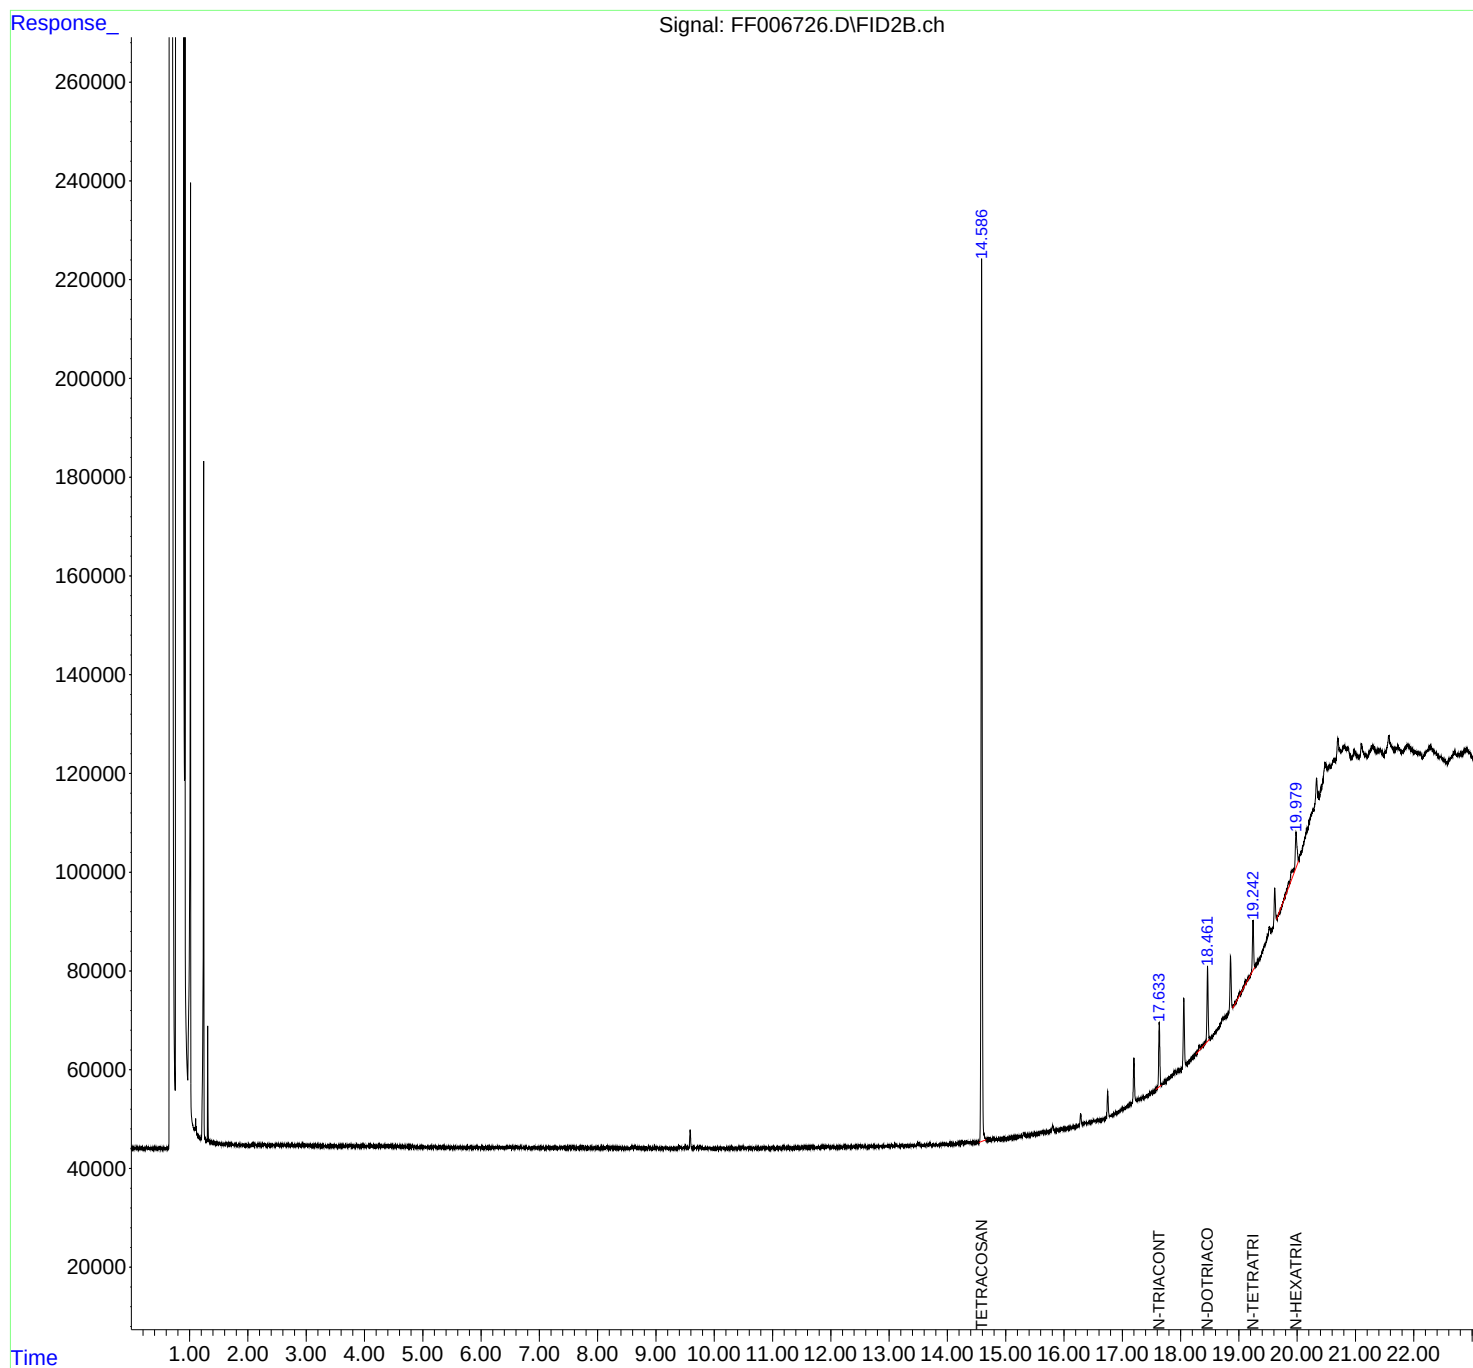

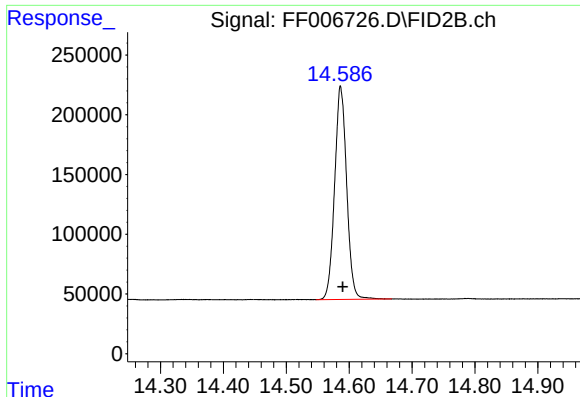


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.586 min
Delta R.T.: -0.003 min
Response: 2372375
Conc: 18.43 ug/ml

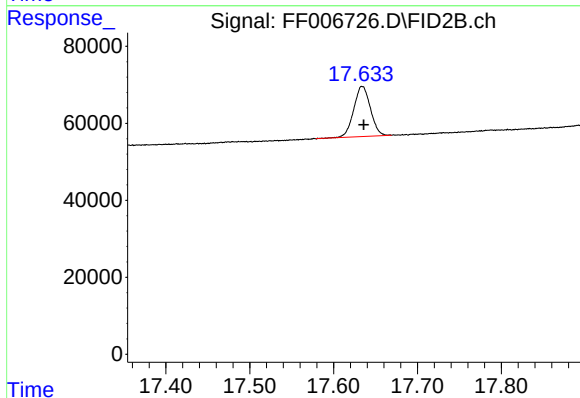


#13 N-TRIACONTANE

R.T.: 17.634 min
Delta R.T.: -0.002 min
Response: 179900
Conc: 1.27 ug/ml

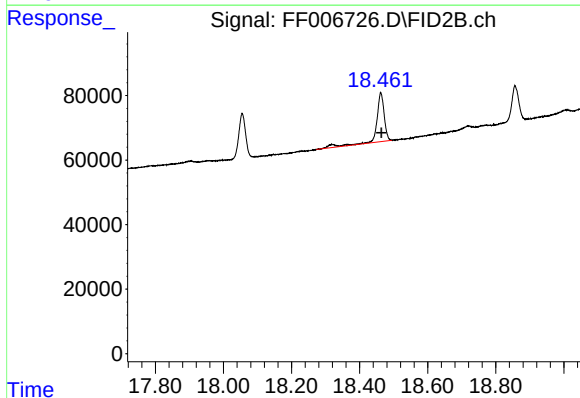


#14 N-DOTRIACONTANE

R.T.: 18.462 min
Delta R.T.: -0.002 min
Response: 234749
Conc: 1.74 ug/ml

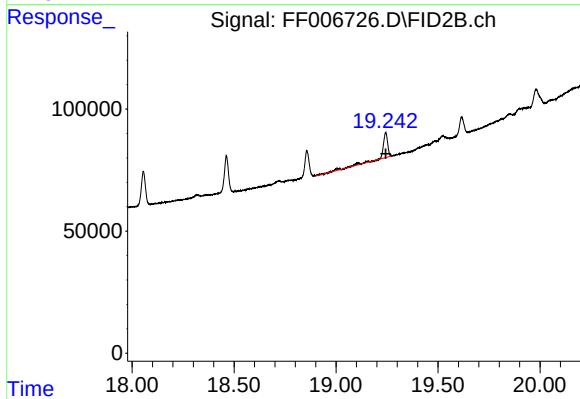

#15 N-TETRATRIACONTANE

R.T.: 19.243 min
Delta R.T.: 0.000 min
Response: 175188
Conc: 1.55 ug/ml

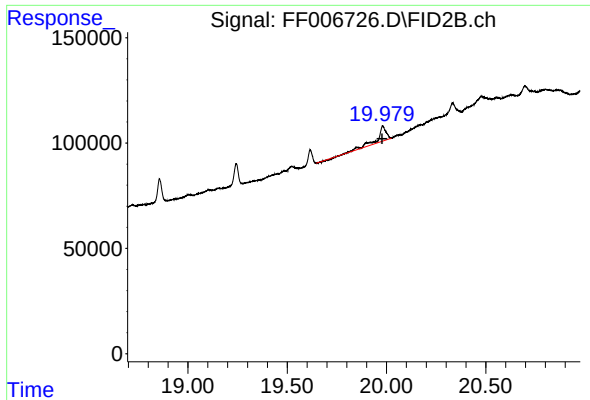

#16 N-HEXATRIACONTANE

R.T.: 19.980 min
Delta R.T.: 0.002 min
Response: 211021
Conc: 2.30 ug/ml