

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
 Data File : FF006749.D
 Signal(s) : FID2B.ch
 Acq On : 03 Apr 2020 02:38
 Operator : DD\AJ
 Sample : L2129-33
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 03 07:39:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.580	3565901	27.707 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.151	101722	0.711 ug/ml
5)	N-HEXADECANE	9.748	222217	1.516 ug/ml
6)	N-OCTADECANE	11.183	168695	1.142 ug/ml
7)	N-EICOSANE	12.484	505748	3.403 ug/ml
8)	N-DOCOSANE	13.683	374746	2.523 ug/ml
10)	N-TETRACOSANE	14.774	1865034	12.619 ug/ml
11)	N-HEXACOSANE	15.798	355338	2.452 ug/ml
12)	N-OCTACOSANE	16.746	550313	3.842 ug/ml
13)	N-TRIACONTANE	17.629	767913	5.426 ug/ml
14)	N-DOTRIACONTANE	18.455	700372	5.196 ug/ml
15)	N-TETRATRIACONTANE	19.236	255917	2.266 ug/ml
16)	N-HEXATRIACONTANE	19.972	193417	2.106 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
Data File : FF006749.D
Signal(s) : FID2B.ch
Acq On : 03 Apr 2020 02:38
Operator : DD\AJ
Sample : L2129-33
Misc :
ALS Vial : 73 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 03 07:39:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

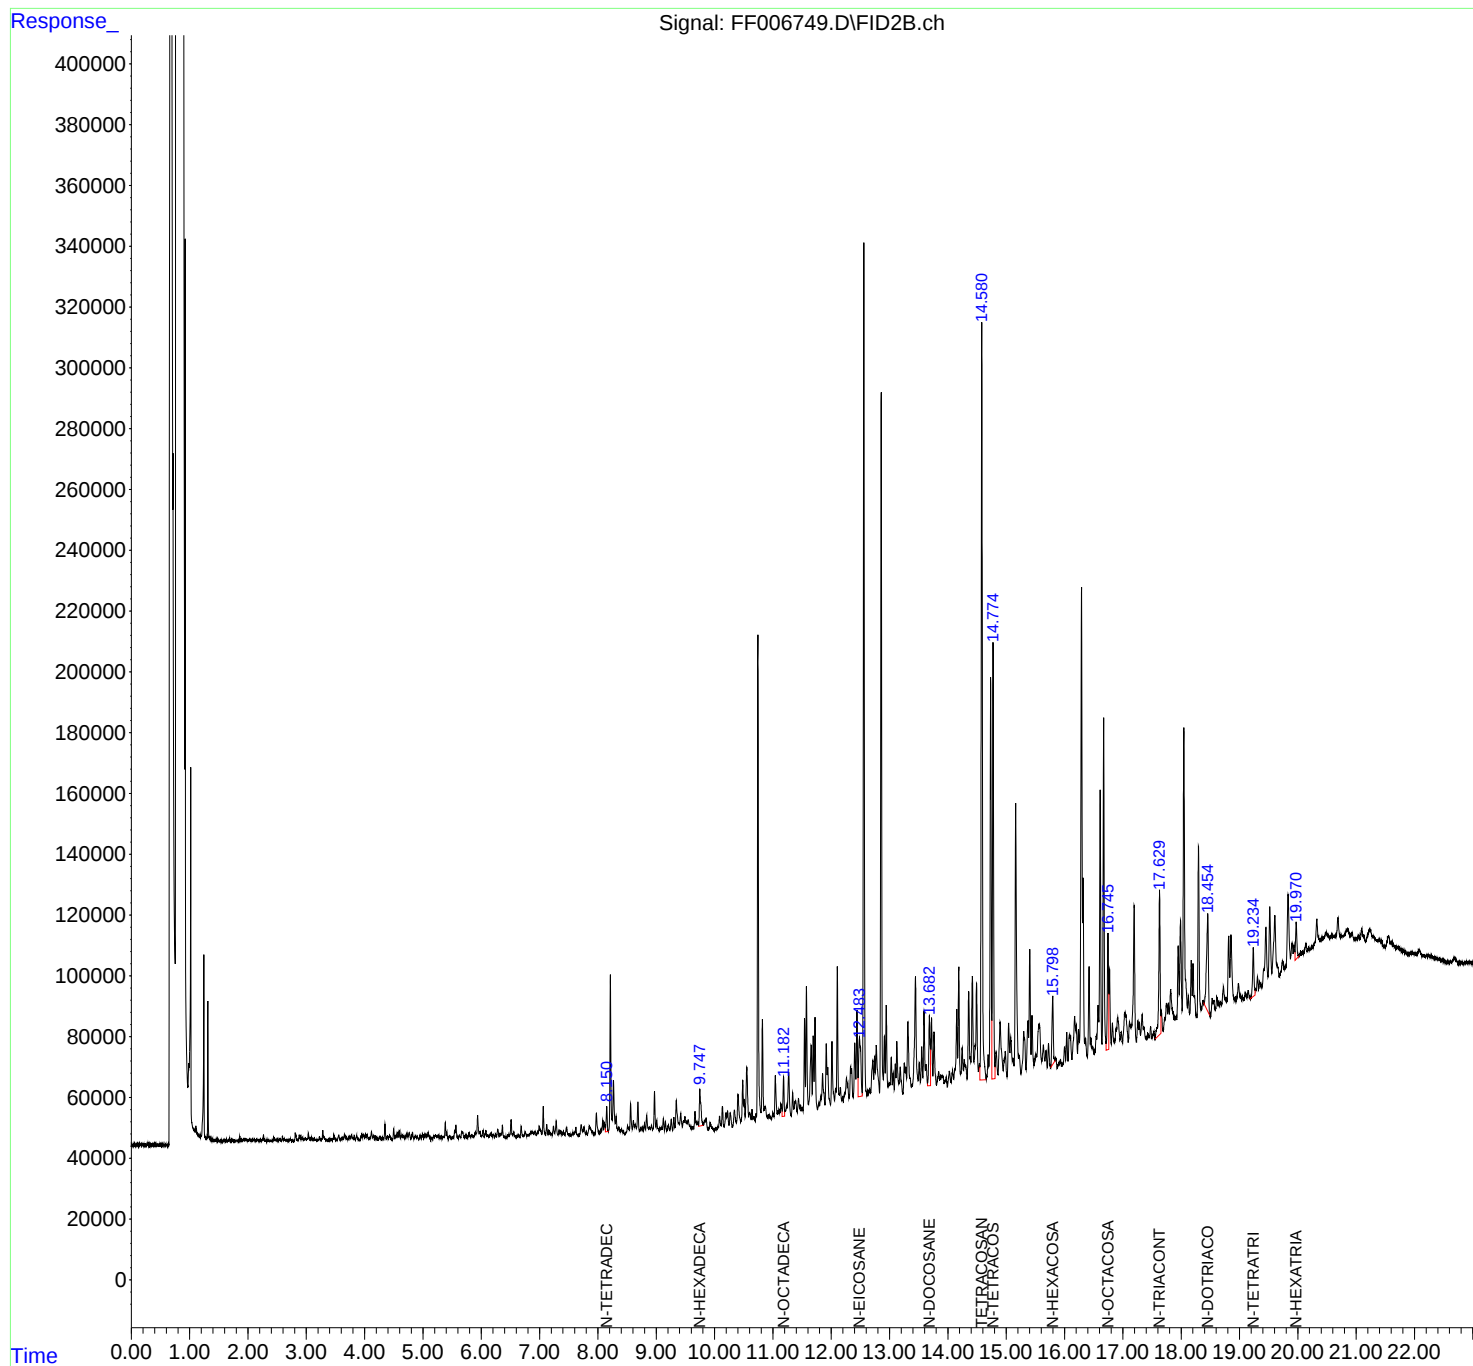

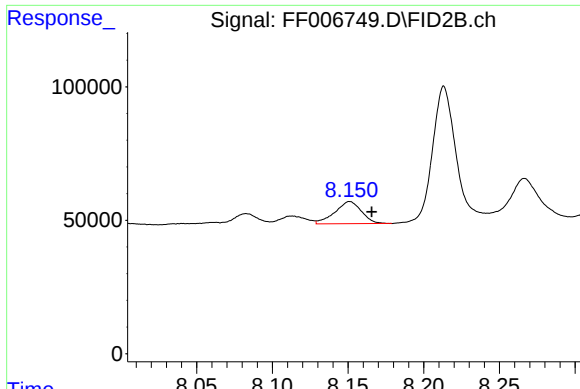


#4 N-TETRADECANE

R.T.: 8.151 min
Delta R.T.: -0.014 min
Response: 101722
Conc: 0.71 ug/ml

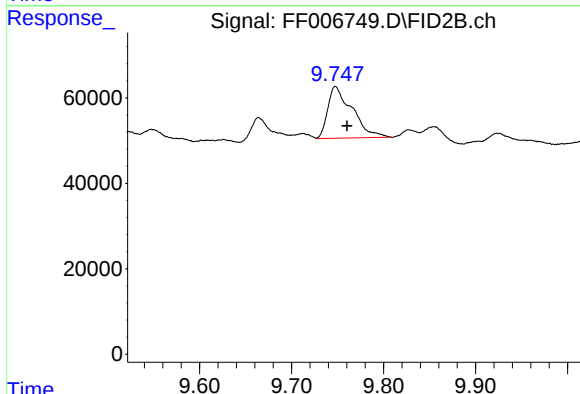


#5 N-HEXADECANE

R.T.: 9.748 min
Delta R.T.: -0.012 min
Response: 222217
Conc: 1.52 ug/ml

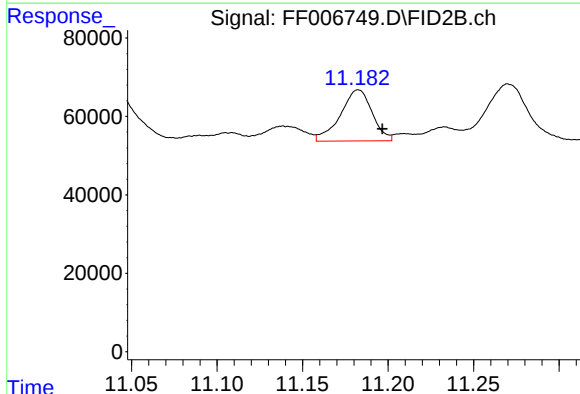


#6 N-OCTADECANE

R.T.: 11.183 min
Delta R.T.: -0.014 min
Response: 168695
Conc: 1.14 ug/ml

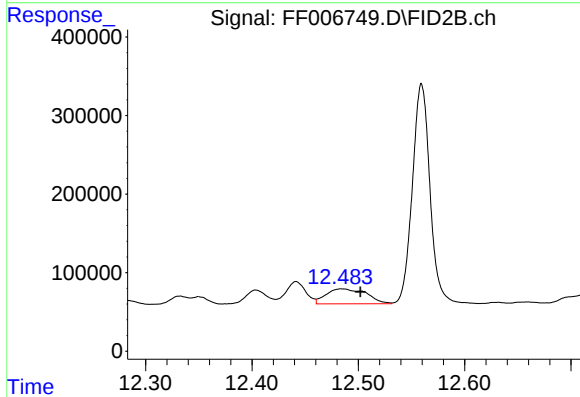


#7 N-EICOSANE

R.T.: 12.484 min
Delta R.T.: -0.018 min
Response: 505748
Conc: 3.40 ug/ml

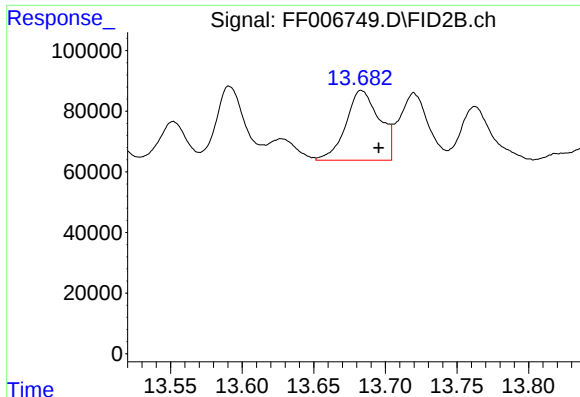


#8 N-DOCOSANE

R.T.: 13.683 min
Delta R.T.: -0.012 min
Response: 374746
Conc: 2.52 ug/ml

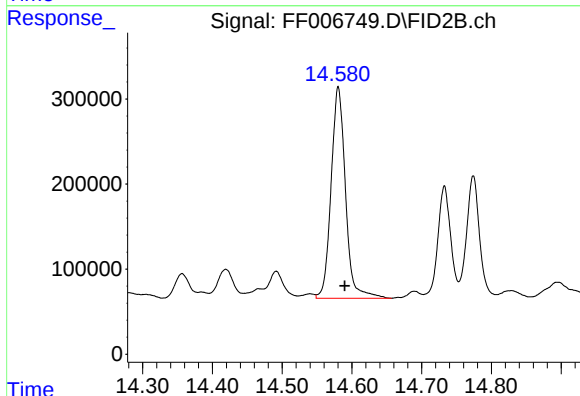


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.580 min
Delta R.T.: -0.009 min
Response: 3565901
Conc: 27.71 ug/ml

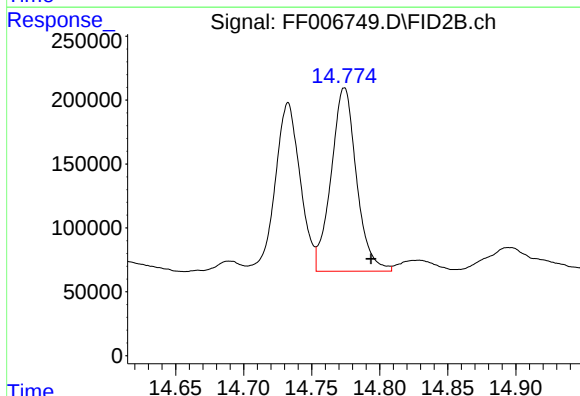


#10 N-TETRACOSANE

R.T.: 14.774 min
Delta R.T.: -0.019 min
Response: 1865034
Conc: 12.62 ug/ml

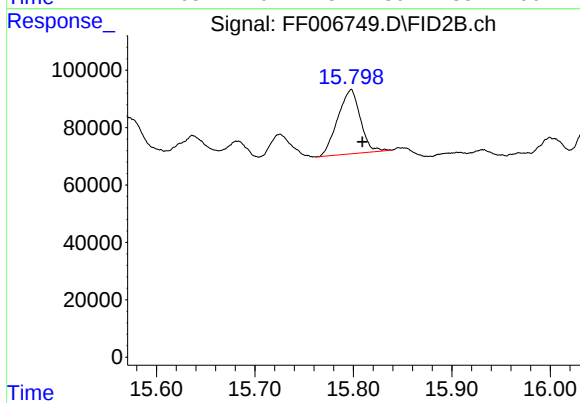


#11 N-HEXACOSANE

R.T.: 15.798 min
Delta R.T.: -0.011 min
Response: 355338
Conc: 2.45 ug/ml

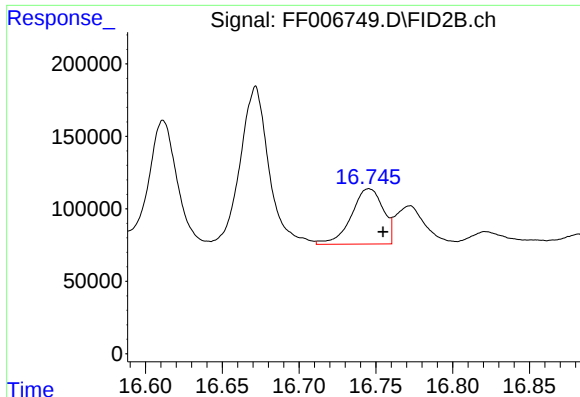


#12 N-OCTACOSANE

R.T.: 16.746 min
Delta R.T.: -0.009 min
Response: 550313
Conc: 3.84 ug/ml

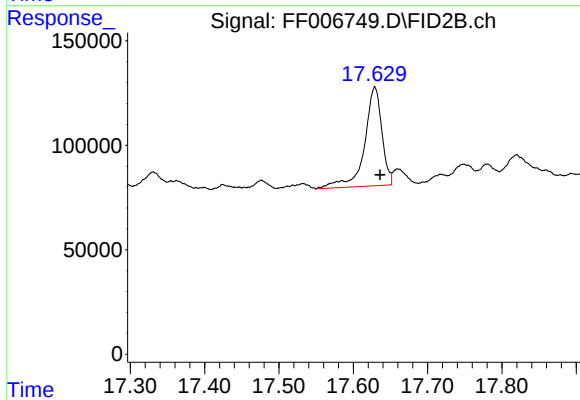


#13 N-TRIACONTANE

R.T.: 17.629 min
Delta R.T.: -0.007 min
Response: 767913
Conc: 5.43 ug/ml

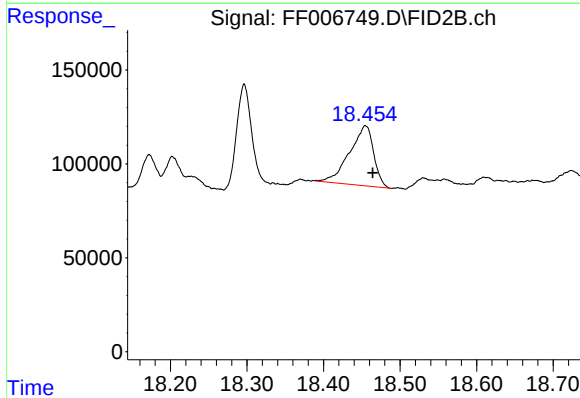


#14 N-DOTRIACONTANE

R.T.: 18.455 min
Delta R.T.: -0.009 min
Response: 700372
Conc: 5.20 ug/ml

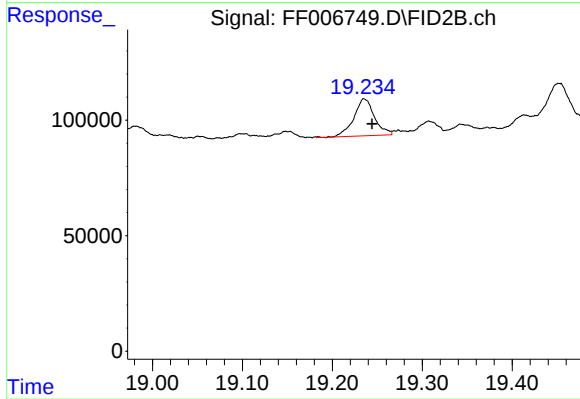

#15 N-TETRATRIACONTANE

R.T.: 19.236 min
Delta R.T.: -0.009 min
Response: 255917
Conc: 2.27 ug/ml

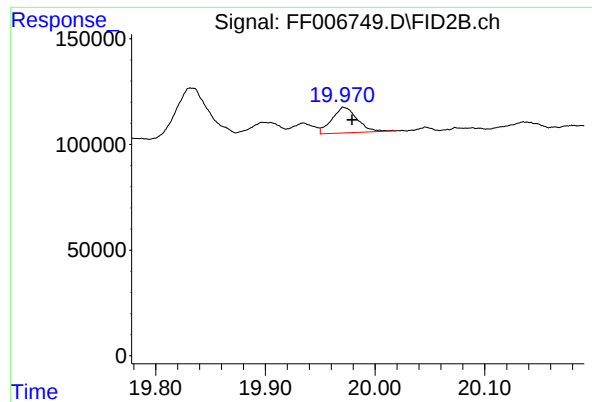

#16 N-HEXATRIACONTANE

R.T.: 19.972 min
Delta R.T.: -0.007 min
Response: 193417
Conc: 2.11 ug/ml