

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
 Data File : FF006754.D
 Signal(s) : FID2B.ch
 Acq On : 03 Apr 2020 05:10
 Operator : DD\AJ
 Sample : L2129-12 5X
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 03 07:40:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.581	1212212	9.419 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.215	219638	1.536 ug/ml
5)	N-HEXADECANE	9.765	1896043	12.935 ug/ml
6)	N-OCTADECANE	11.178	333718	2.258 ug/ml
7)	N-EICOSANE	12.512	1169252	7.867 ug/ml
8)	N-DOCOSANE	13.686	1185776	7.984 ug/ml
10)	N-TETRACOSANE	14.785	6634928	44.893 ug/ml
11)	N-HEXACOSANE	15.788	984759	6.795 ug/ml
12)	N-OCTACOSANE	16.748	290220	2.026 ug/ml
13)	N-TRIACONTANE	17.629	502562	3.551 ug/ml
14)	N-DOTRIACONTANE	18.435	1172920	8.701 ug/ml
15)	N-TETRATRIACONTANE	19.236	158350	1.402 ug/ml
16)	N-HEXATRIACONTANE	19.974	188136	2.048 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
Data File : FF006754.D
Signal(s) : FID2B.ch
Acq On : 03 Apr 2020 05:10
Operator : DD\AJ
Sample : L2129-12 5X
Misc :
ALS Vial : 76 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 03 07:40:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

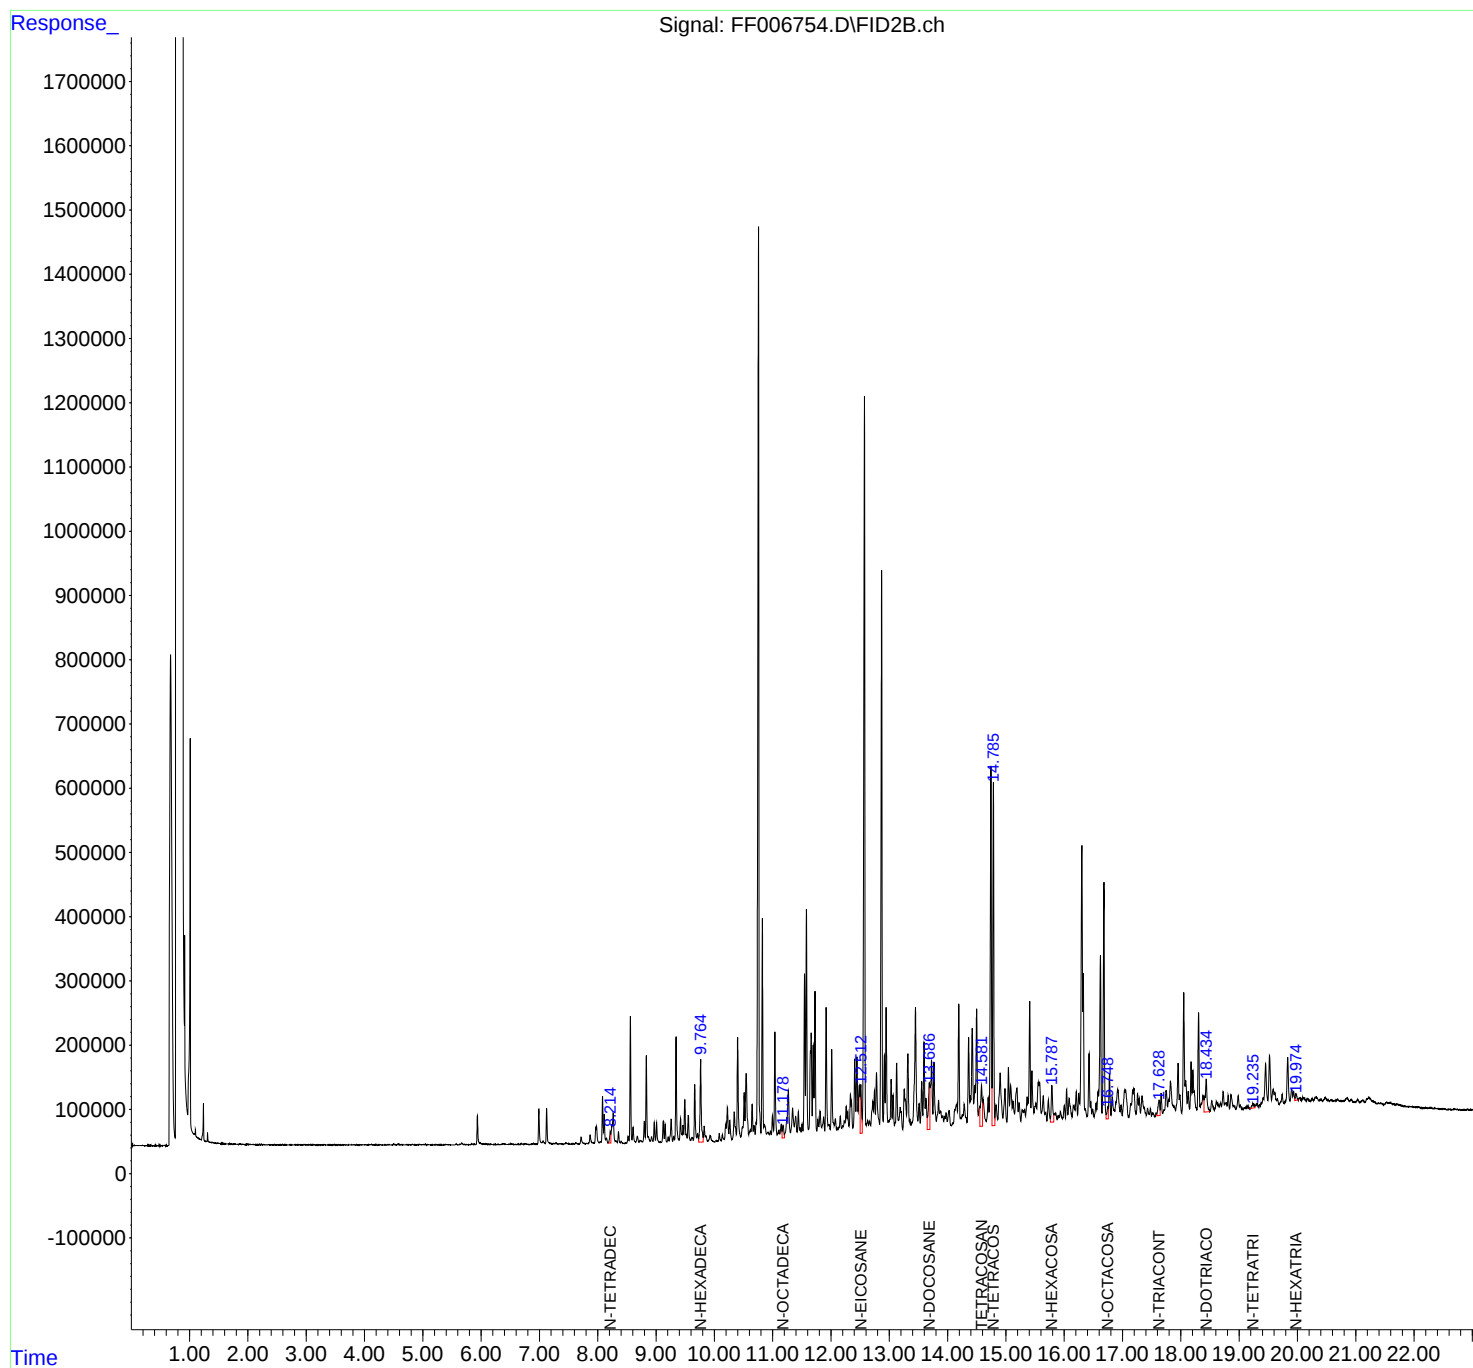

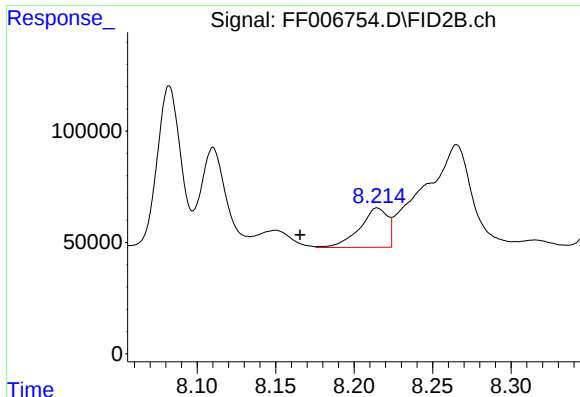


#4 N-TETRADECANE

R.T.: 8.215 min
Delta R.T.: 0.049 min
Response: 219638
Conc: 1.54 ug/ml

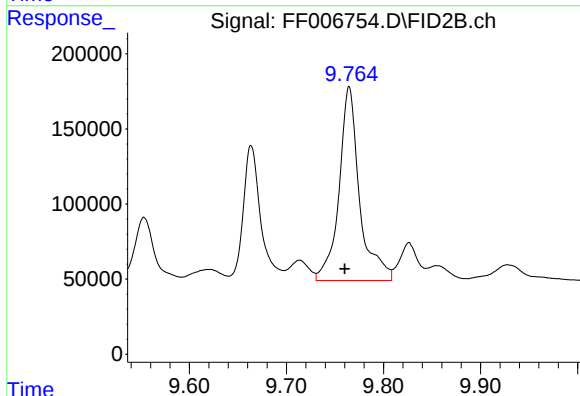


#5 N-HEXADECANE

R.T.: 9.765 min
Delta R.T.: 0.005 min
Response: 1896043
Conc: 12.93 ug/ml

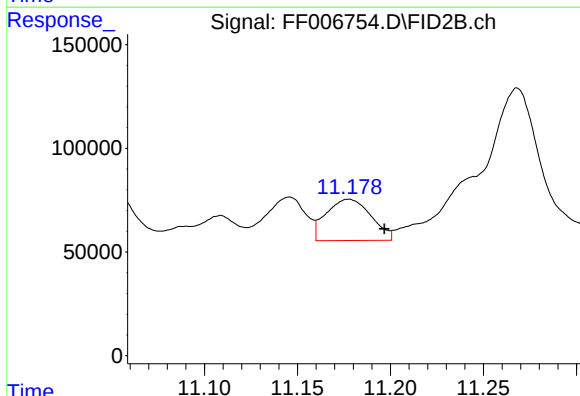


#6 N-OCTADECANE

R.T.: 11.178 min
Delta R.T.: -0.019 min
Response: 333718
Conc: 2.26 ug/ml

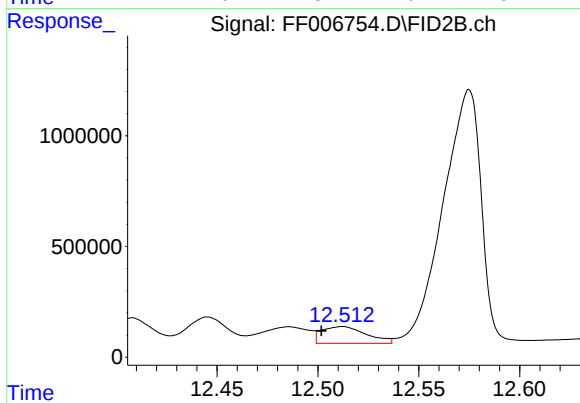


#7 N-EICOSANE

R.T.: 12.512 min
Delta R.T.: 0.010 min
Response: 1169252
Conc: 7.87 ug/ml

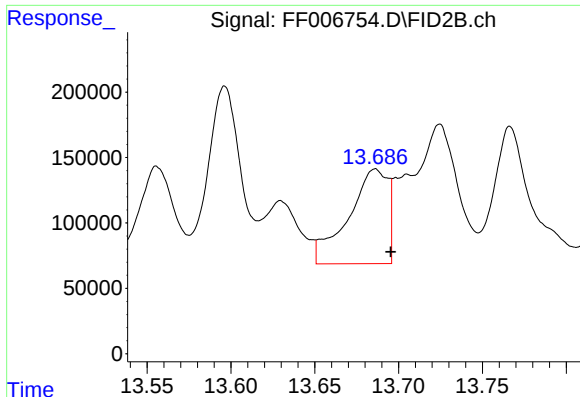


#8 N-DOCOSANE

R.T.: 13.686 min
Delta R.T.: -0.009 min
Response: 1185776
Conc: 7.98 ug/ml

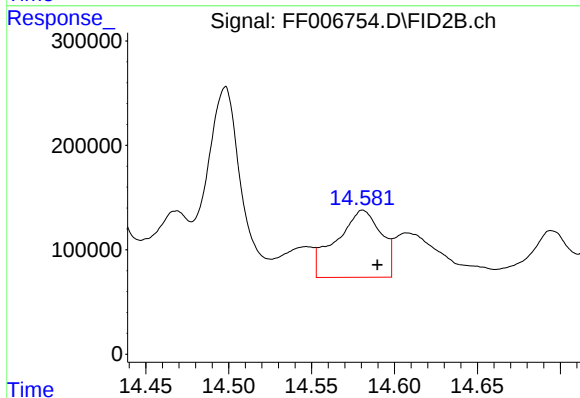


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.581 min
Delta R.T.: -0.009 min
Response: 1212212
Conc: 9.42 ug/ml

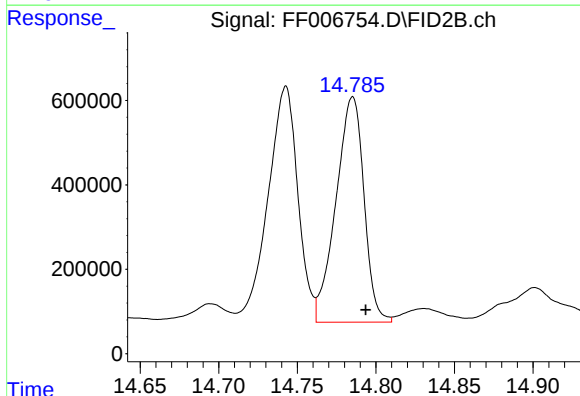


#10 N-TETRACOSANE

R.T.: 14.785 min
Delta R.T.: -0.008 min
Response: 6634928
Conc: 44.89 ug/ml

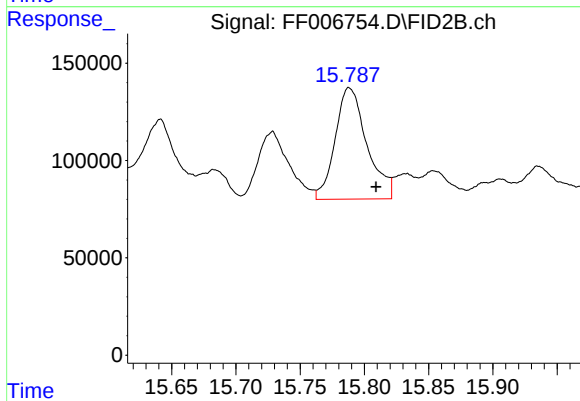


#11 N-HEXACOSANE

R.T.: 15.788 min
Delta R.T.: -0.021 min
Response: 984759
Conc: 6.80 ug/ml

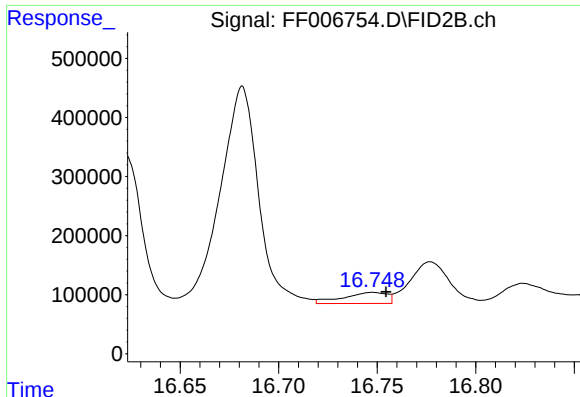


#12 N-OCTACOSANE

R.T.: 16.748 min
Delta R.T.: -0.007 min
Response: 290220
Conc: 2.03 ug/ml

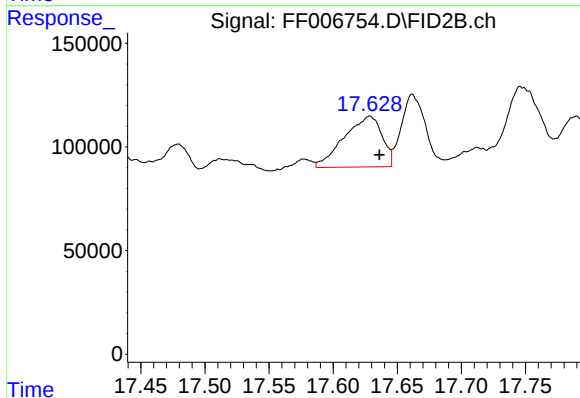


#13 N-TRIACONTANE

R.T.: 17.629 min
Delta R.T.: -0.007 min
Response: 502562
Conc: 3.55 ug/ml

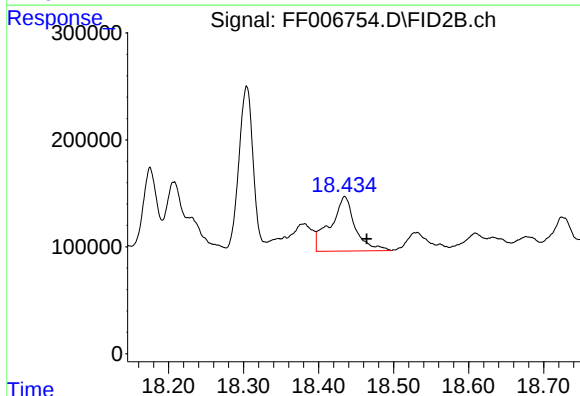


#14 N-DOTRIACONTANE

R.T.: 18.435 min
Delta R.T.: -0.029 min
Response: 1172920
Conc: 8.70 ug/ml

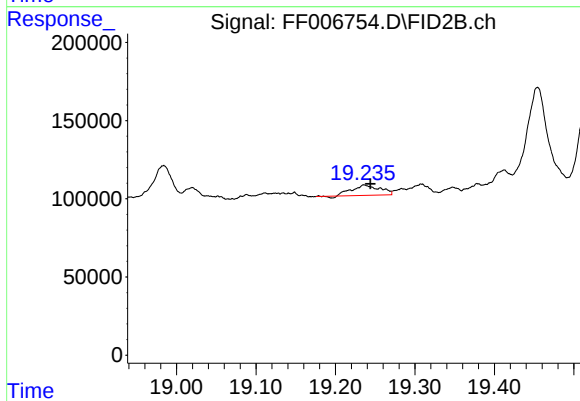

#15 N-TETRATRIACONTANE

R.T.: 19.236 min
Delta R.T.: -0.008 min
Response: 158350
Conc: 1.40 ug/ml

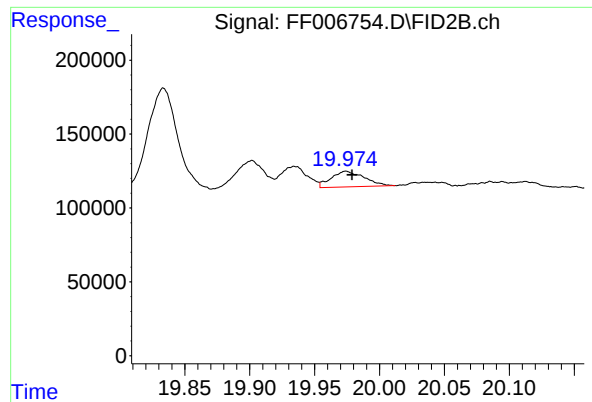

#16 N-HEXATRIACONTANE

R.T.: 19.974 min
Delta R.T.: -0.005 min
Response: 188136
Conc: 2.05 ug/ml