

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
 Data File : FF006760.D
 Signal(s) : FID2B.ch
 Acq On : 03 Apr 2020 08:12
 Operator : DD\AJ
 Sample : L2129-03 10X
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 03 08:50:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.578	490073	3.808 ug/ml
Target Compounds			
5) N-HEXADECANE	9.764	159735	1.090 ug/ml
7) N-EICOSANE	12.508	428827	2.885 ug/ml
8) N-DOCOSANE	13.683	462892	3.117 ug/ml
10) N-TETRACOSANE	14.780	6000020	40.597 ug/ml
11) N-HEXACOSANE	15.786	512885	3.539 ug/ml
12) N-OCTACOSANE	16.772	1811790	12.650 ug/ml
13) N-TRIACONTANE	17.627	268477	1.897 ug/ml
14) N-DOTRIACONTANE	18.431	1216363	9.024 ug/ml
15) N-TETRATRIACONTANE	19.305f	118616	1.050 ug/ml
16) N-HEXATRIACONTANE	19.970	343903	3.745 ug/ml
18) N-TETRACONTANE	21.591	102009	1.474 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
Data File : FF006760.D
Signal(s) : FID2B.ch
Acq On : 03 Apr 2020 08:12
Operator : DD\AJ
Sample : L2129-03 10X
Misc :
ALS Vial : 82 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 03 08:50:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

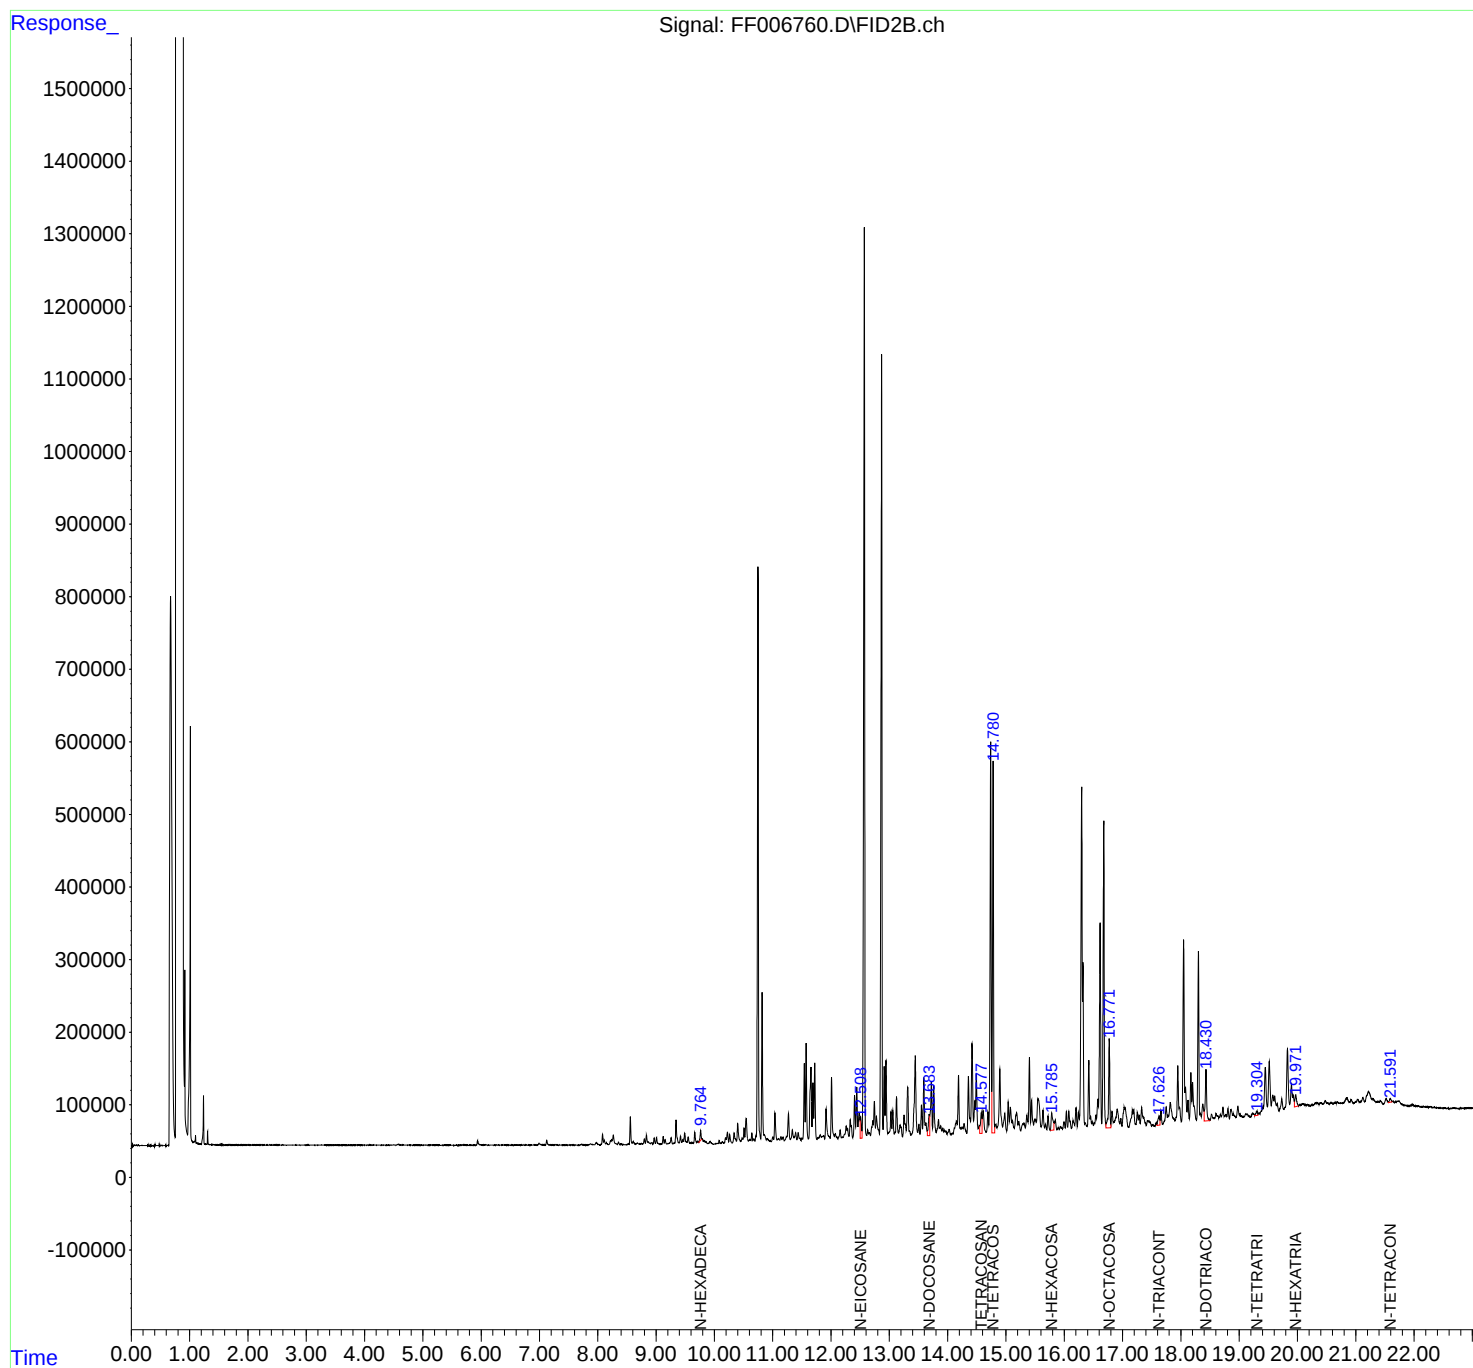

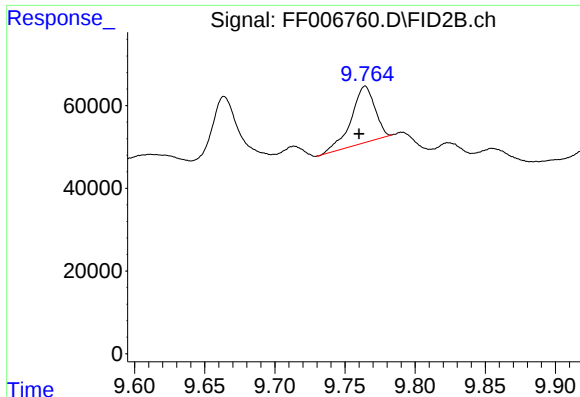


#5 N-HEXADECANE

R.T.: 9.764 min
Delta R.T.: 0.004 min
Response: 159735
Conc: 1.09 ug/ml

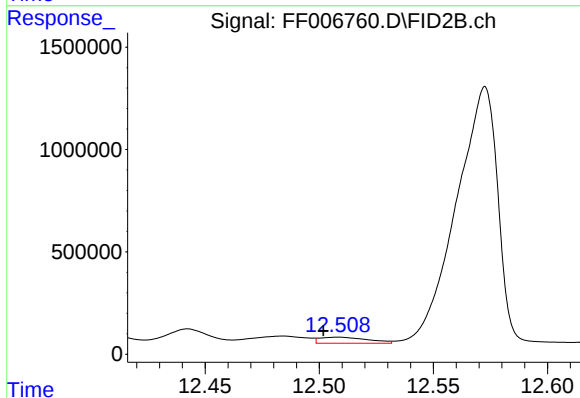


#7 N-EICOSANE

R.T.: 12.508 min
Delta R.T.: 0.007 min
Response: 428827
Conc: 2.89 ug/ml

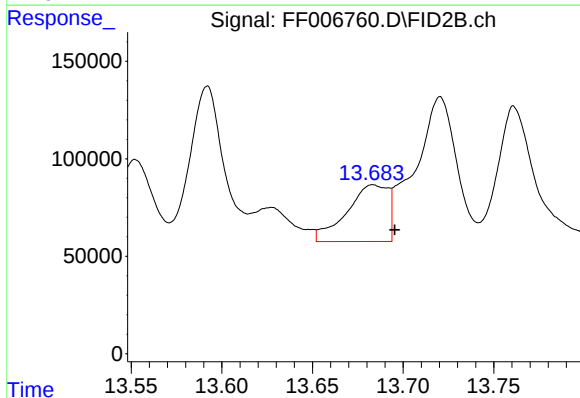


#8 N-DOCOSANE

R.T.: 13.683 min
Delta R.T.: -0.012 min
Response: 462892
Conc: 3.12 ug/ml

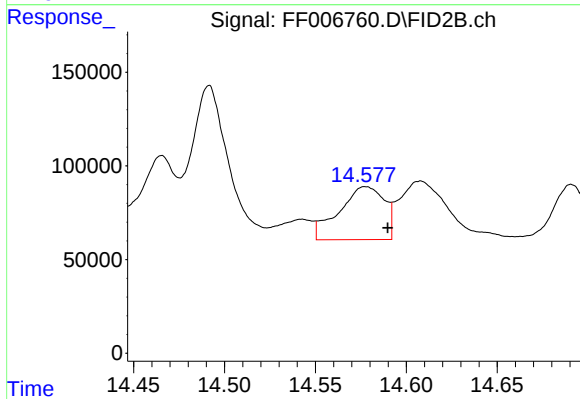


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.578 min
Delta R.T.: -0.012 min
Response: 490073
Conc: 3.81 ug/ml

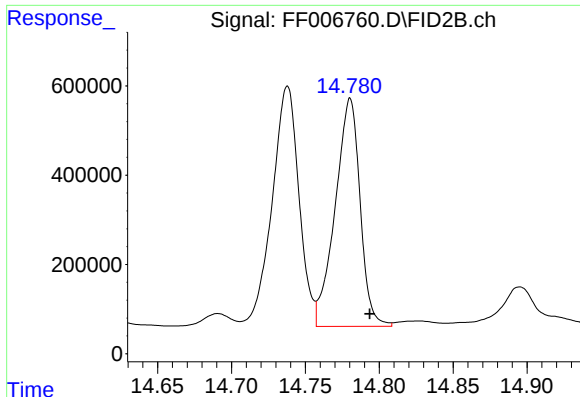


#10 N-TETRACOSANE

R.T.: 14.780 min
Delta R.T.: -0.013 min
Response: 6000020
Conc: 40.60 ug/ml

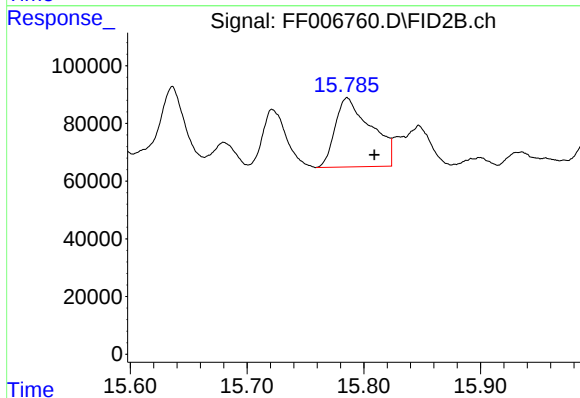


#11 N-HEXACOSANE

R.T.: 15.786 min
Delta R.T.: -0.023 min
Response: 512885
Conc: 3.54 ug/ml

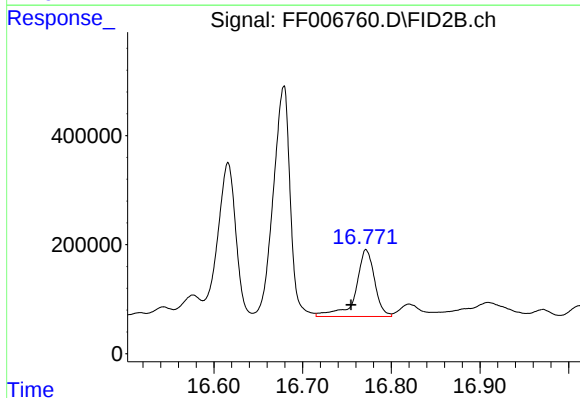


#12 N-OCTACOSANE

R.T.: 16.772 min
Delta R.T.: 0.017 min
Response: 1811790
Conc: 12.65 ug/ml

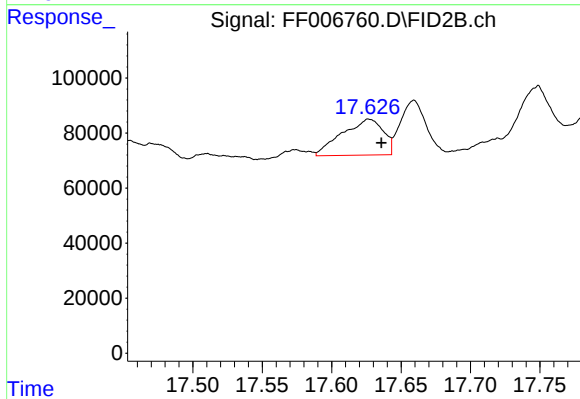


#13 N-TRIACONTANE

R.T.: 17.627 min
Delta R.T.: -0.009 min
Response: 268477
Conc: 1.90 ug/ml

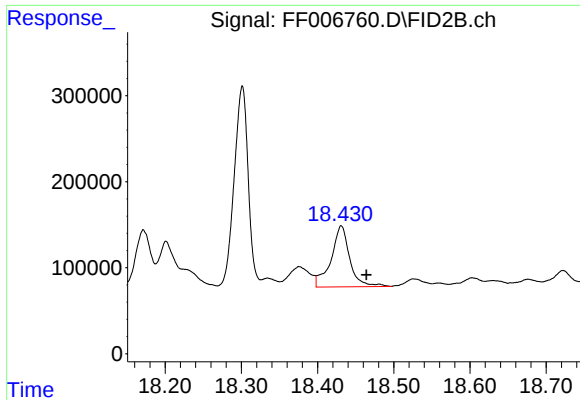


#14 N-DOTRIACONTANE

R.T.: 18.431 min
Delta R.T.: -0.033 min
Response: 1216363
Conc: 9.02 ug/ml

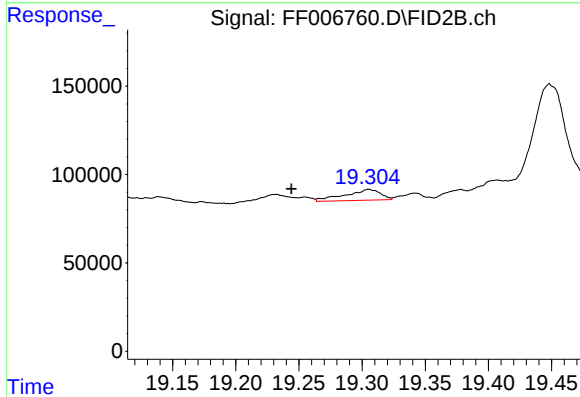


#15 N-TETRATRIACONTANE

R.T.: 19.305 min
Delta R.T.: 0.061 min
Response: 118616
Conc: 1.05 ug/ml

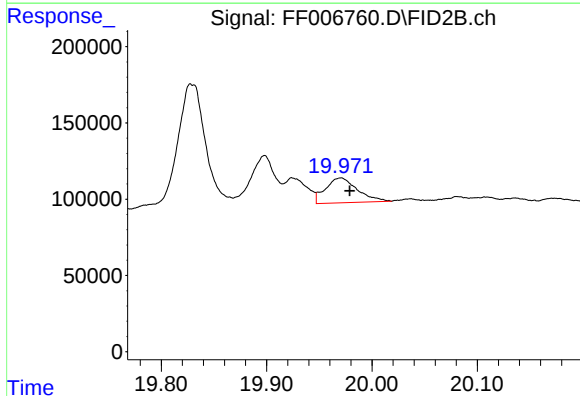

#16 N-HEXATRIACONTANE

R.T.: 19.970 min
Delta R.T.: -0.008 min
Response: 343903
Conc: 3.74 ug/ml

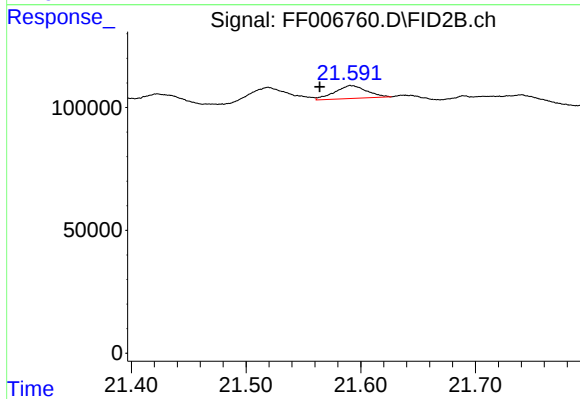

#18 N-TETRACONTANE

R.T.: 21.591 min
Delta R.T.: 0.027 min
Response: 102009
Conc: 1.47 ug/ml