

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
 Data File : FF006730.D
 Signal(s) : FID2B.ch
 Acq On : 02 Apr 2020 14:38
 Operator : DD\AJ
 Sample : PB127957BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 02 17:49:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.586	2920852	22.695 ug/ml
Target Compounds			
2) N-DECANE	4.352	3502762	25.447 ug/ml
3) N-DODECANE	6.367	3571046	25.319 ug/ml
4) N-TETRADECANE	8.156	3556825	24.870 ug/ml
5) N-HEXADECANE	9.752	3474747	23.704 ug/ml
6) N-OCTADECANE	11.190	3530073	23.890 ug/ml
7) N-EICOSANE	12.494	3372788	22.693 ug/ml
8) N-DOCOSANE	13.689	3294421	22.182 ug/ml
10) N-TETRACOSANE	14.787	3177642	21.500 ug/ml
11) N-HEXACOSANE	15.805	3102890	21.411 ug/ml
12) N-OCTACOSANE	16.751	3080248	21.506 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
Data File : FF006730.D
Signal(s) : FID2B.ch
Acq On : 02 Apr 2020 14:38
Operator : DD\AJ
Sample : PB127957BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 02 17:49:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

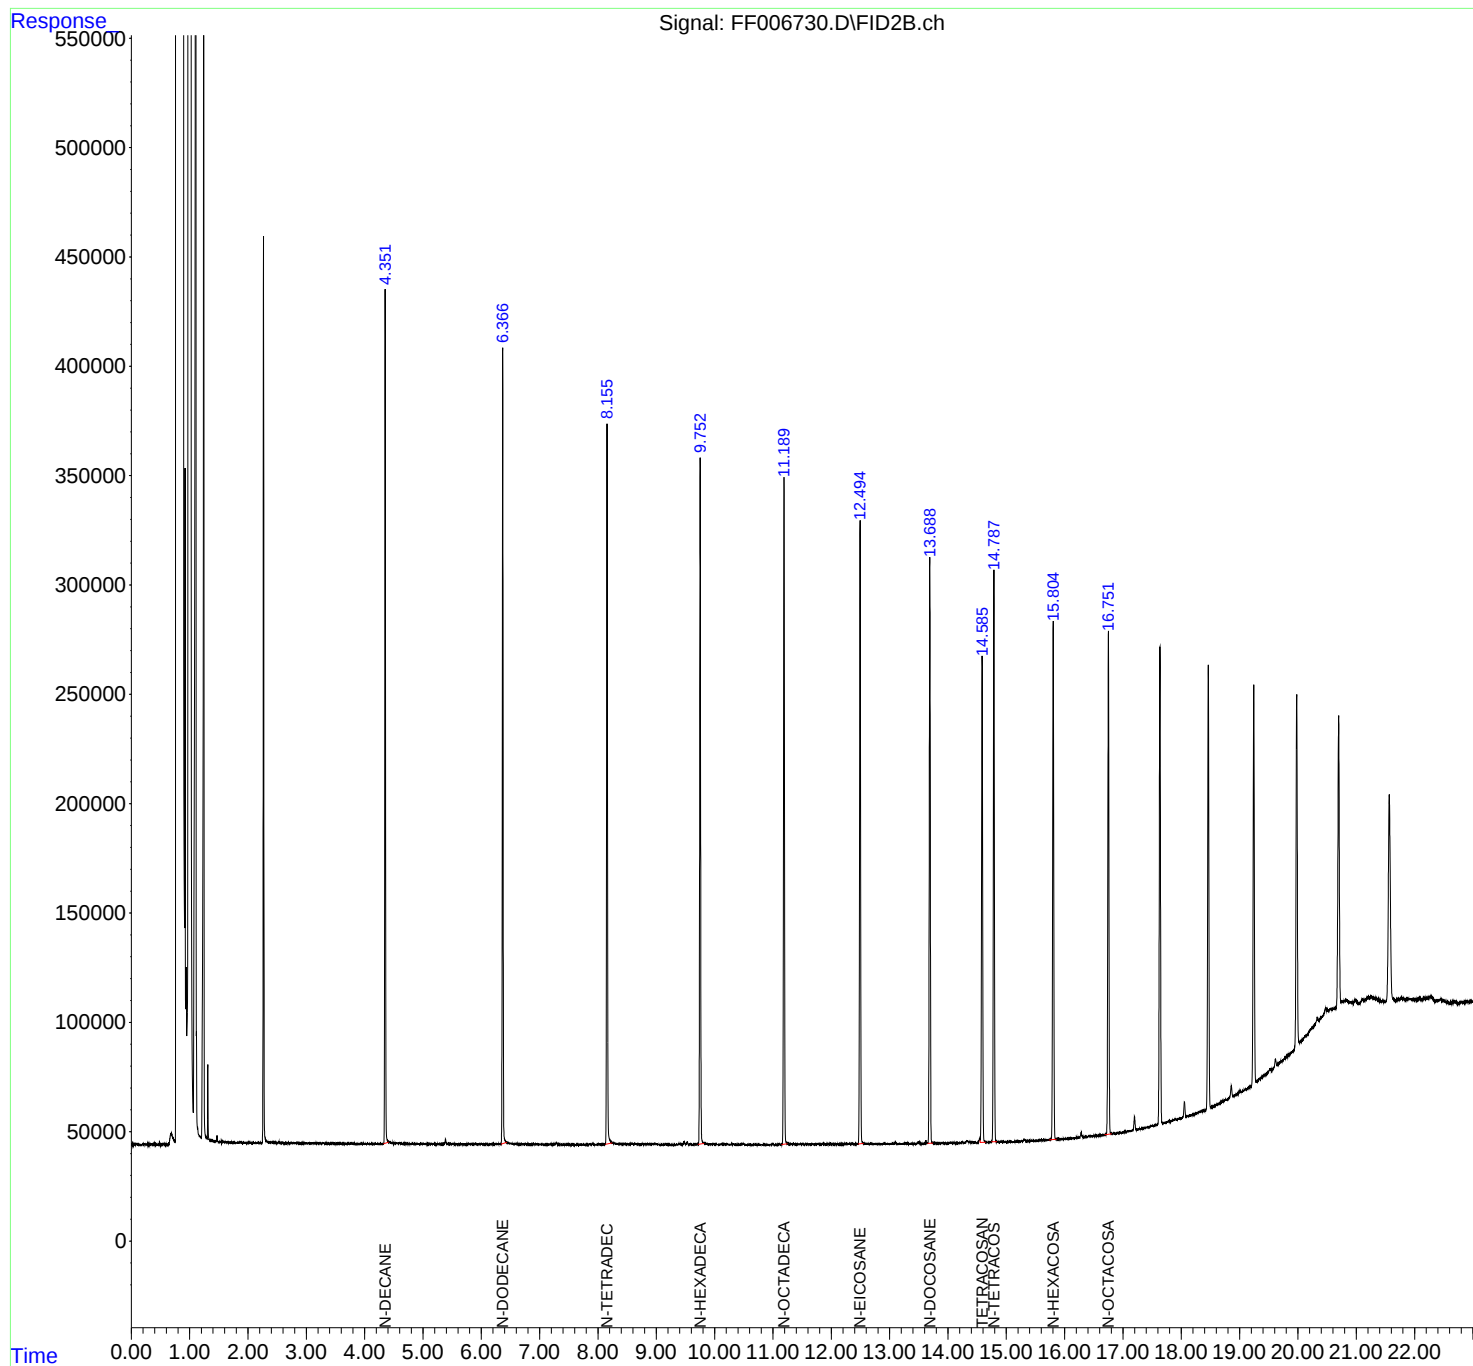

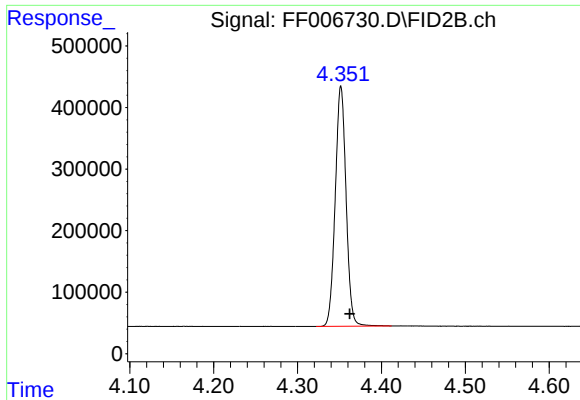


#2 N-DECANE

R.T.: 4.352 min
Delta R.T.: -0.010 min
Response: 3502762
Conc: 25.45 ug/ml

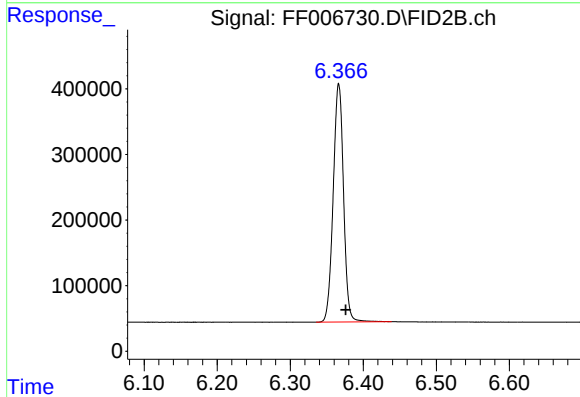


#3 N-DODECANE

R.T.: 6.367 min
Delta R.T.: -0.010 min
Response: 3571046
Conc: 25.32 ug/ml

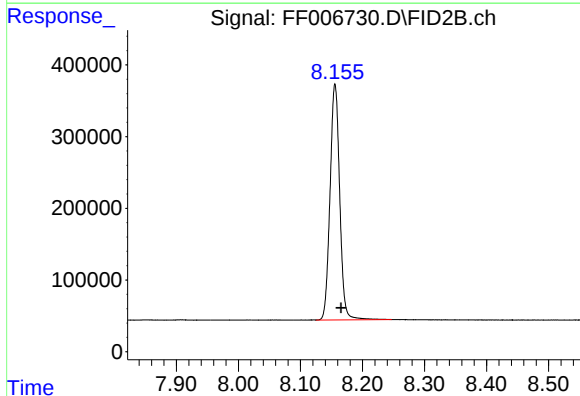


#4 N-TETRADECANE

R.T.: 8.156 min
Delta R.T.: -0.010 min
Response: 3556825
Conc: 24.87 ug/ml

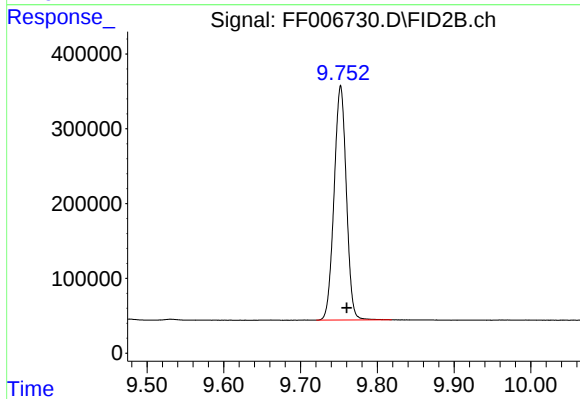


#5 N-HEXADECANE

R.T.: 9.752 min
Delta R.T.: -0.008 min
Response: 3474747
Conc: 23.70 ug/ml

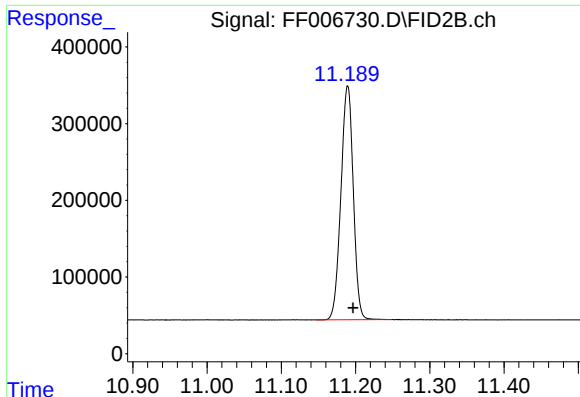


#6 N-OCTADECANE

R.T.: 11.190 min
Delta R.T.: -0.007 min
Response: 3530073
Conc: 23.89 ug/ml

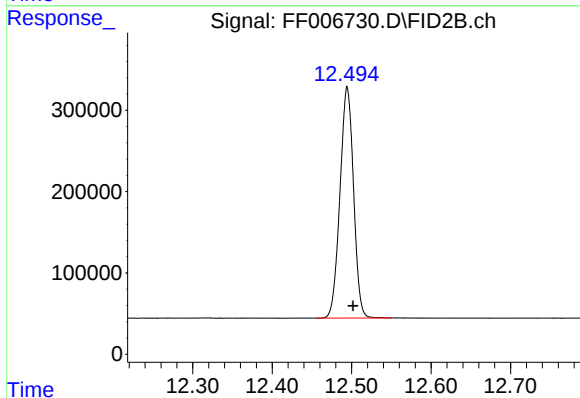


#7 N-EICOSANE

R.T.: 12.494 min
Delta R.T.: -0.007 min
Response: 3372788
Conc: 22.69 ug/ml

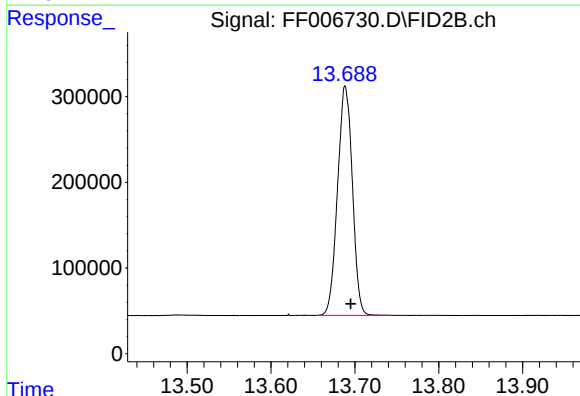


#8 N-DOCOSANE

R.T.: 13.689 min
Delta R.T.: -0.007 min
Response: 3294421
Conc: 22.18 ug/ml

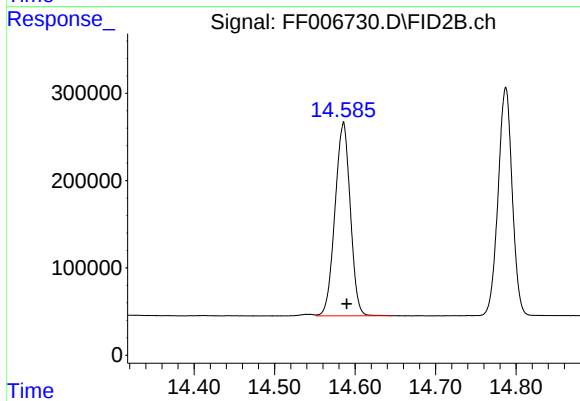


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.586 min
Delta R.T.: -0.004 min
Response: 2920852
Conc: 22.69 ug/ml

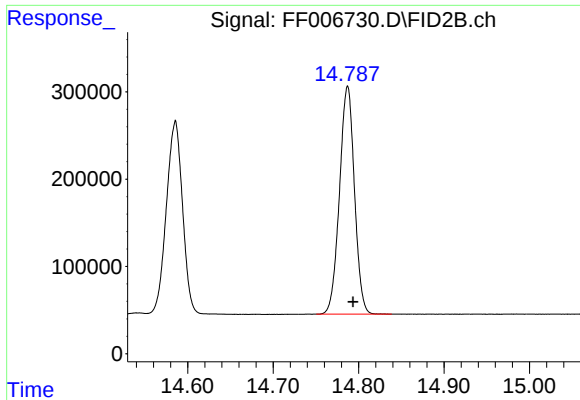


#10 N-TETRACOSANE

R.T.: 14.787 min
Delta R.T.: -0.006 min
Response: 3177642
Conc: 21.50 ug/ml

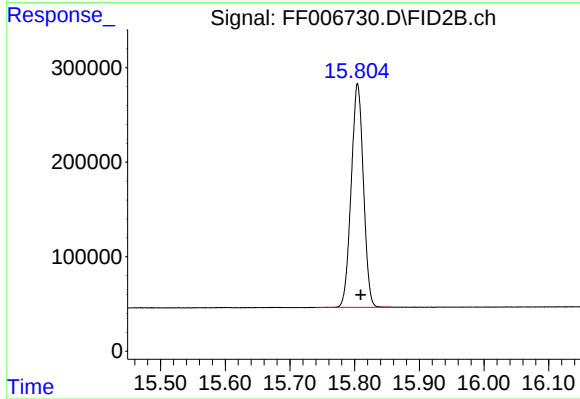

#11 N-HEXACOSANE

R.T.: 15.805 min
Delta R.T.: -0.005 min
Response: 3102890
Conc: 21.41 ug/ml

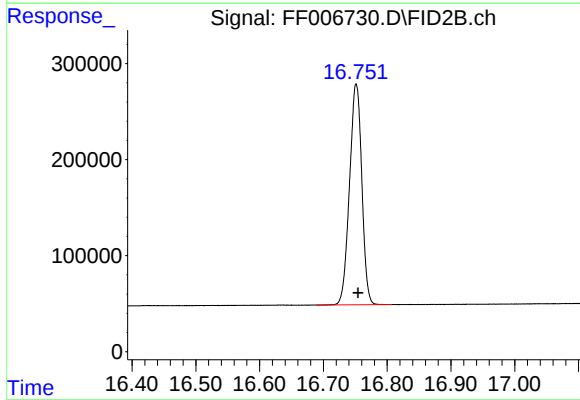

#12 N-OCTACOSANE

R.T.: 16.751 min
Delta R.T.: -0.003 min
Response: 3080248
Conc: 21.51 ug/ml