

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
 Data File : FF006736.D
 Signal(s) : FID2B.ch
 Acq On : 02 Apr 2020 18:29
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 03 01:07:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.588	5648795	43.891 ug/ml
Target Compounds			
2) N-DECANE	4.353	6976368	50.683 ug/ml
3) N-DODECANE	6.369	7093276	50.292 ug/ml
4) N-TETRADECANE	8.160	7028423	49.144 ug/ml
5) N-HEXADECANE	9.755	7076411	48.275 ug/ml
6) N-OCTADECANE	11.192	6963549	47.126 ug/ml
7) N-EICOSANE	12.498	6805682	45.790 ug/ml
8) N-DOCOSANE	13.692	6618093	44.561 ug/ml
10) N-TETRACOSANE	14.791	6423618	43.463 ug/ml
11) N-HEXACOSANE	15.808	6221950	42.935 ug/ml
12) N-OCTACOSANE	16.753	6174749	43.112 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
Data File : FF006736.D
Signal(s) : FID2B.ch
Acq On : 02 Apr 2020 18:29
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 03 01:07:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

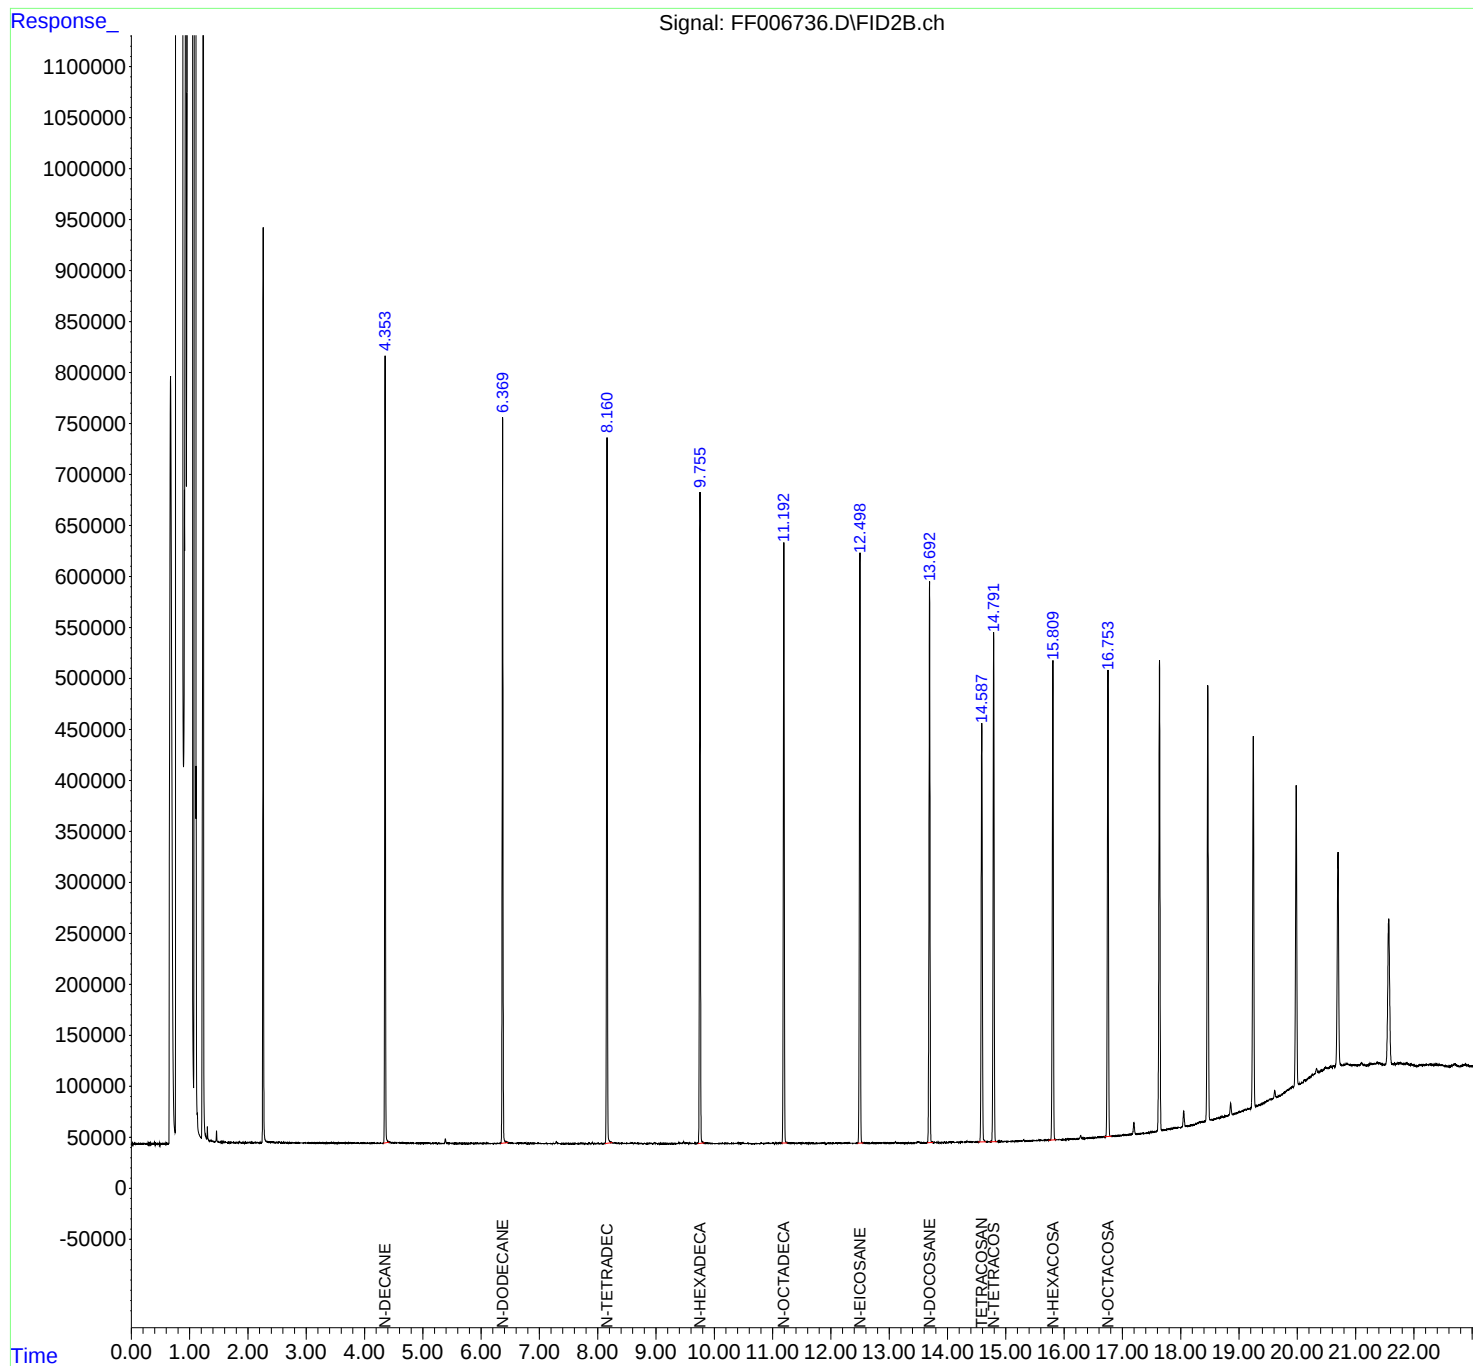

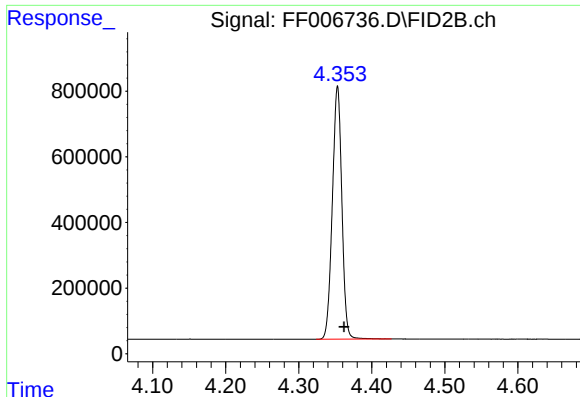


#2 N-DECANE

R.T.: 4.353 min
Delta R.T.: -0.009 min
Response: 6976368
Conc: 50.68 ug/ml

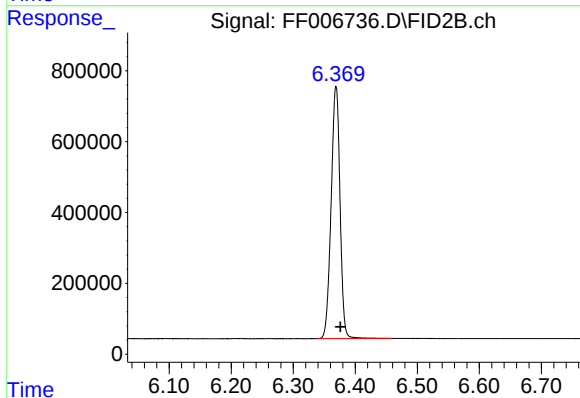


#3 N-DODECANE

R.T.: 6.369 min
Delta R.T.: -0.007 min
Response: 7093276
Conc: 50.29 ug/ml

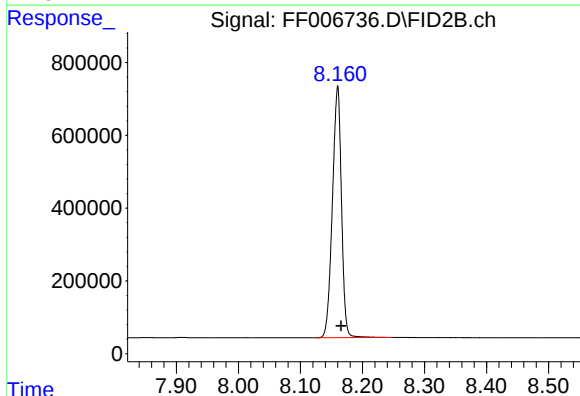


#4 N-TETRADECANE

R.T.: 8.160 min
Delta R.T.: -0.006 min
Response: 7028423
Conc: 49.14 ug/ml

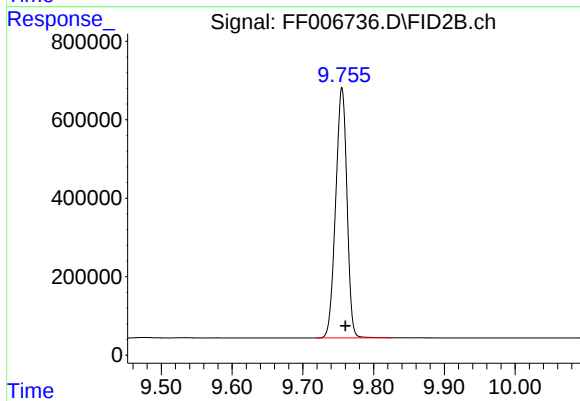


#5 N-HEXADECANE

R.T.: 9.755 min
Delta R.T.: -0.005 min
Response: 7076411
Conc: 48.27 ug/ml

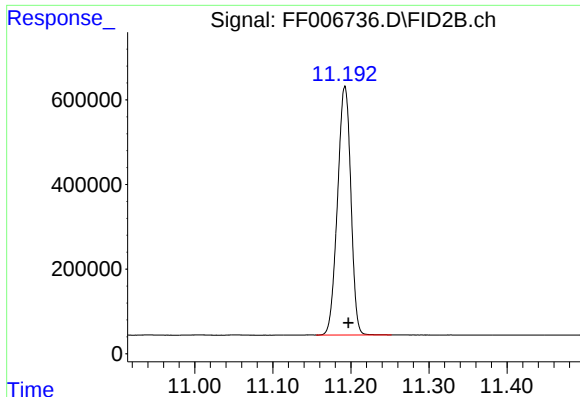


#6 N-OCTADECANE

R.T.: 11.192 min
Delta R.T.: -0.004 min
Response: 6963549
Conc: 47.13 ug/ml

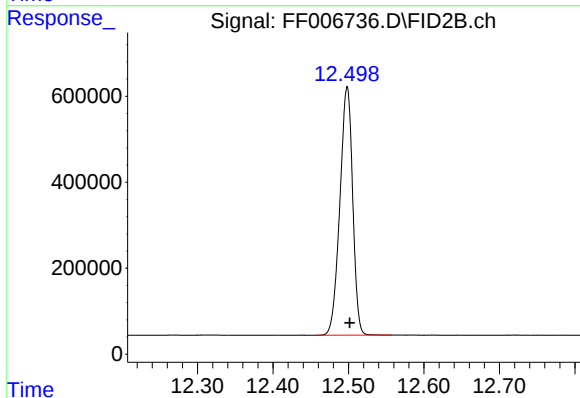


#7 N-EICOSANE

R.T.: 12.498 min
Delta R.T.: -0.004 min
Response: 6805682
Conc: 45.79 ug/ml

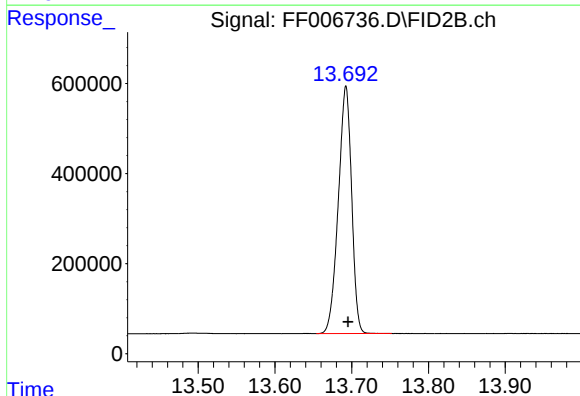


#8 N-DOCOSANE

R.T.: 13.692 min
Delta R.T.: -0.003 min
Response: 6618093
Conc: 44.56 ug/ml

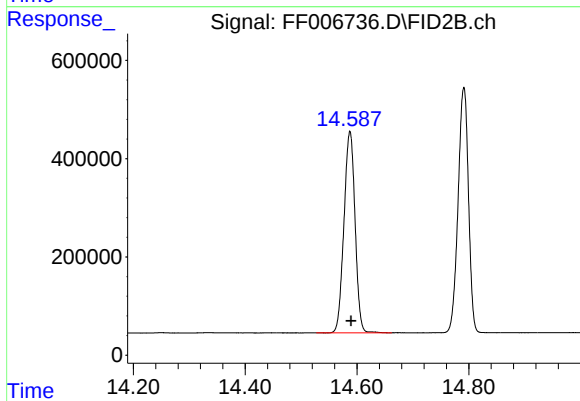


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.588 min
Delta R.T.: -0.002 min
Response: 5648795
Conc: 43.89 ug/ml

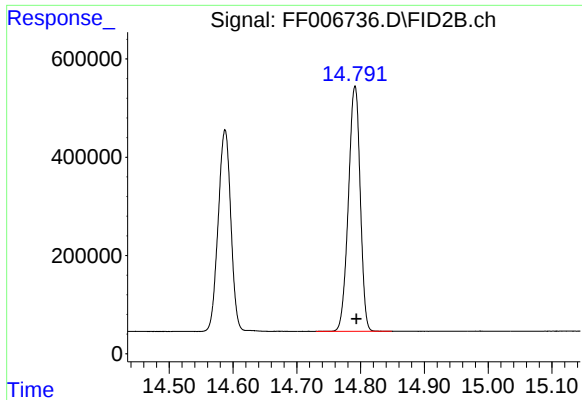


#10 N-TETRACOSANE

R.T.: 14.791 min
Delta R.T.: -0.002 min
Response: 6423618
Conc: 43.46 ug/ml

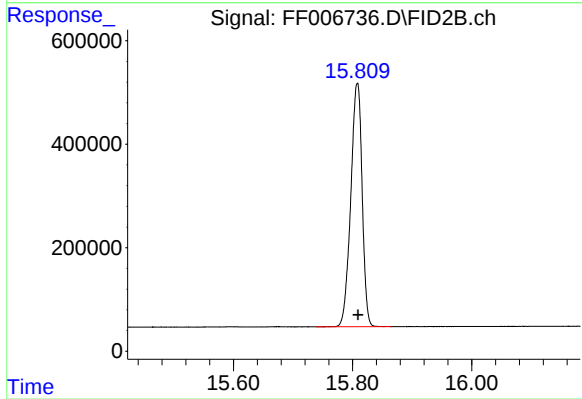

#11 N-HEXACOSANE

R.T.: 15.808 min
Delta R.T.: -0.001 min
Response: 6221950
Conc: 42.93 ug/ml

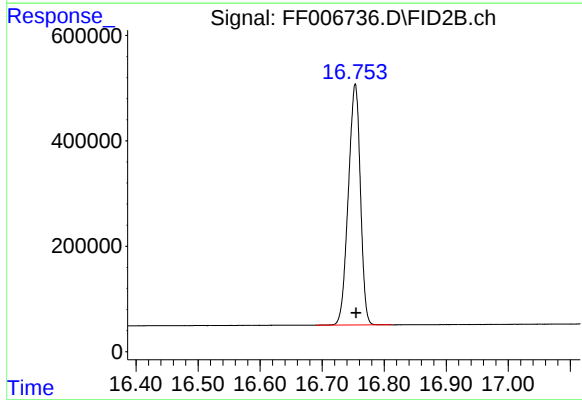

#12 N-OCTACOSANE

R.T.: 16.753 min
Delta R.T.: -0.001 min
Response: 6174749
Conc: 43.11 ug/ml