

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
 Data File : FF006747.D
 Signal(s) : FID2B.ch
 Acq On : 03 Apr 2020 00:04
 Operator : DD\AJ
 Sample : L2129-27MSD
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 03 01:06:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.582	2057404	15.986 ug/ml
Target Compounds			
2) N-DECANE	4.351	3393868	24.656 ug/ml
3) N-DODECANE	6.366	3626256	25.711 ug/ml
4) N-TETRADECANE	8.155	3789905	26.500 ug/ml
5) N-HEXADECANE	9.751	3875264	26.437 ug/ml
6) N-OCTADECANE	11.188	4019520	27.202 ug/ml
7) N-EICOSANE	12.494	3867377	26.021 ug/ml
8) N-DOCOSANE	13.687	3844935	25.889 ug/ml
10) N-TETRACOSANE	14.786	3726100	25.211 ug/ml
11) N-HEXACOSANE	15.802	3753822	25.903 ug/ml
12) N-OCTACOSANE	16.747	3934733	27.472 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040220\
Data File : FF006747.D
Signal(s) : FID2B.ch
Acq On : 03 Apr 2020 00:04
Operator : DD\AJ
Sample : L2129-27MSD
Misc :
ALS Vial : 71 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 03 01:06:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

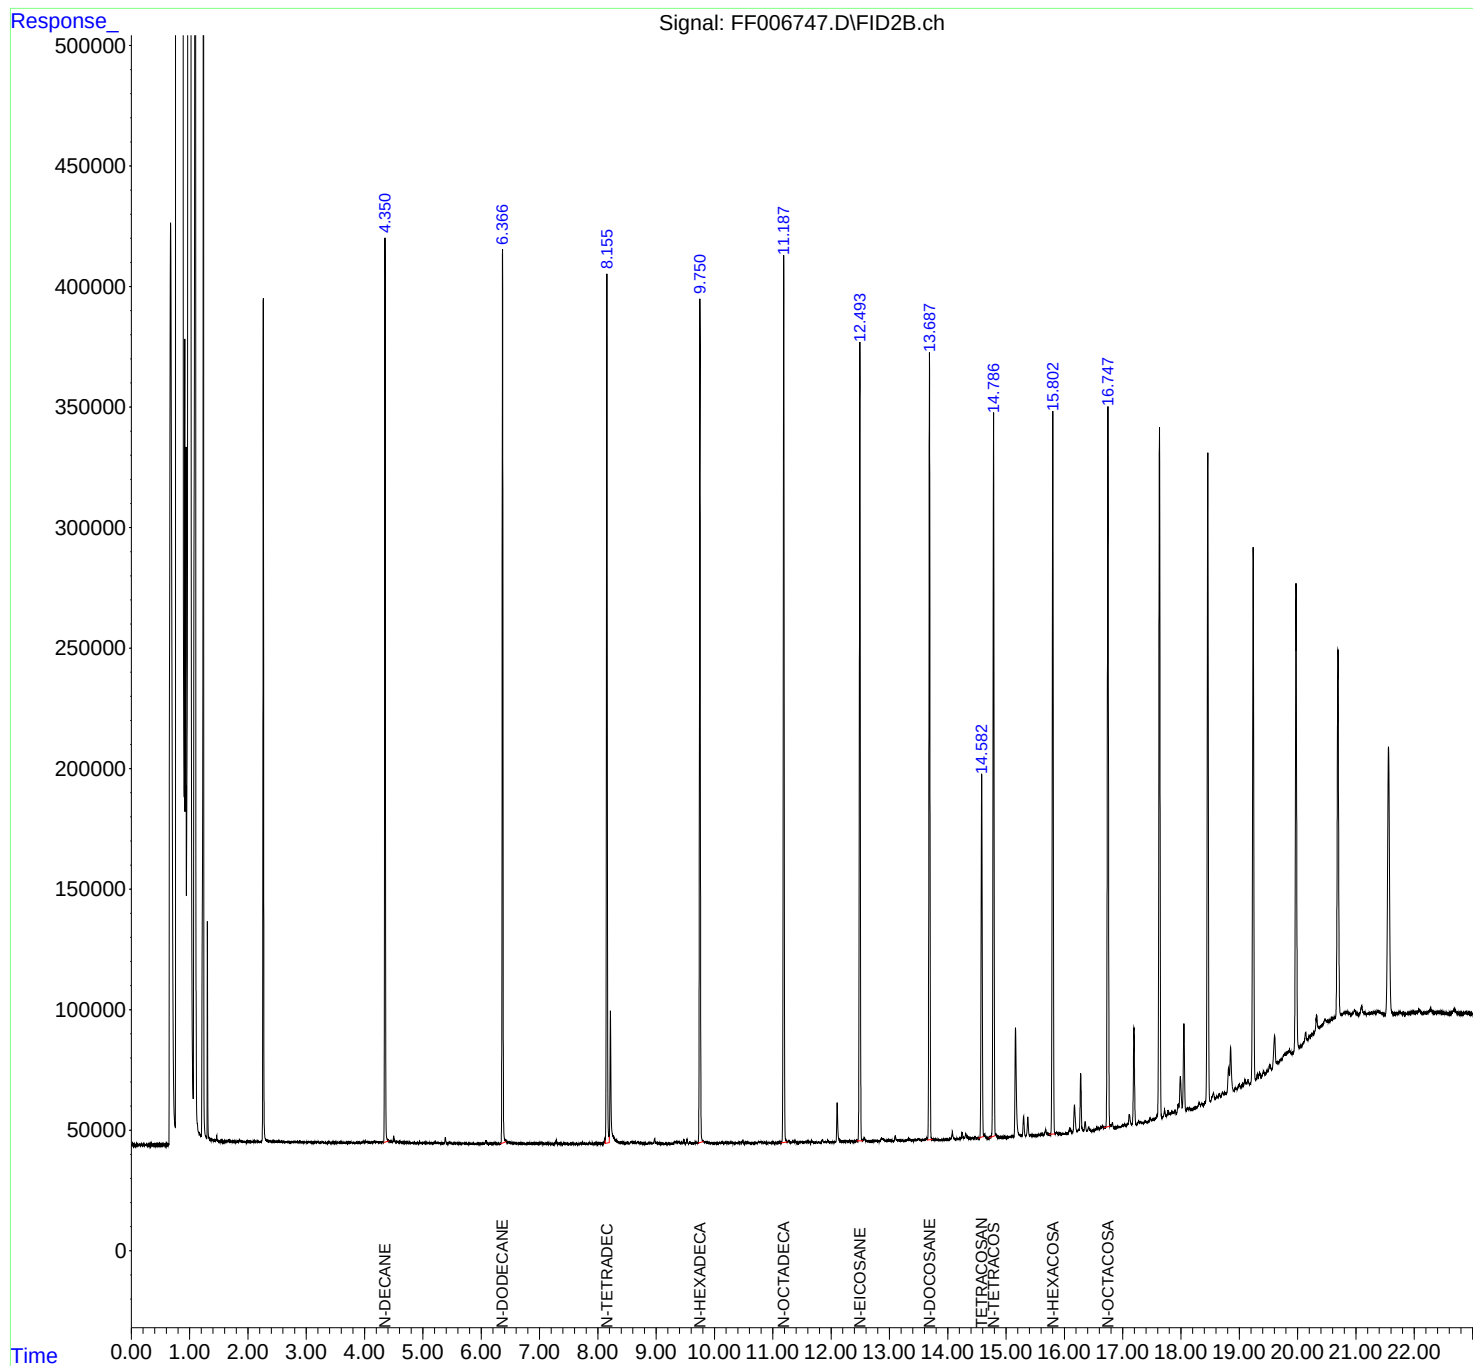

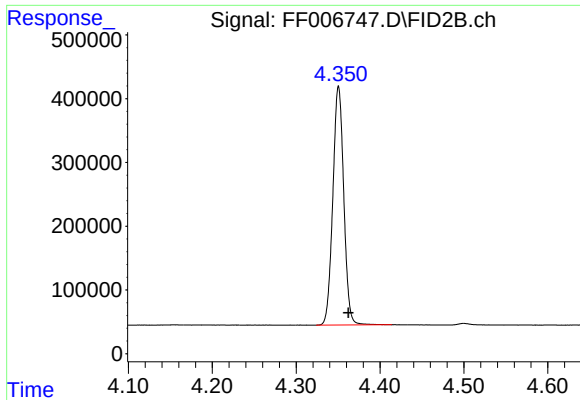


#2 N-DECANE

R.T.: 4.351 min
Delta R.T.: -0.012 min
Response: 3393868
Conc: 24.66 ug/ml

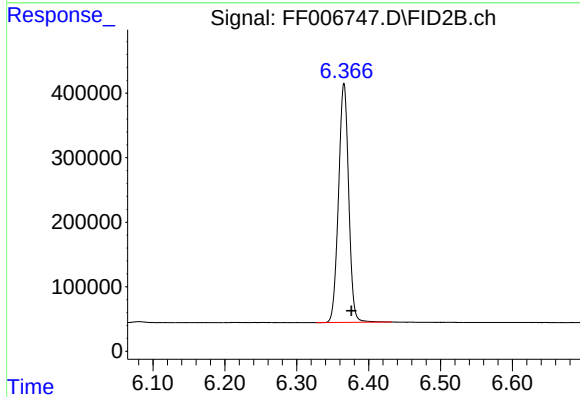


#3 N-DODECANE

R.T.: 6.366 min
Delta R.T.: -0.010 min
Response: 3626256
Conc: 25.71 ug/ml

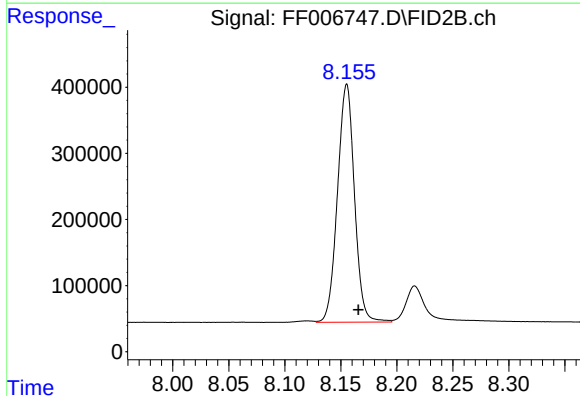


#4 N-TETRADECANE

R.T.: 8.155 min
Delta R.T.: -0.010 min
Response: 3789905
Conc: 26.50 ug/ml

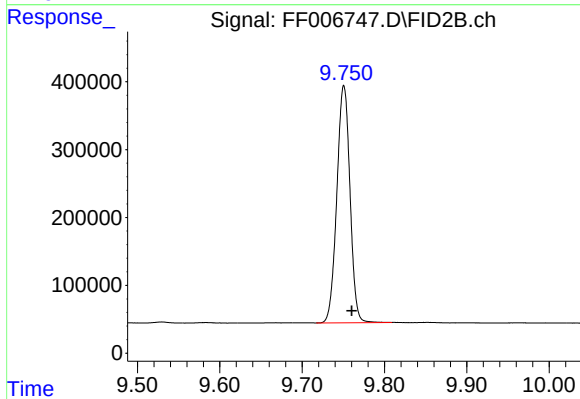


#5 N-HEXADECANE

R.T.: 9.751 min
Delta R.T.: -0.009 min
Response: 3875264
Conc: 26.44 ug/ml

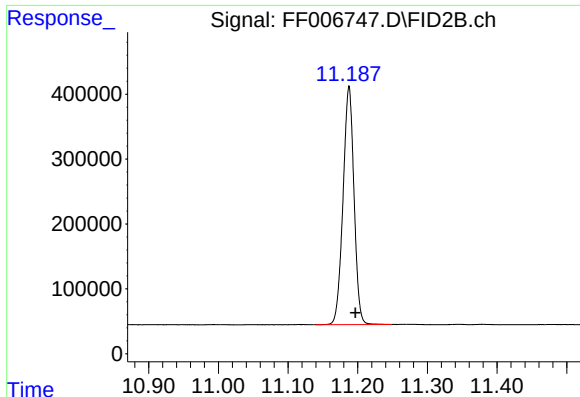


#6 N-OCTADECANE

R.T.: 11.188 min
Delta R.T.: -0.009 min
Response: 4019520
Conc: 27.20 ug/ml

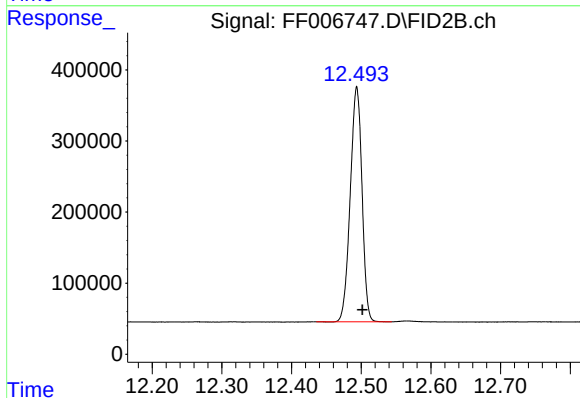


#7 N-EICOSANE

R.T.: 12.494 min
Delta R.T.: -0.008 min
Response: 3867377
Conc: 26.02 ug/ml

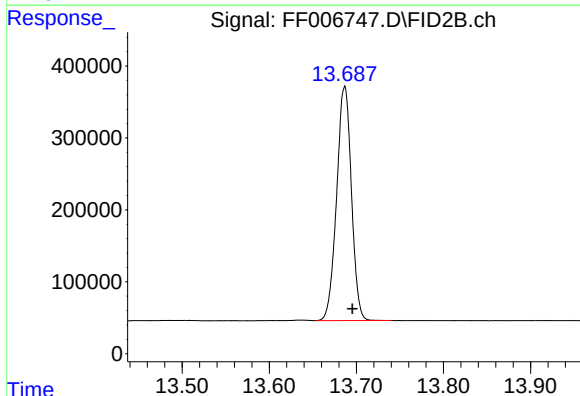


#8 N-DOCOSANE

R.T.: 13.687 min
Delta R.T.: -0.009 min
Response: 3844935
Conc: 25.89 ug/ml

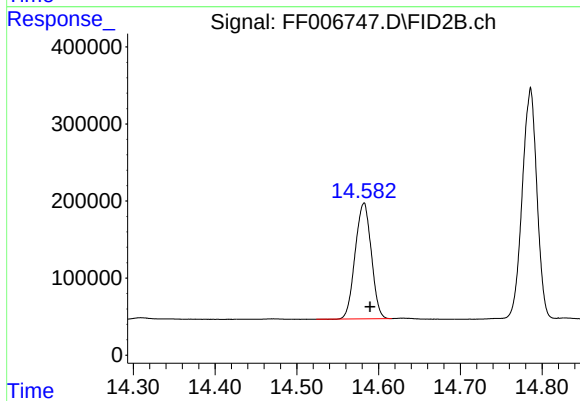


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.582 min
Delta R.T.: -0.008 min
Response: 2057404
Conc: 15.99 ug/ml

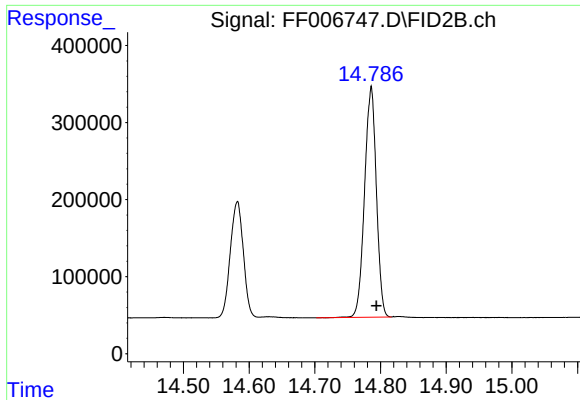


#10 N-TETRACOSANE

R.T.: 14.786 min
Delta R.T.: -0.008 min
Response: 3726100
Conc: 25.21 ug/ml

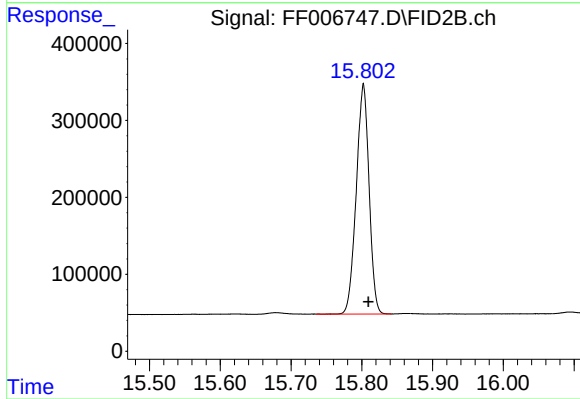

#11 N-HEXACOSANE

R.T.: 15.802 min
Delta R.T.: -0.007 min
Response: 3753822
Conc: 25.90 ug/ml

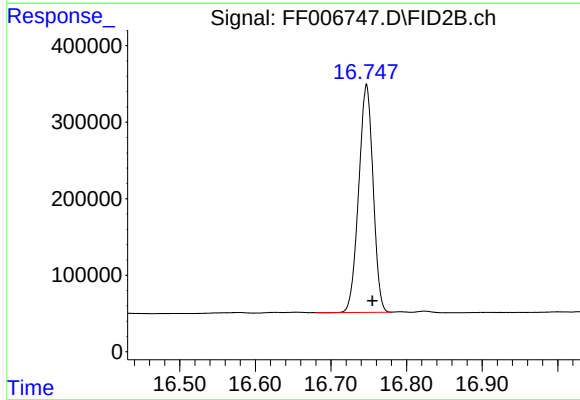

#12 N-OCTACOSANE

R.T.: 16.747 min
Delta R.T.: -0.008 min
Response: 3934733
Conc: 27.47 ug/ml