

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040319\
Data File : FF004078.D
Signal(s) : FID2B.ch
Acq On : 03 Apr 2019 12:27
Operator : AJ\SJ
Sample : K2186-01 50X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 03 14:43:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.317	52292	0.373 ug/ml
7) N-EICOSANE	12.524f	260979	1.737 ug/ml
10) N-TETRACOSANE	14.757	170437	1.157 ug/ml
12) N-OCTACOSANE	16.668f	79390	0.552 ug/ml
13) N-TRIACONTANE	17.628	136939	0.959 ug/ml
14) N-DOTRIACONTANE	18.463	140414	0.995 ug/ml
15) N-TETRATRIACONTANE	19.255	93550	0.701 ug/ml
16) N-HEXATRIACONTANE	19.999	67821	0.535 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040319\
Data File : FF04078.D
Signal(s) : FID2B.ch
Acq On : 03 Apr 2019 12:27
Operator : AJ\SJ
Sample : K2186-01 50X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 03 14:43:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

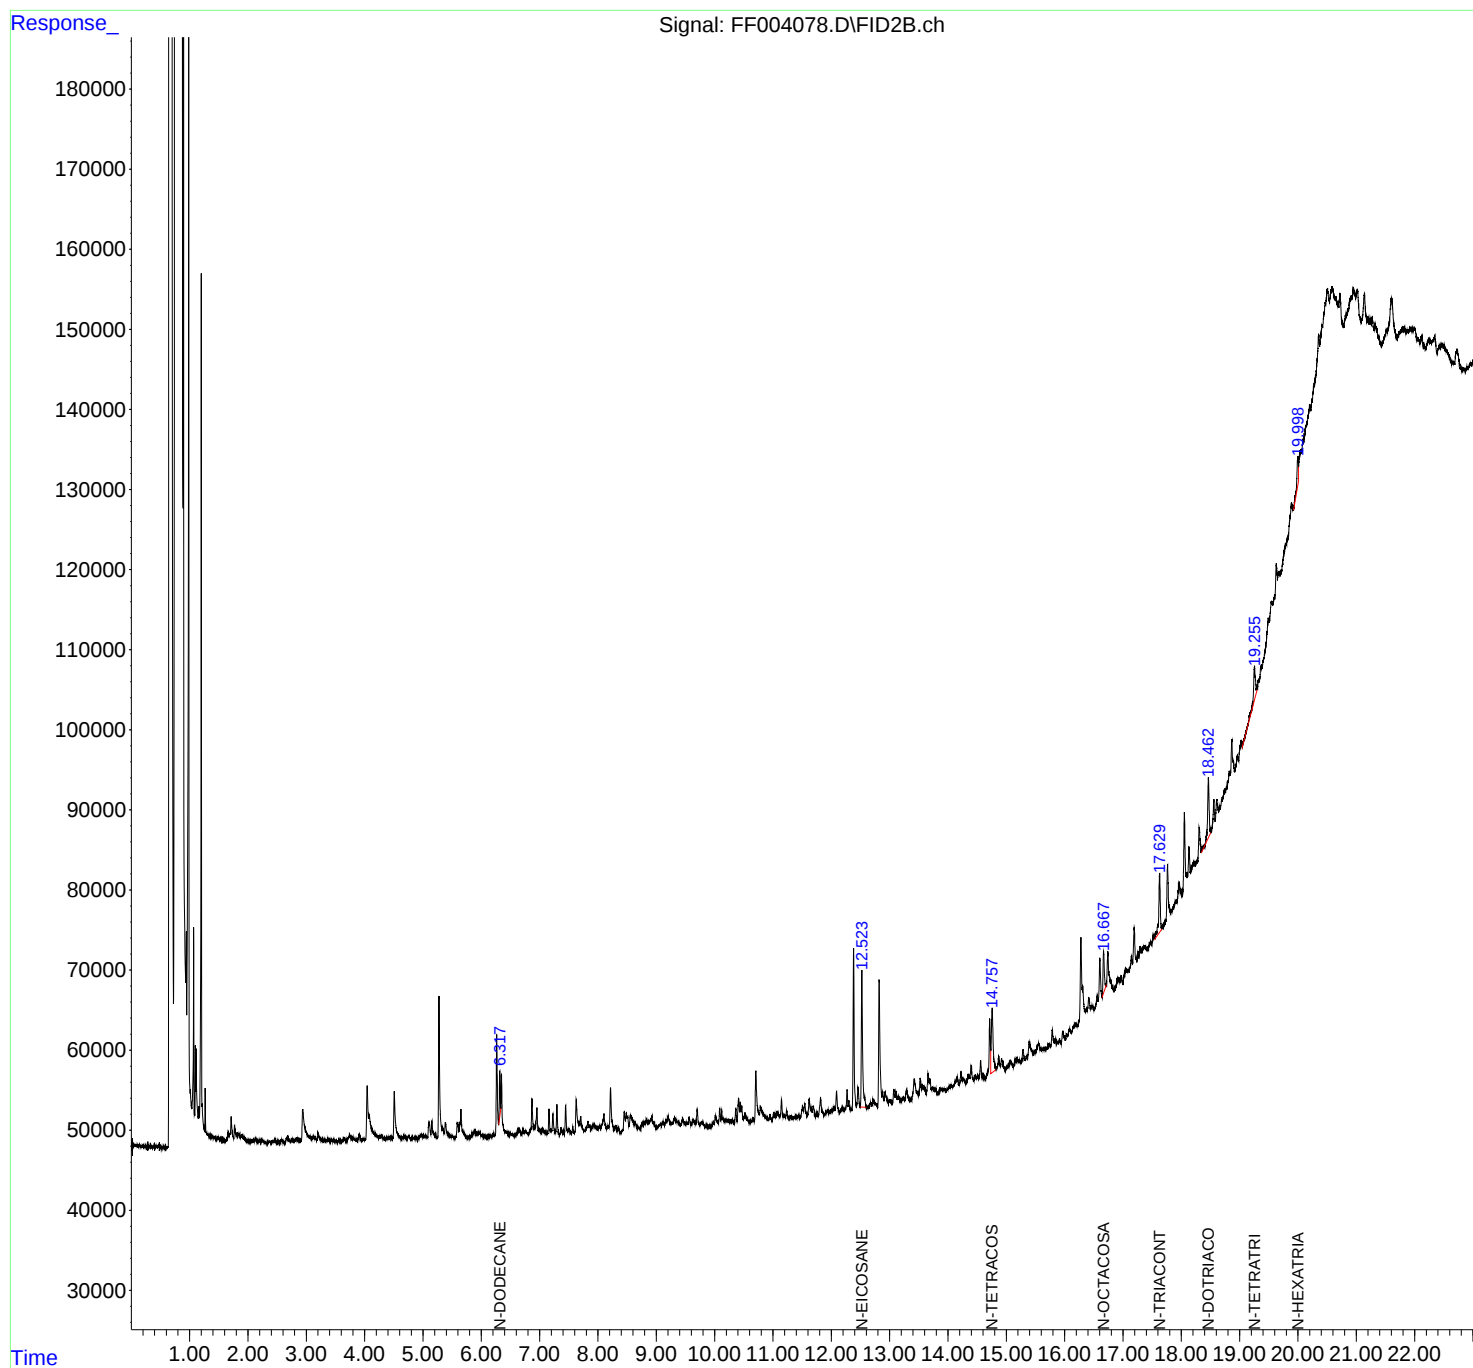

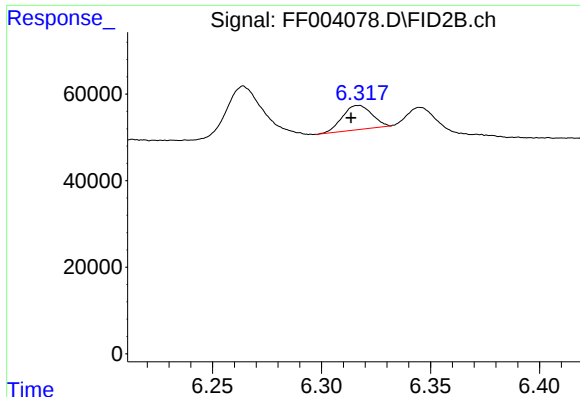


#3 N-DODECANE

R.T.: 6.317 min
Delta R.T.: 0.003 min
Response: 52292
Conc: 0.37 ug/ml

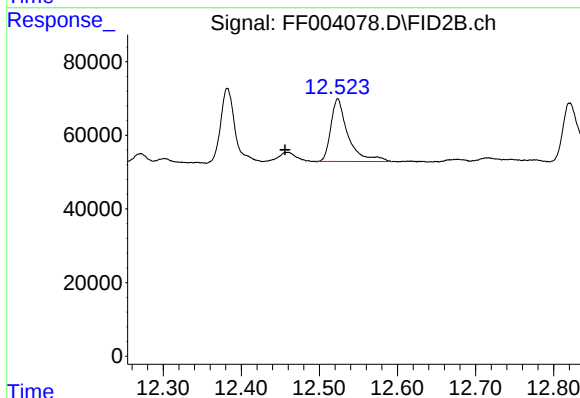


#7 N-EICOSANE

R.T.: 12.524 min
Delta R.T.: 0.068 min
Response: 260979
Conc: 1.74 ug/ml

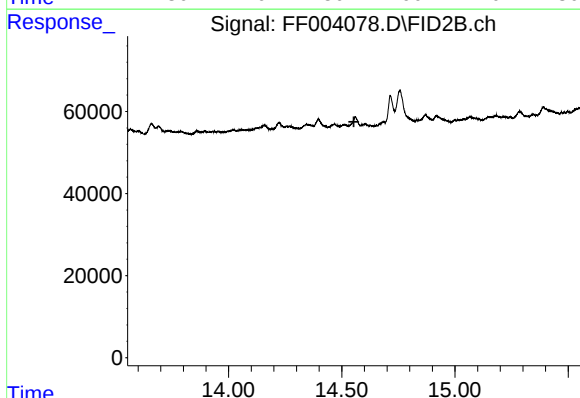


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.553 min
Response: 0
Conc: N.D.

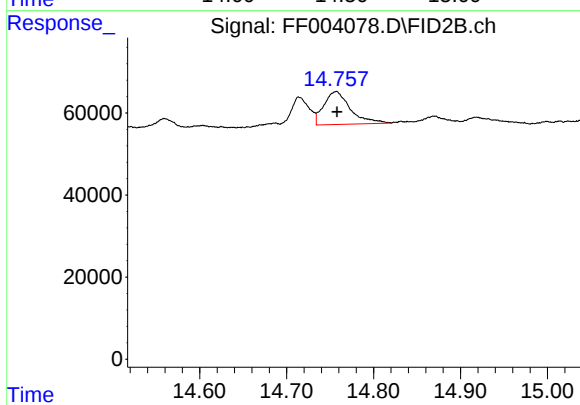


#10 N-TETRACOSANE

R.T.: 14.757 min
Delta R.T.: 0.000 min
Response: 170437
Conc: 1.16 ug/ml

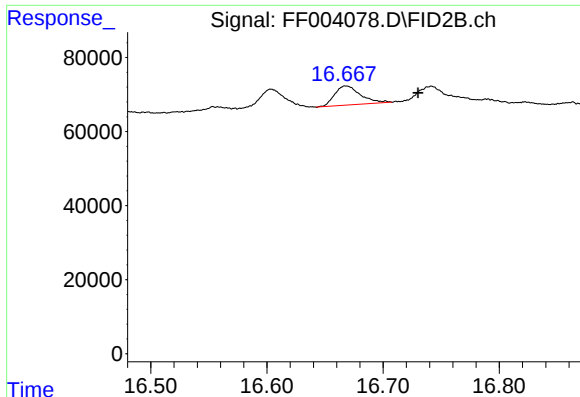


#12 N-OCTACOSANE

R.T.: 16.668 min
Delta R.T.: -0.062 min
Response: 79390
Conc: 0.55 ug/ml

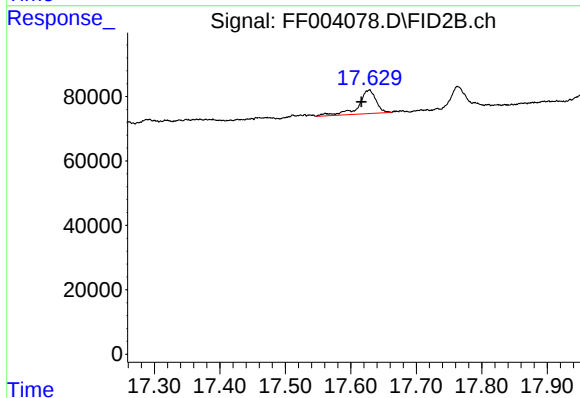


#13 N-TRIACONTANE

R.T.: 17.628 min
Delta R.T.: 0.012 min
Response: 136939
Conc: 0.96 ug/ml

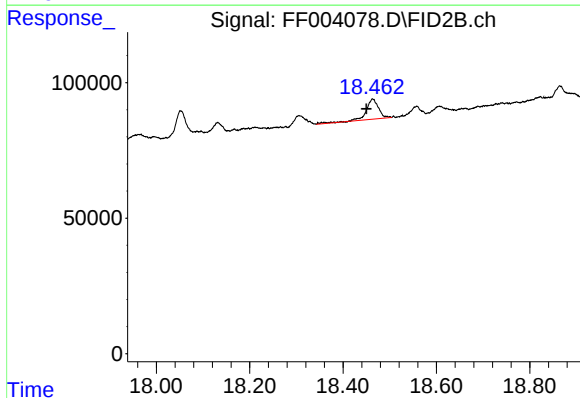


#14 N-DOTRIACONTANE

R.T.: 18.463 min
Delta R.T.: 0.013 min
Response: 140414
Conc: 0.99 ug/ml

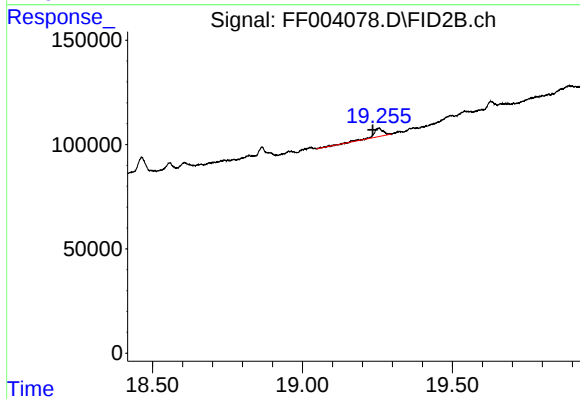

#15 N-TETRATRIACONTANE

R.T.: 19.255 min
Delta R.T.: 0.021 min
Response: 93550
Conc: 0.70 ug/ml

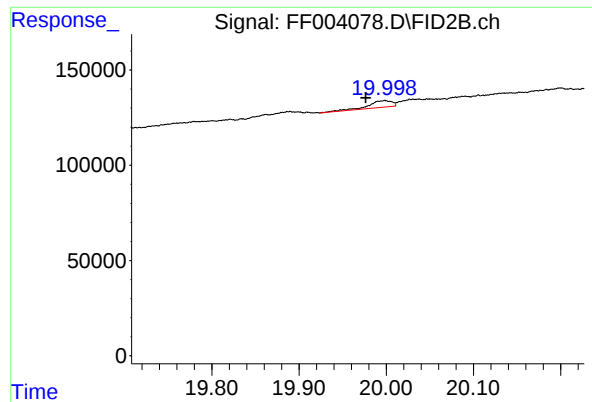

#16 N-HEXATRIACONTANE

R.T.: 19.999 min
Delta R.T.: 0.022 min
Response: 67821
Conc: 0.53 ug/ml