

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040319\
 Data File : FF004087.D
 Signal(s) : FID2B.ch
 Acq On : 03 Apr 2019 17:07
 Operator : AJ\SJ
 Sample : K2213-07
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 04 01:57:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.559	2074754	15.960 ug/ml
Target Compounds			
4) N-TETRADECANE	8.172f	162920	1.146 ug/ml
7) N-EICOSANE	12.524f	257968	1.717 ug/ml
8) N-DOCOSANE	13.658	107244	0.716 ug/ml
10) N-TETRACOSANE	14.759	214724	1.458 ug/ml
11) N-HEXACOSANE	15.785	118326	0.815 ug/ml
12) N-OCTACOSANE	16.737	252184	1.754 ug/ml
13) N-TRIACONTANE	17.625	295556	2.069 ug/ml
14) N-DOTRIACONTANE	18.456	267882	1.898 ug/ml
16) N-HEXATRIACONTANE	19.990	101822	0.802 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040319\
Data File : FF004087.D
Signal(s) : FID2B.ch
Acq On : 03 Apr 2019 17:07
Operator : AJ\SJ
Sample : K2213-07
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 04 01:57:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

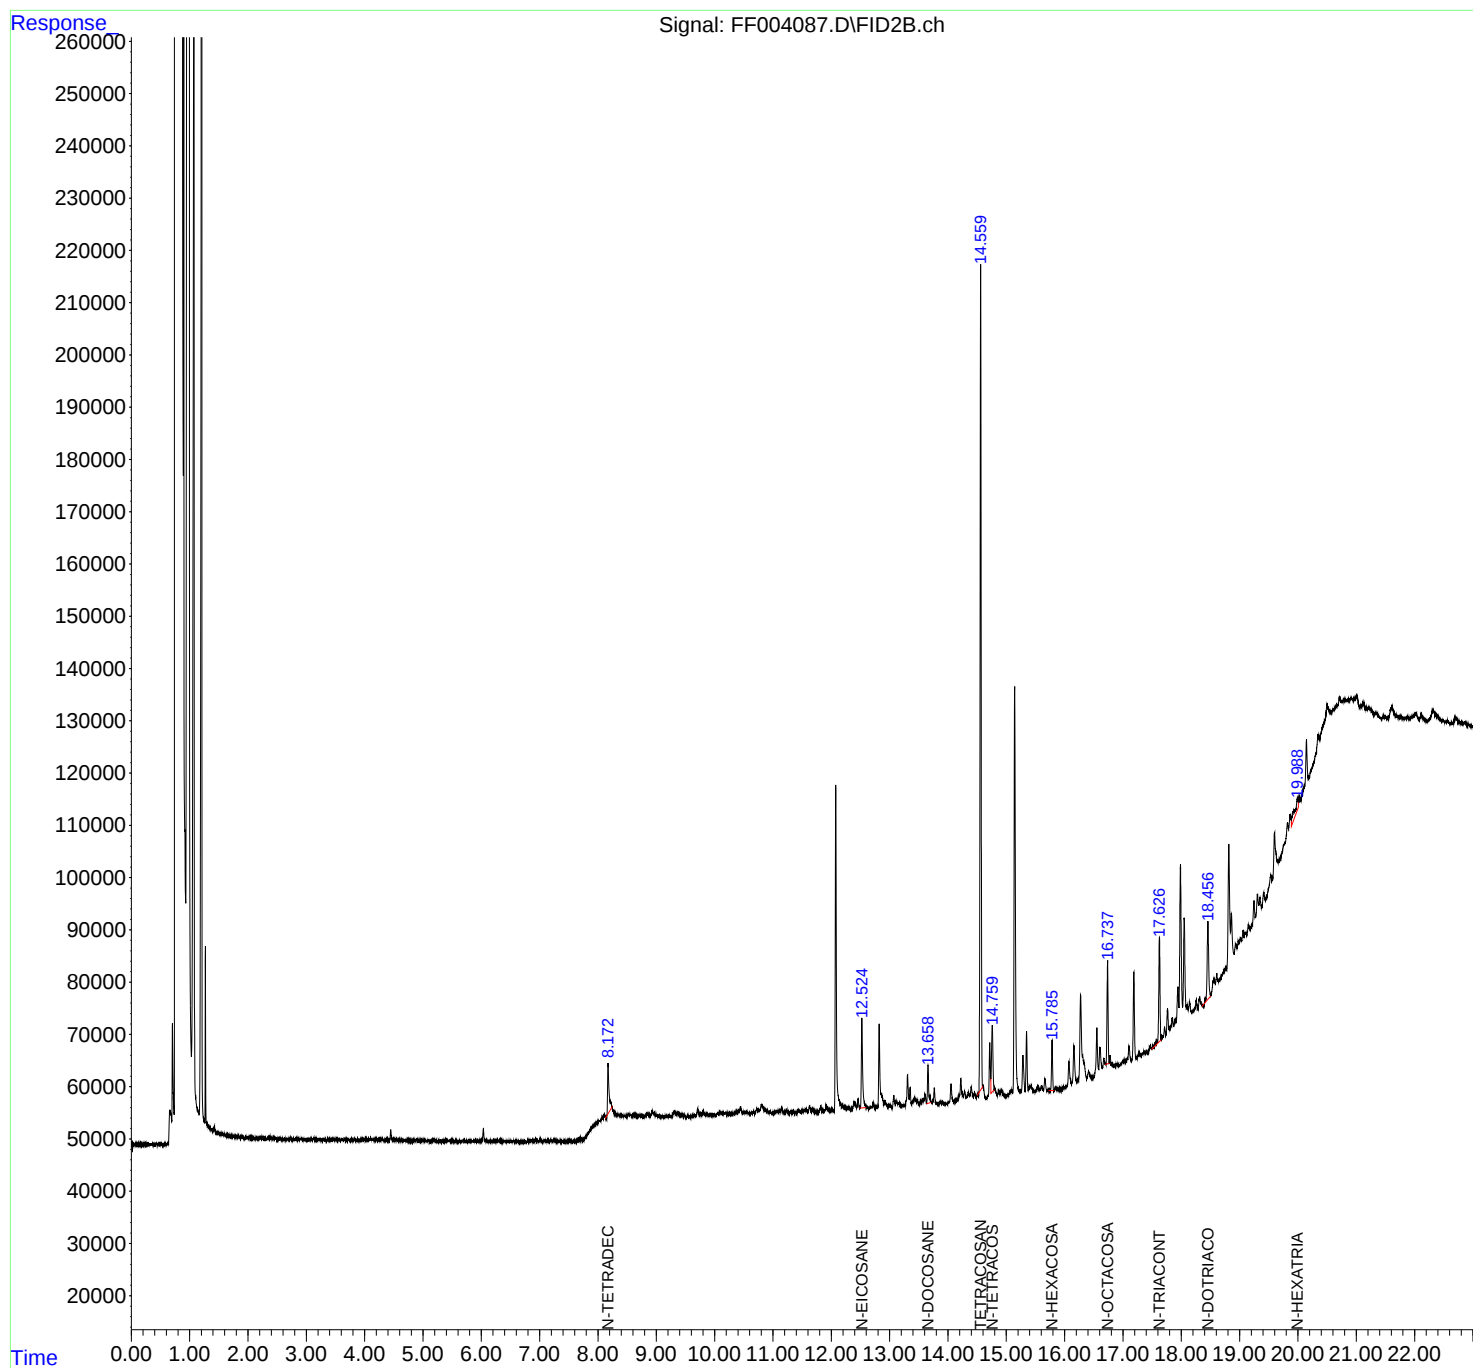

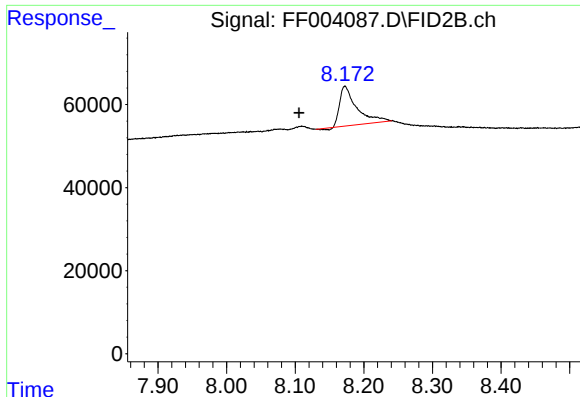


#4 N-TETRADECANE

R.T.: 8.172 min
Delta R.T.: 0.067 min
Response: 162920
Conc: 1.15 ug/ml

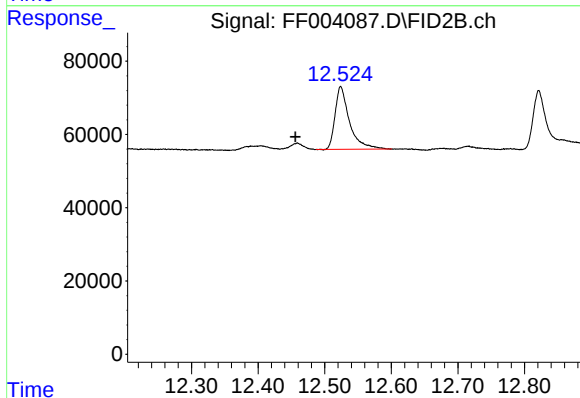


#7 N-EICOSANE

R.T.: 12.524 min
Delta R.T.: 0.068 min
Response: 257968
Conc: 1.72 ug/ml

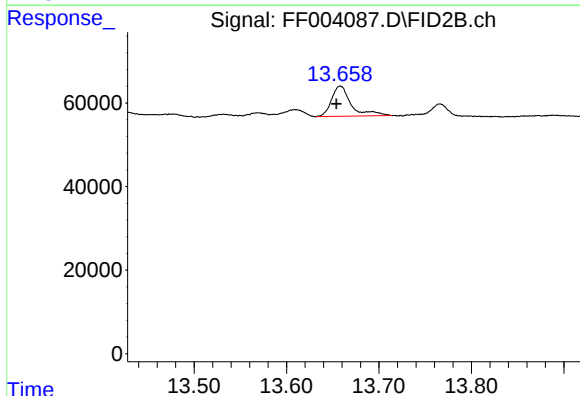


#8 N-DOCOSANE

R.T.: 13.658 min
Delta R.T.: 0.004 min
Response: 107244
Conc: 0.72 ug/ml

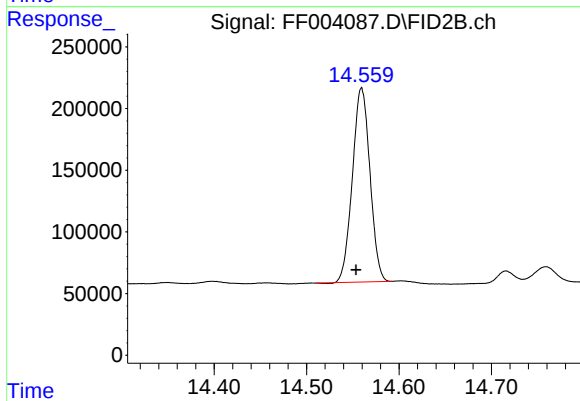


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.559 min
Delta R.T.: 0.006 min
Response: 2074754
Conc: 15.96 ug/ml

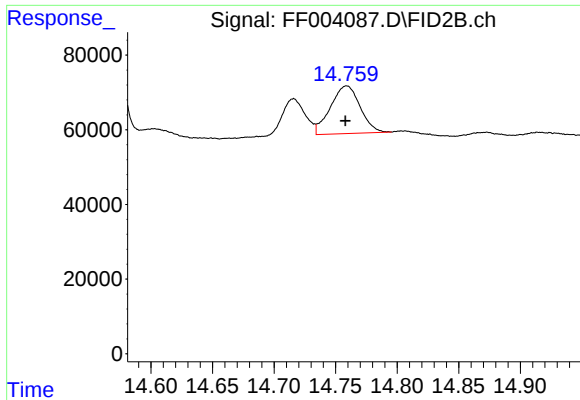


#10 N-TETRACOSANE

R.T.: 14.759 min
Delta R.T.: 0.001 min
Response: 214724
Conc: 1.46 ug/ml

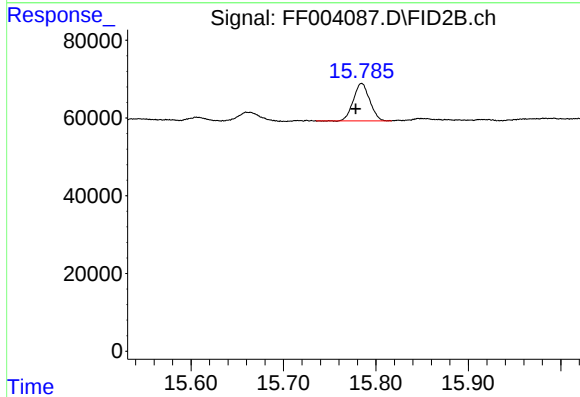


#11 N-HEXACOSANE

R.T.: 15.785 min
Delta R.T.: 0.006 min
Response: 118326
Conc: 0.82 ug/ml

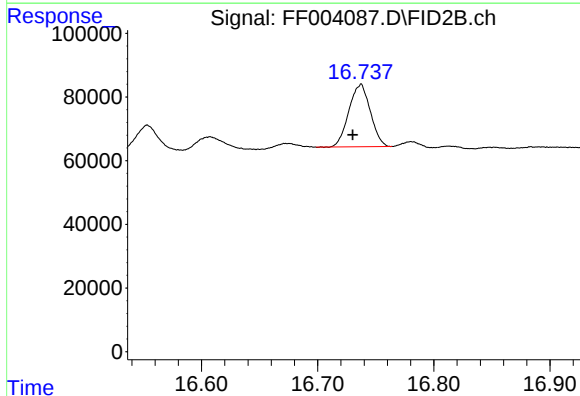


#12 N-OCTACOSANE

R.T.: 16.737 min
Delta R.T.: 0.007 min
Response: 252184
Conc: 1.75 ug/ml

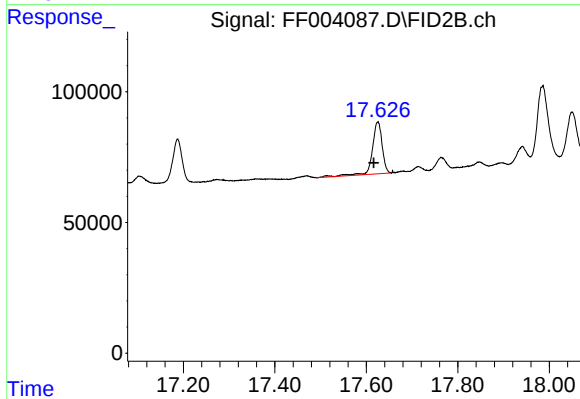


#13 N-TRIACONTANE

R.T.: 17.625 min
Delta R.T.: 0.009 min
Response: 295556
Conc: 2.07 ug/ml

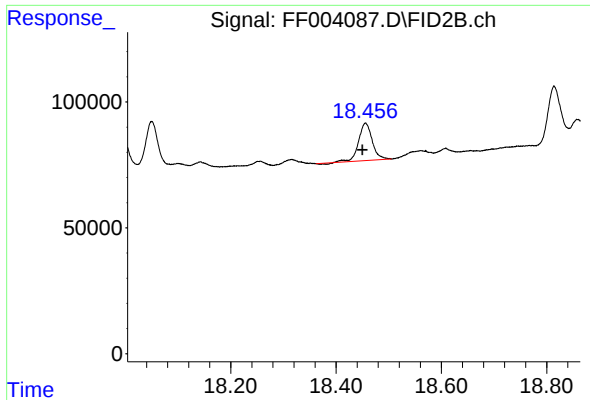

#14 N-DOTRIACONTANE

R.T.: 18.456 min
Delta R.T.: 0.006 min
Response: 267882
Conc: 1.90 ug/ml

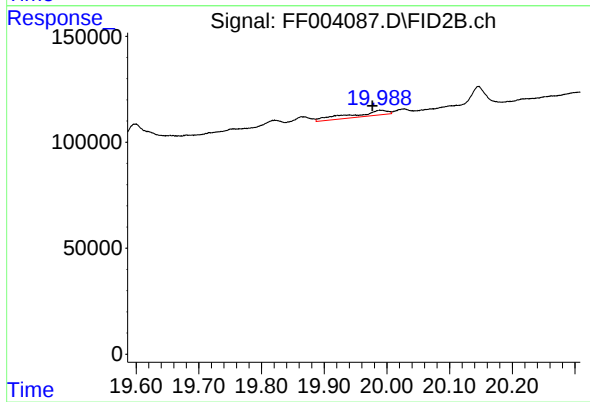

#16 N-HEXATRIACONTANE

R.T.: 19.990 min
Delta R.T.: 0.013 min
Response: 101822
Conc: 0.80 ug/ml