

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040319\
 Data File : FF004089.D
 Signal(s) : FID2B.ch
 Acq On : 03 Apr 2019 18:10
 Operator : AJ\SJ
 Sample : K2213-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 04 01:57:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.561	1981233	15.240 ug/ml
Target Compounds			
4) N-TETRADECANE	8.173f	134421	0.945 ug/ml
7) N-EICOSANE	12.525f	245101	1.631 ug/ml
10) N-TETRACOSANE	14.756	266425	1.809 ug/ml
11) N-HEXACOSANE	15.786	88301	0.608 ug/ml
12) N-OCTACOSANE	16.737	154197	1.072 ug/ml
13) N-TRIACONTANE	17.626	206698	1.447 ug/ml
14) N-DOTRIACONTANE	18.460	200756	1.422 ug/ml
16) N-HEXATRIACONTANE	19.988	289972	2.285 ug/ml
18) N-TETRACONTANE	21.608	243751	2.010 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040319\
 Data File : FF004089.D
 Signal(s) : FID2B.ch
 Acq On : 03 Apr 2019 18:10
 Operator : AJ\SJ
 Sample : K2213-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1


Integration File: autoint1.e
 Quant Time: Apr 04 01:57:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

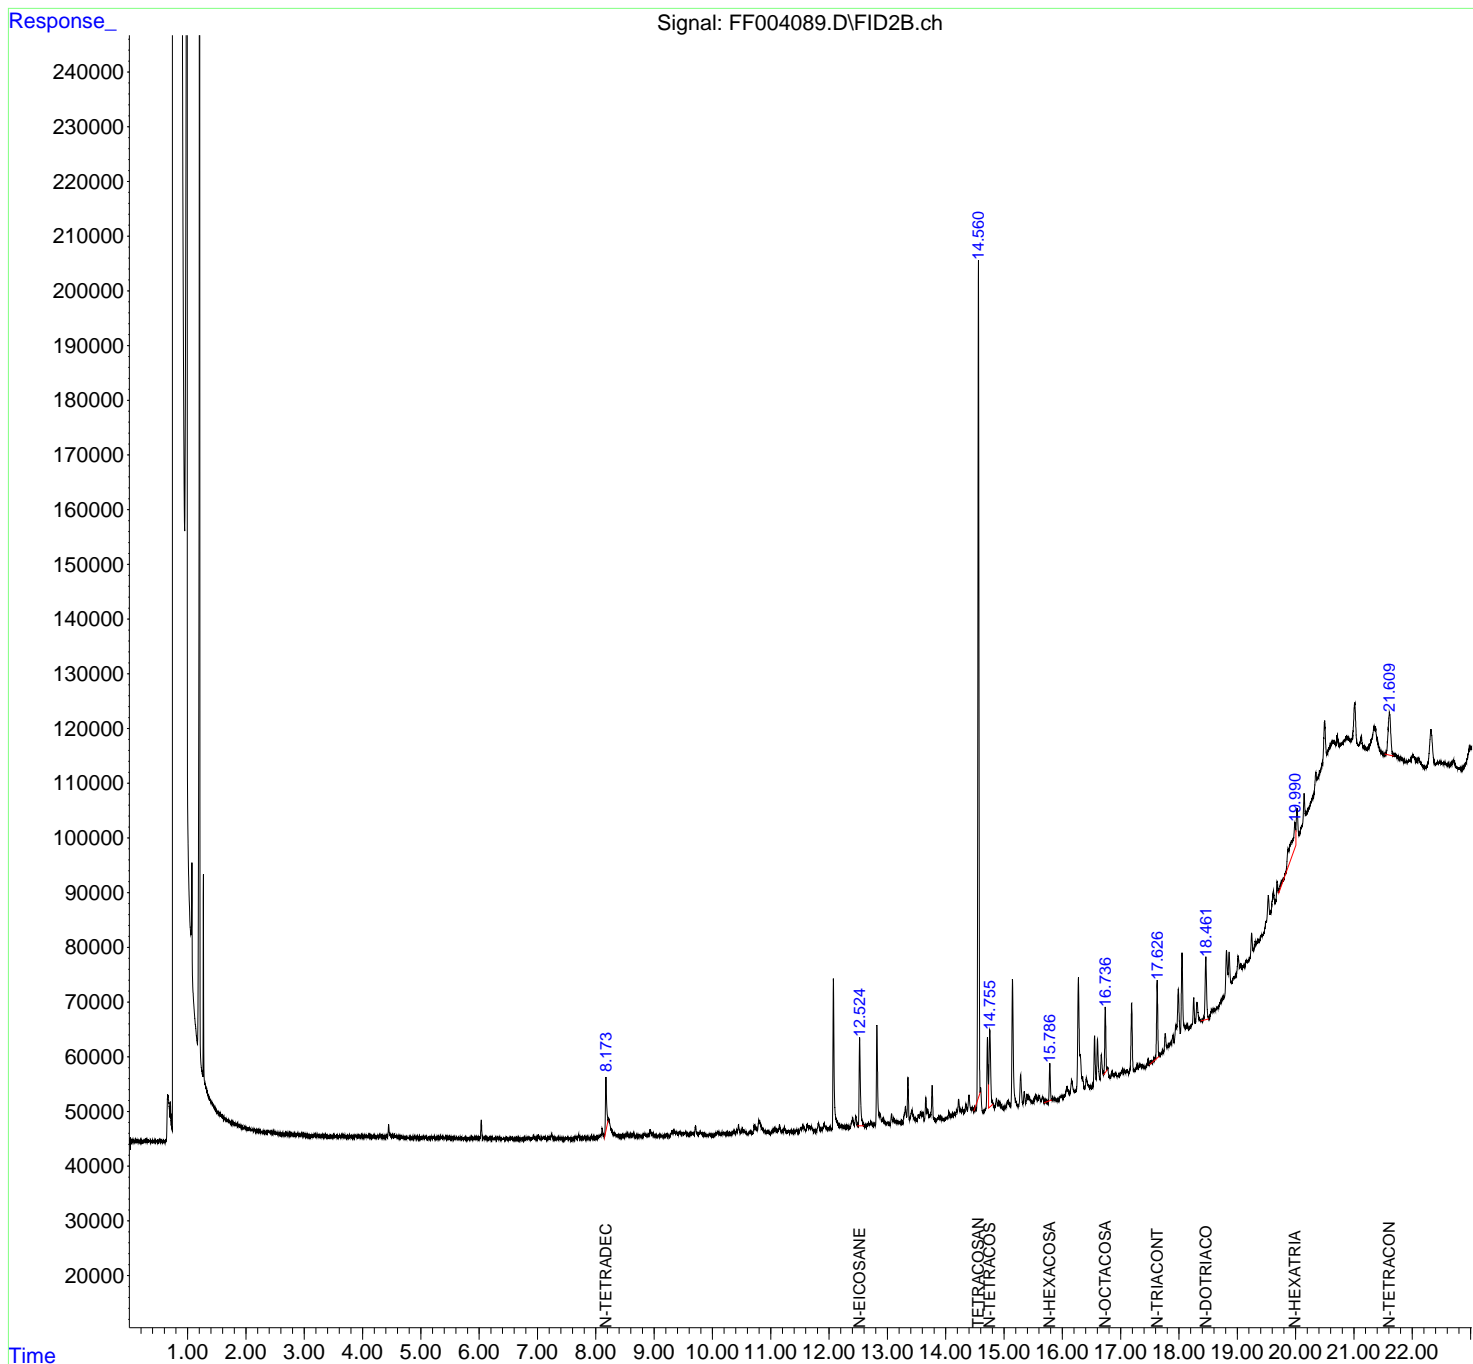


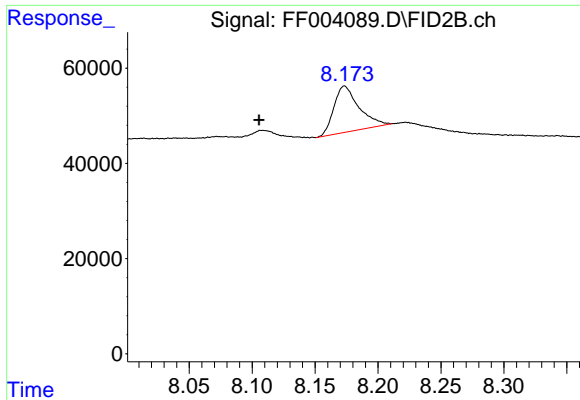


#4 N-TETRADECANE
 R.T.: 8.173 min
 Delta R.T.: 0.068 min
 Response: 134421
 Conc: 0.95 ug/ml

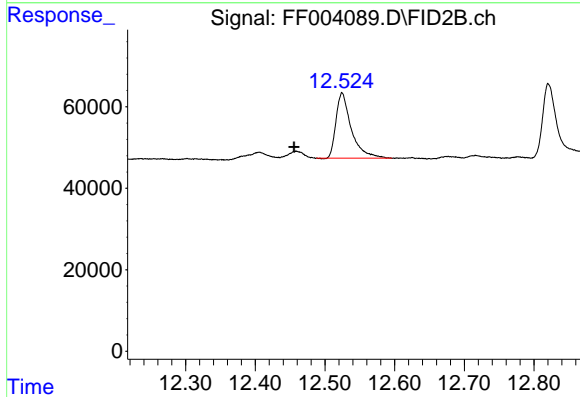


#7 N-EICOSANE
 R.T.: 12.525 min
 Delta R.T.: 0.069 min
 Response: 245101
 Conc: 1.63 ug/ml

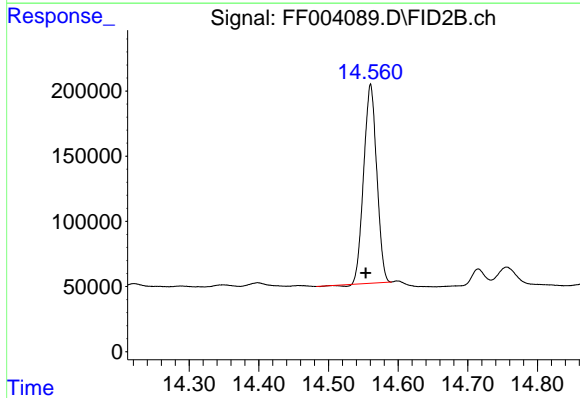


#9 TETRACOSANE-d50 (SURROGATE)
 R.T.: 14.561 min
 Delta R.T.: 0.007 min
 Response: 1981233
 Conc: 15.24 ug/ml

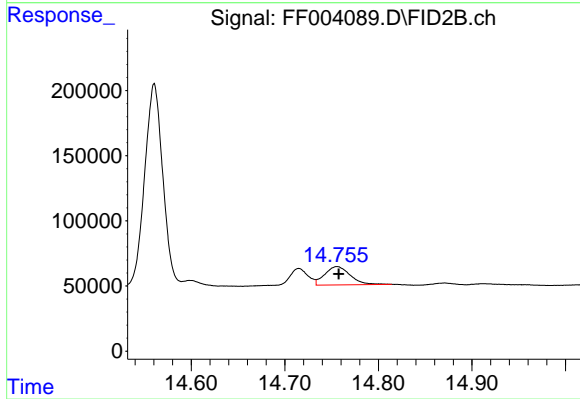


#10 N-TETRACOSANE
 R.T.: 14.756 min
 Delta R.T.: -0.002 min
 Response: 266425
 Conc: 1.81 ug/ml

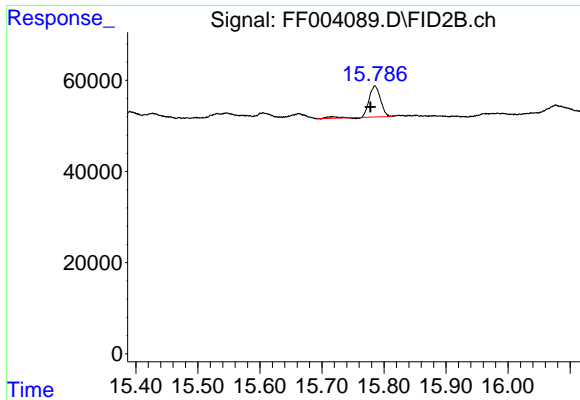


#11 N-HEXACOSANE
R.T.: 15.786 min
Delta R.T.: 0.007 min
Response: 88301
Conc: 0.61 ug/ml

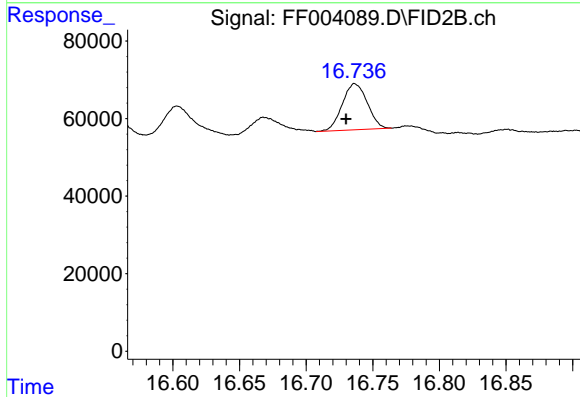


#12 N-OCTACOSANE
R.T.: 16.737 min
Delta R.T.: 0.006 min
Response: 154197
Conc: 1.07 ug/ml

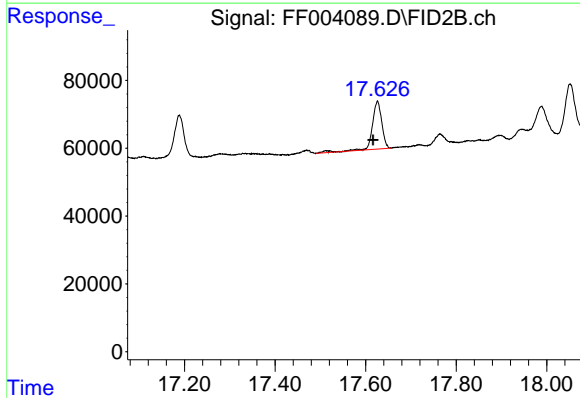

#13 N-TRIACONTANE
R.T.: 17.626 min
Delta R.T.: 0.010 min
Response: 206698
Conc: 1.45 ug/ml

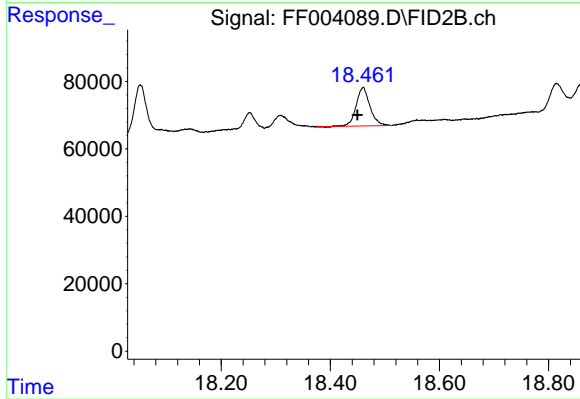


#14 N-DOTRIACONTANE
R.T.: 18.460 min
Delta R.T.: 0.010 min
Response: 200756
Conc: 1.42 ug/ml

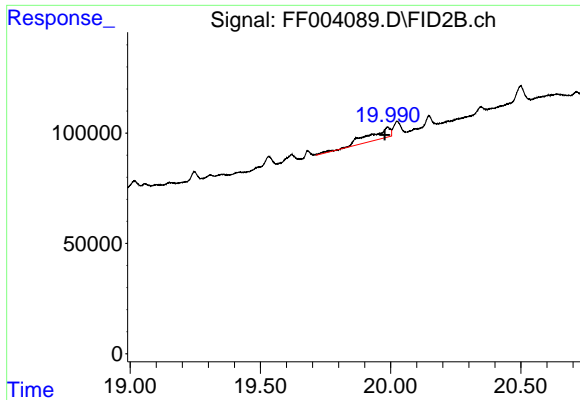

#16 N-HEXATRIACONTANE

R.T.: 19.988 min
Delta R.T.: 0.012 min
Response: 289972
Conc: 2.29 ug/ml

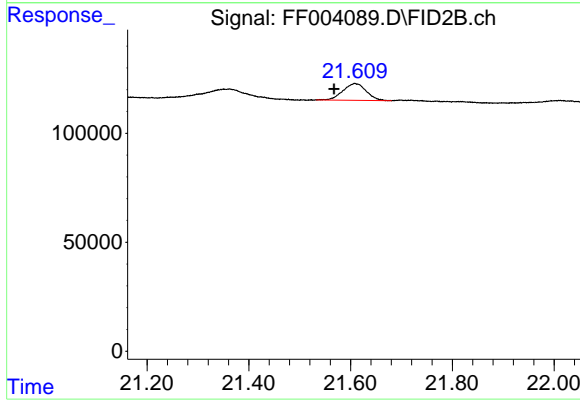

#18 N-TETRACONTANE

R.T.: 21.608 min
Delta R.T.: 0.041 min
Response: 243751
Conc: 2.01 ug/ml