

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040320\
 Data File : FF006768.D
 Signal(s) : FID2B.ch
 Acq On : 03 Apr 2020 14:36
 Operator : DD\AJ
 Sample : L2129-12 25X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 04 00:31:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
5) N-HEXADECANE	9.764	238335	1.626 ug/ml
6) N-OCTADECANE	11.265f	244146	1.652 ug/ml
7) N-EICOSANE	12.500	172255	1.159 ug/ml
8) N-DOCOSANE	13.682	222094	1.495 ug/ml
10) N-TETRACOSANE	14.768	1165998	7.889 ug/ml
11) N-HEXACOSANE	15.781	114138	0.788 ug/ml
12) N-OCTACOSANE	16.767	194450	1.358 ug/ml
13) N-TRIACONTANE	17.623	70583	0.499 ug/ml
14) N-DOTRIACONTANE	18.425	37236	0.276 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040320\
Data File : FF006768.D
Signal(s) : FID2B.ch
Acq On : 03 Apr 2020 14:36
Operator : DD\AJ
Sample : L2129-12 25X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 04 00:31:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

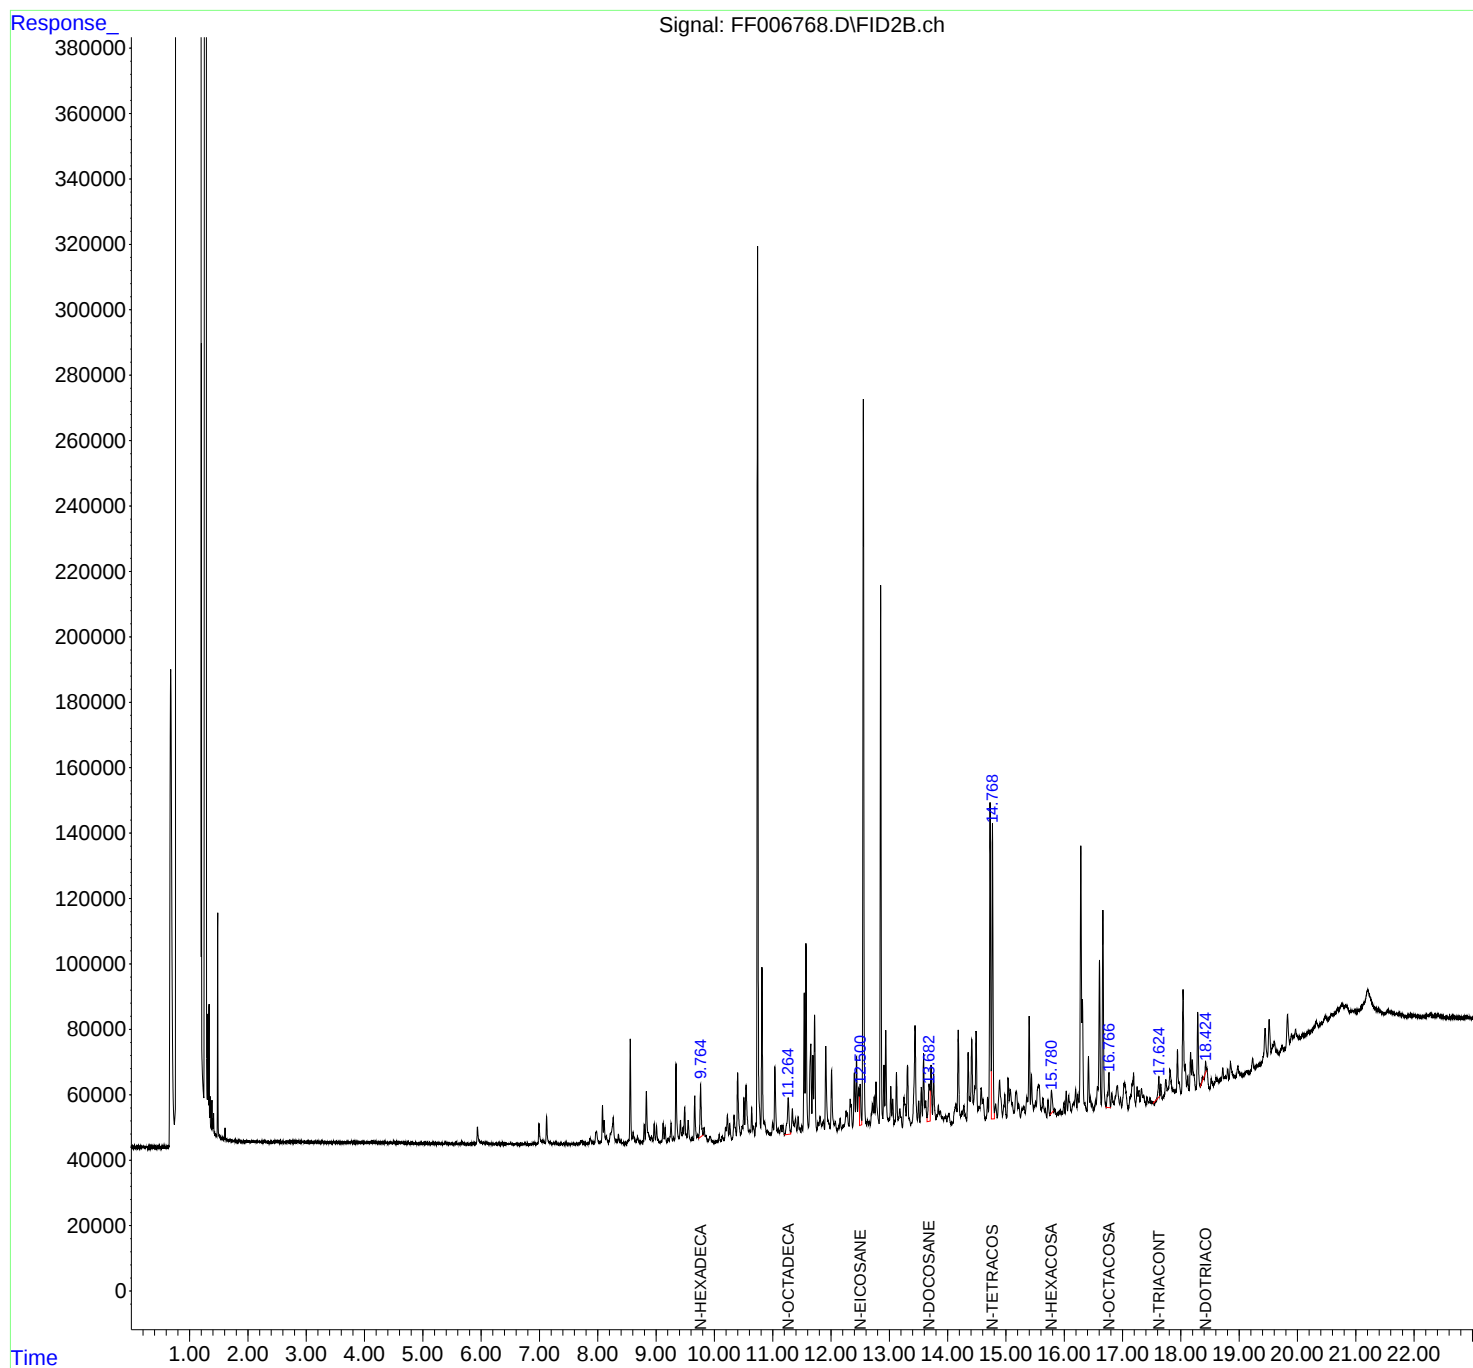

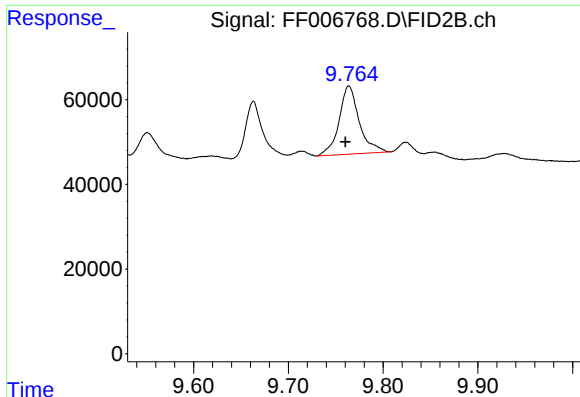


#5 N-HEXADECANE

R.T.: 9.764 min
Delta R.T.: 0.004 min
Response: 238335
Conc: 1.63 ug/ml

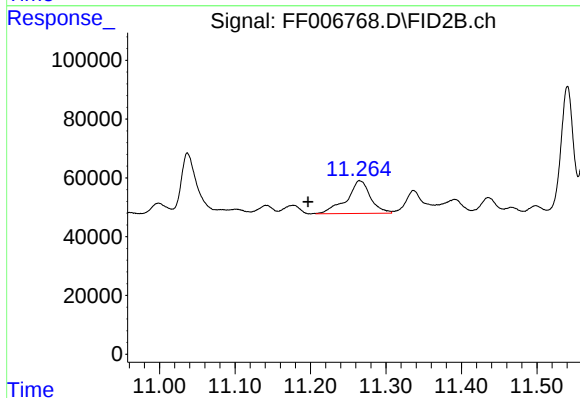


#6 N-OCTADECANE

R.T.: 11.265 min
Delta R.T.: 0.068 min
Response: 244146
Conc: 1.65 ug/ml

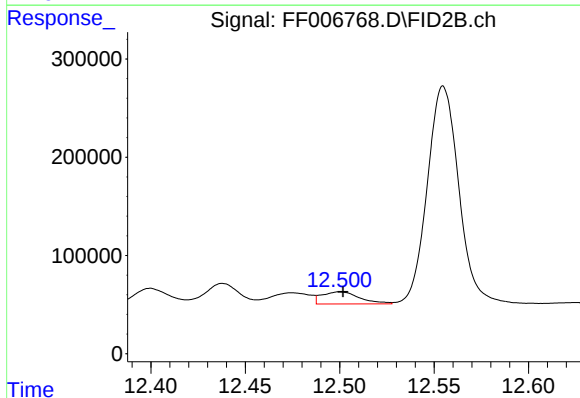


#7 N-EICOSANE

R.T.: 12.500 min
Delta R.T.: -0.001 min
Response: 172255
Conc: 1.16 ug/ml

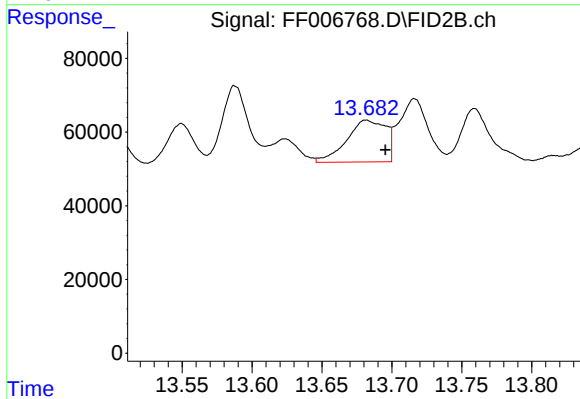


#8 N-DOCOSANE

R.T.: 13.682 min
Delta R.T.: -0.014 min
Response: 222094
Conc: 1.50 ug/ml

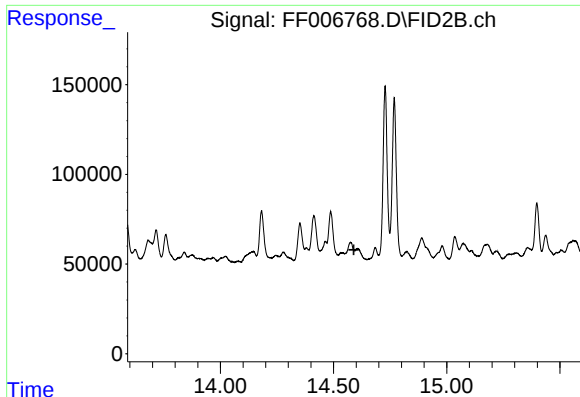


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.590 min
Response: 0
Conc: N.D.

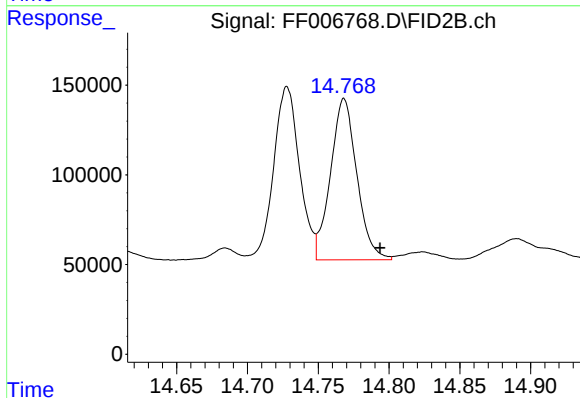


#10 N-TETRACOSANE

R.T.: 14.768 min
Delta R.T.: -0.025 min
Response: 116598
Conc: 7.89 ug/ml

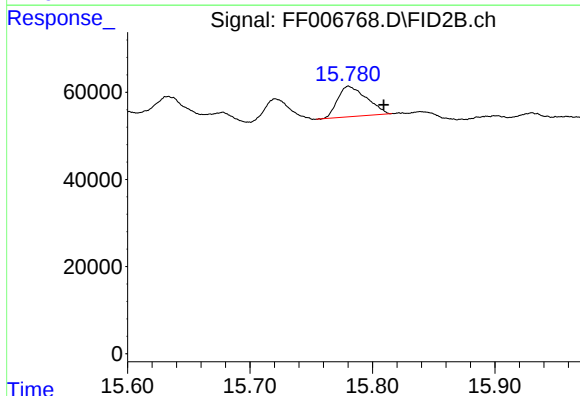


#11 N-HEXACOSANE

R.T.: 15.781 min
Delta R.T.: -0.029 min
Response: 114138
Conc: 0.79 ug/ml

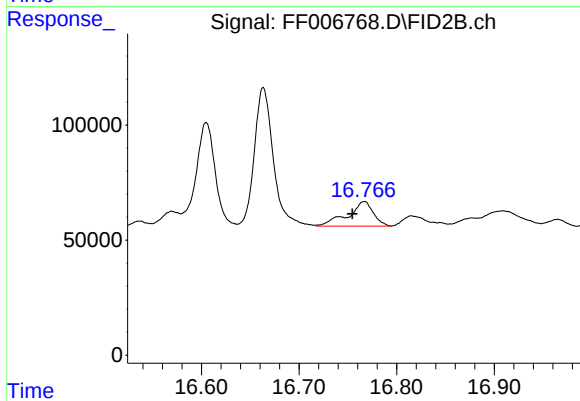


#12 N-OCTACOSANE

R.T.: 16.767 min
Delta R.T.: 0.012 min
Response: 194450
Conc: 1.36 ug/ml

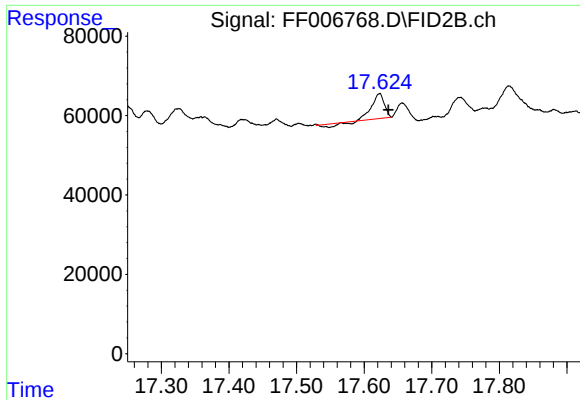

#13 N-TRIACONTANE

R.T.: 17.623 min
Delta R.T.: -0.013 min
Response: 70583
Conc: 0.50 ug/ml

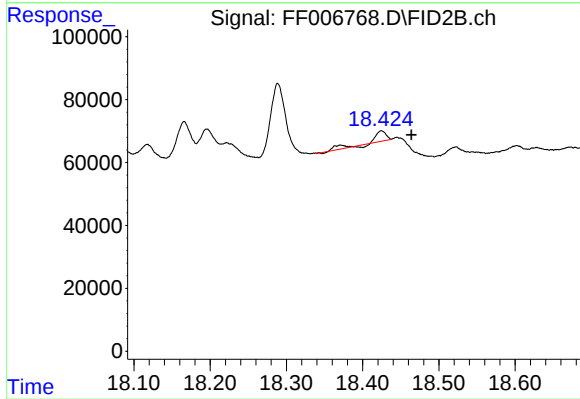

#14 N-DOTRIACONTANE

R.T.: 18.425 min
Delta R.T.: -0.039 min
Response: 37236
Conc: 0.28 ug/ml