

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040419\
 Data File : FF0404121.D
 Signal(s) : FID2B.ch
 Acq On : 04 Apr 2019 21:53
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 05 01:12:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.545	6005239	46.194 ug/ml
Target Compounds			
2) N-DECANE	4.293	7527803	55.624 ug/ml
3) N-DODECANE	6.312	7570359	53.959 ug/ml
4) N-TETRADECANE	8.102	7530076	52.958 ug/ml
5) N-HEXADECANE	9.700	7454995	50.370 ug/ml
6) N-OCTADECANE	11.140	7338352	48.728 ug/ml
7) N-EICOSANE	12.449	7123074	47.399 ug/ml
8) N-DOCOSANE	13.646	6945271	46.401 ug/ml
10) N-TETRACOSANE	14.749	6773592	45.986 ug/ml
11) N-HEXACOSANE	15.770	6701021	46.159 ug/ml
12) N-OCTACOSANE	16.720	6765347	47.050 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040419\
Data File : FF04121.D
Signal(s) : FID2B.ch
Acq On : 04 Apr 2019 21:53
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 05 01:12:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

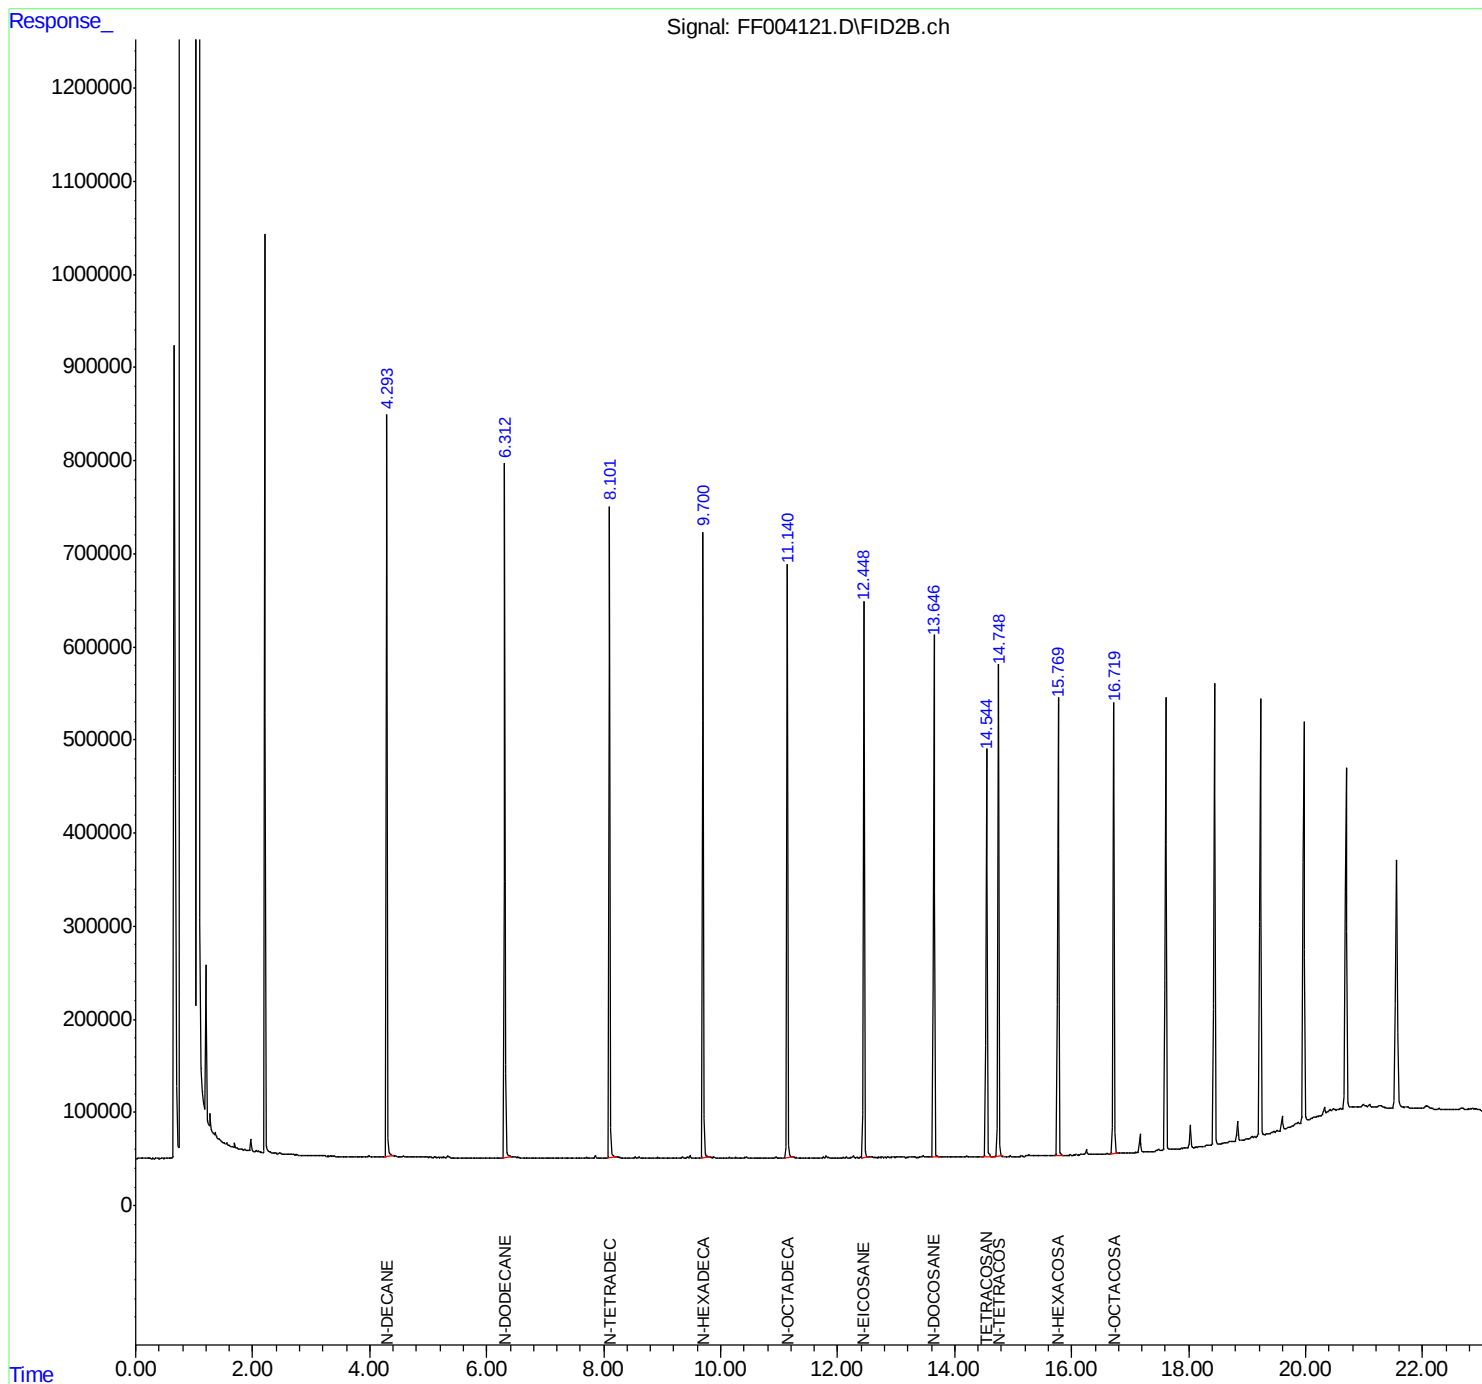

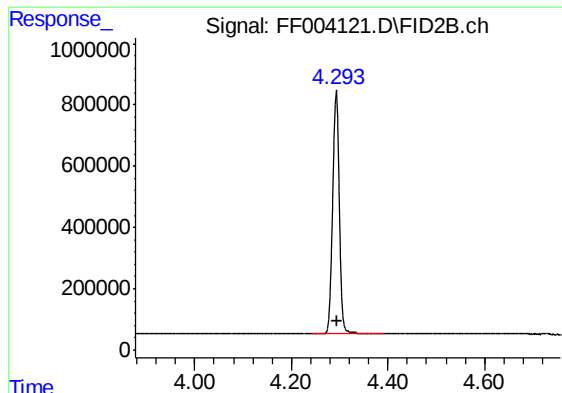


#2 N-DECANE

R.T.: 4.293 min
Delta R.T.: 0.000 min
Response: 7527803
Conc: 55.62 ug/ml

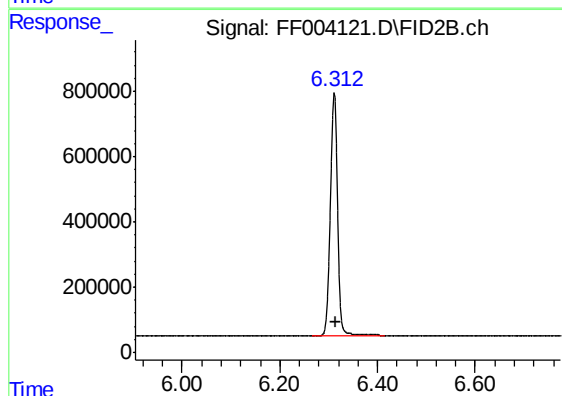


#3 N-DODECANE

R.T.: 6.312 min
Delta R.T.: -0.002 min
Response: 7570359
Conc: 53.96 ug/ml

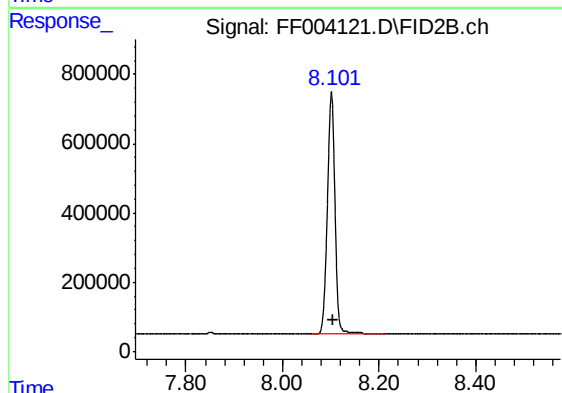


#4 N-TETRADECANE

R.T.: 8.102 min
Delta R.T.: -0.004 min
Response: 7530076
Conc: 52.96 ug/ml

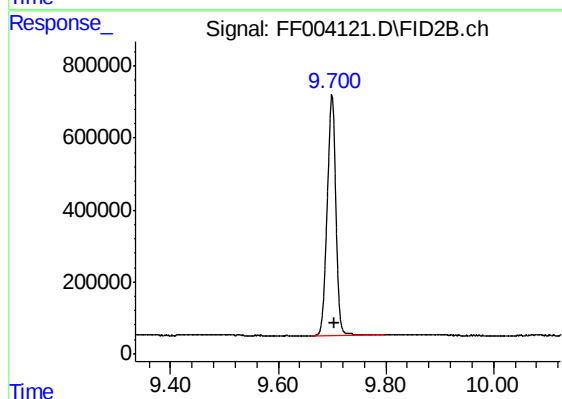


#5 N-HEXADECANE

R.T.: 9.700 min
Delta R.T.: -0.004 min
Response: 7454995
Conc: 50.37 ug/ml

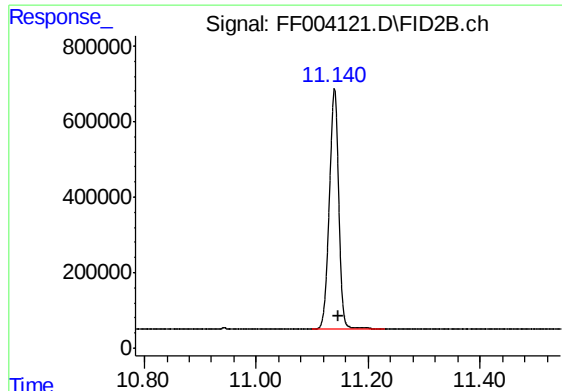


#6 N-OCTADECANE

R.T.: 11.140 min
Delta R.T.: -0.006 min
Response: 7338352
Conc: 48.73 ug/ml

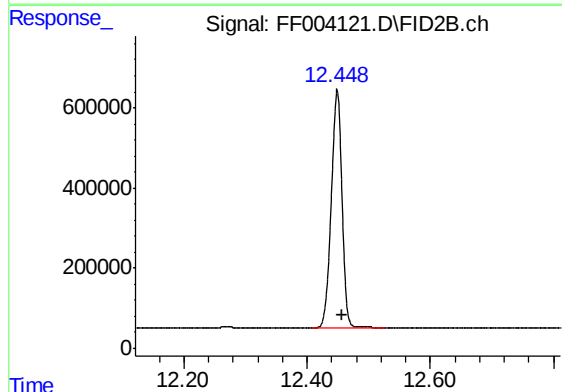


#7 N-EICOSANE

R.T.: 12.449 min
Delta R.T.: -0.007 min
Response: 7123074
Conc: 47.40 ug/ml

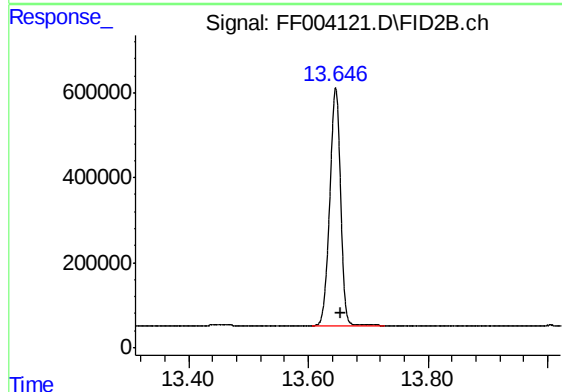


#8 N-DOCOSANE

R.T.: 13.646 min
Delta R.T.: -0.008 min
Response: 6945271
Conc: 46.40 ug/ml

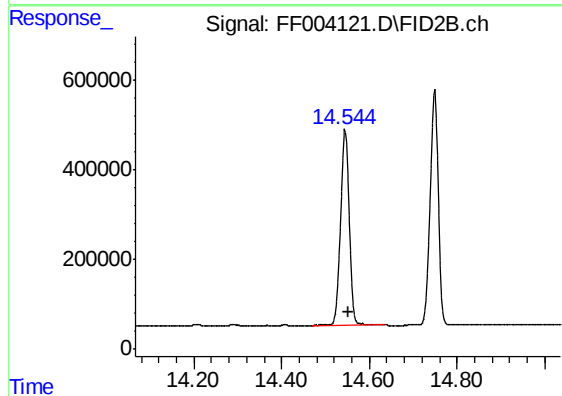


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.545 min
Delta R.T.: -0.009 min
Response: 6005239
Conc: 46.19 ug/ml

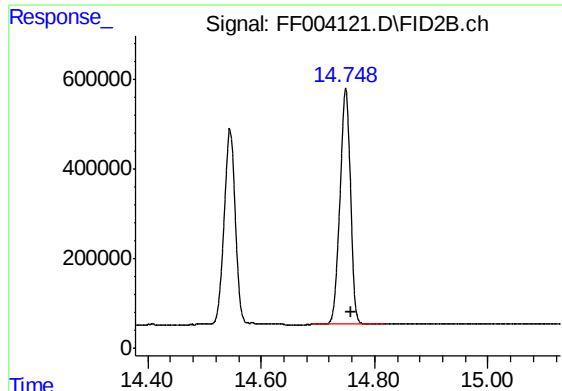


#10 N-TETRACOSANE

R.T.: 14.749 min
Delta R.T.: -0.009 min
Response: 6773592
Conc: 45.99 ug/ml

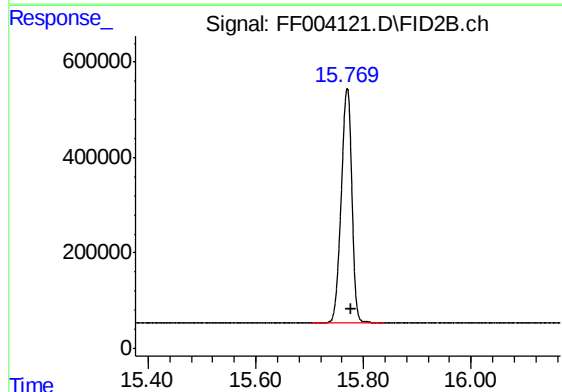

#11 N-HEXACOSANE

R.T.: 15.770 min
Delta R.T.: -0.008 min
Response: 6701021
Conc: 46.16 ug/ml

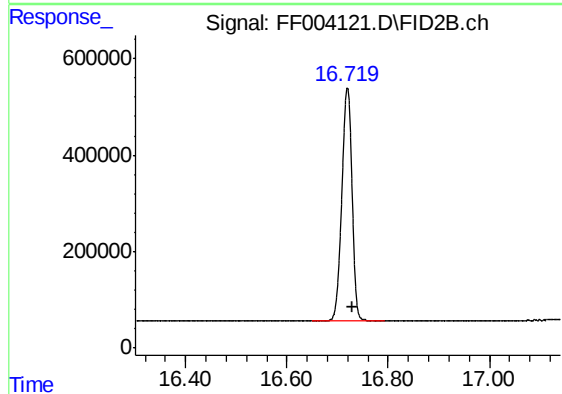

#12 N-OCTACOSANE

R.T.: 16.720 min
Delta R.T.: -0.011 min
Response: 6765347
Conc: 47.05 ug/ml