

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040422\
 Data File : FF010248.D
 Signal(s) : FID2B.ch
 Acq On : 04 Apr 2022 11:43
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 05 01:12:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
 Quant Title :
 QLast Update : Fri Apr 01 11:58:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.379	3185359	23.923 ug/ml
12)	N-OCTACOSANE	16.798	3300401	24.901 ug/ml
13)	N-TRIACONTANE	17.683	266892	2.021 ug/ml
14)	N-DOTRIACONTANE	18.516	170385	1.320 ug/ml
15)	N-TETRATRIACONTANE	19.298	131418	1.129 ug/ml
16)	N-HEXATRIACONTANE	20.038	193121	1.852 ug/ml
18)	N-TETRACONTANE	21.614	850995	9.715 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040422\
Data File : FF010248.D
Signal(s) : FID2B.ch
Acq On : 04 Apr 2022 11:43
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 05 01:12:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

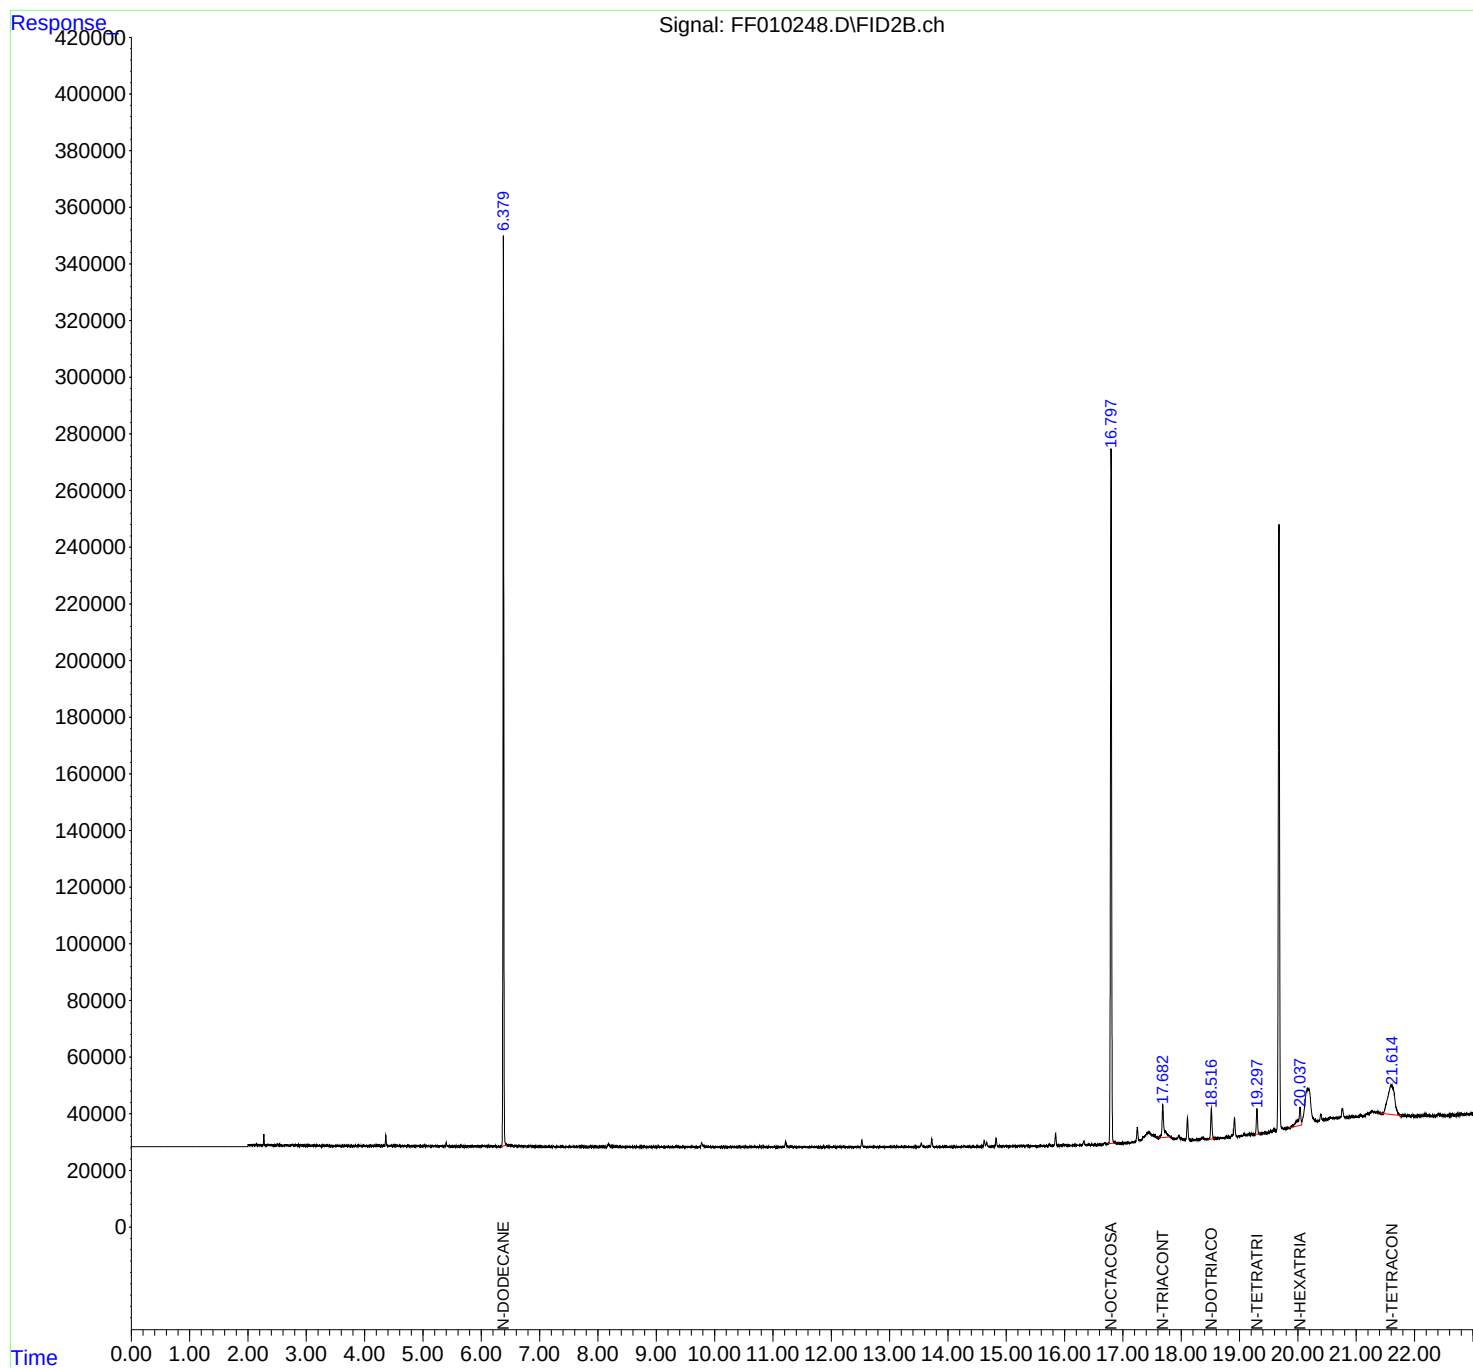


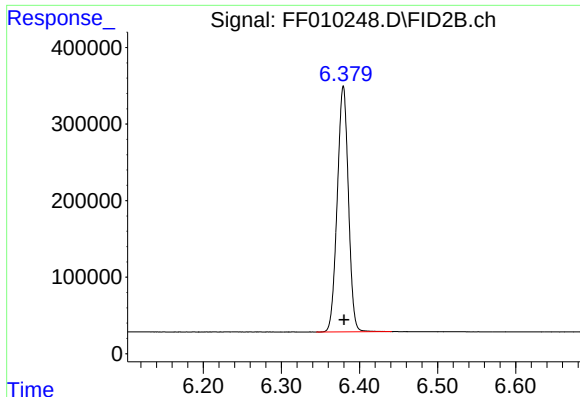

#3 N-DODECANE


R.T.: 6.379 min
Delta R.T.: -0.001 min
Response: 3185359
Conc: 23.92 ug/ml

Instrument :
FID_F
ClientSampleId :

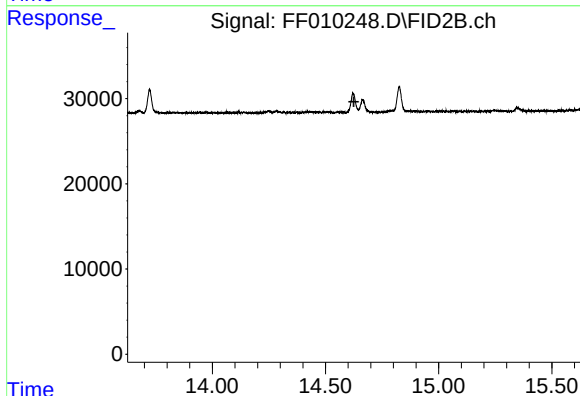


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.625 min
Response: 0
Conc: N.D.

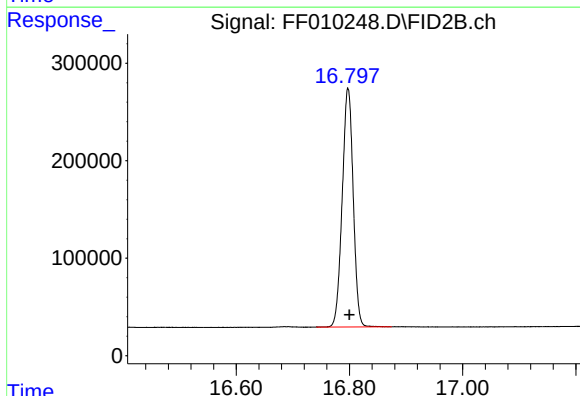


#12 N-OCTACOSANE

R.T.: 16.798 min
Delta R.T.: -0.002 min
Response: 3300401
Conc: 24.90 ug/ml

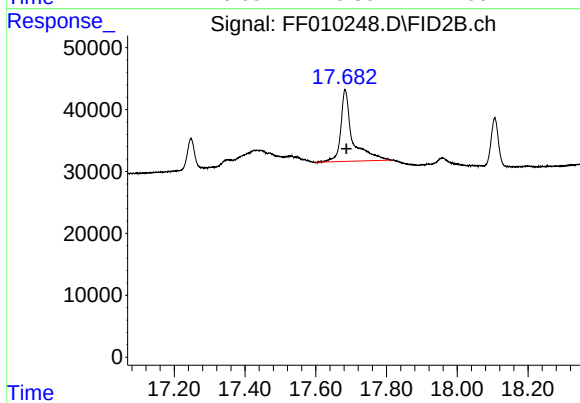

#13 N-TRIACONTANE


R.T.: 17.683 min
Delta R.T.: -0.004 min
Response: 266892
Conc: 2.02 ug/ml

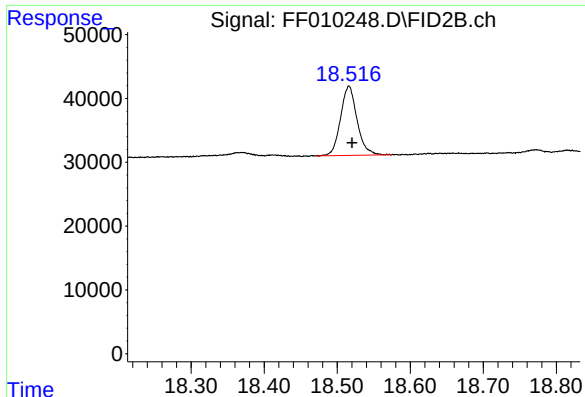

#14 N-DOTRIACONTANE


R.T.: 18.516 min
Delta R.T.: -0.004 min
Response: 170385
Conc: 1.32 ug/ml

Instrument :
FID_F
ClientSampleId :

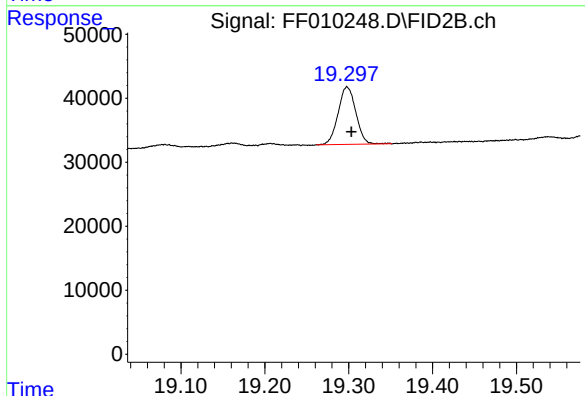


#15 N-TETRATRIACONTANE

R.T.: 19.298 min
Delta R.T.: -0.005 min
Response: 131418
Conc: 1.13 ug/ml

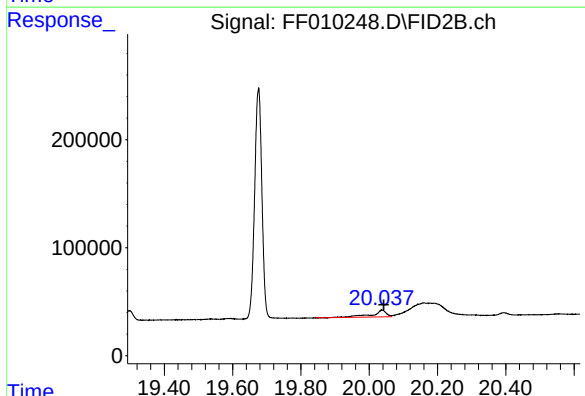

#16 N-HEXATRIACONTANE

R.T.: 20.038 min
Delta R.T.: -0.005 min
Response: 193121
Conc: 1.85 ug/ml

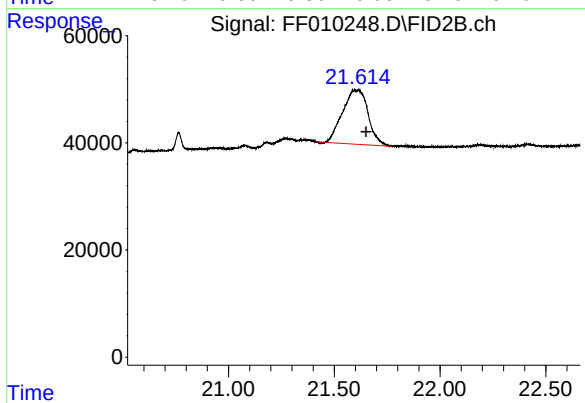

#18 N-TETRACONTANE

R.T.: 21.614 min
Delta R.T.: -0.037 min
Response: 850995
Conc: 9.71 ug/ml