

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040422\
 Data File : FF010251.D
 Signal(s) : FID2B.ch
 Acq On : 04 Apr 2022 13:46
 Operator : AJ\MA
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 05 01:12:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
 Quant Title :
 QLast Update : Fri Apr 01 11:58:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.626	5868904	49.100 ug/ml
Target Compounds			
1) N-OCTANE	2.271	6473264	49.395 ug/ml
2) N-DECANE	4.364	6710612	50.475 ug/ml
3) N-DODECANE	6.381	6709517	50.391 ug/ml
4) N-TETRADECANE	8.175	6703486	50.559 ug/ml
5) N-HEXADECANE	9.776	6709971	50.542 ug/ml
6) N-OCTADECANE	11.217	6867908	49.952 ug/ml
7) N-EICOSANE	12.528	6662952	49.593 ug/ml
8) N-DOCOSANE	13.726	6612658	49.422 ug/ml
10) N-TETRACOSANE	14.830	6595253	49.252 ug/ml
11) N-HEXACOSANE	15.851	6516354	49.129 ug/ml
12) N-OCTACOSANE	16.801	6480674	48.896 ug/ml
13) N-TRIACONTANE	17.688	6416488	48.597 ug/ml
14) N-DOTRIACONTANE	18.520	6203421	48.061 ug/ml
15) N-TETRATRIACONTANE	19.303	5692902	48.914 ug/ml
16) N-HEXATRIACONTANE	20.041	4970196	47.653 ug/ml
17) N-OCTATRIACONTANE	20.766	4502686	50.397 ug/ml
18) N-TETRACONTANE	21.649	4431925	50.593 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040422\
Data File : FF010251.D
Signal(s) : FID2B.ch
Acq On : 04 Apr 2022 13:46
Operator : AJ\MA
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 05 01:12:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

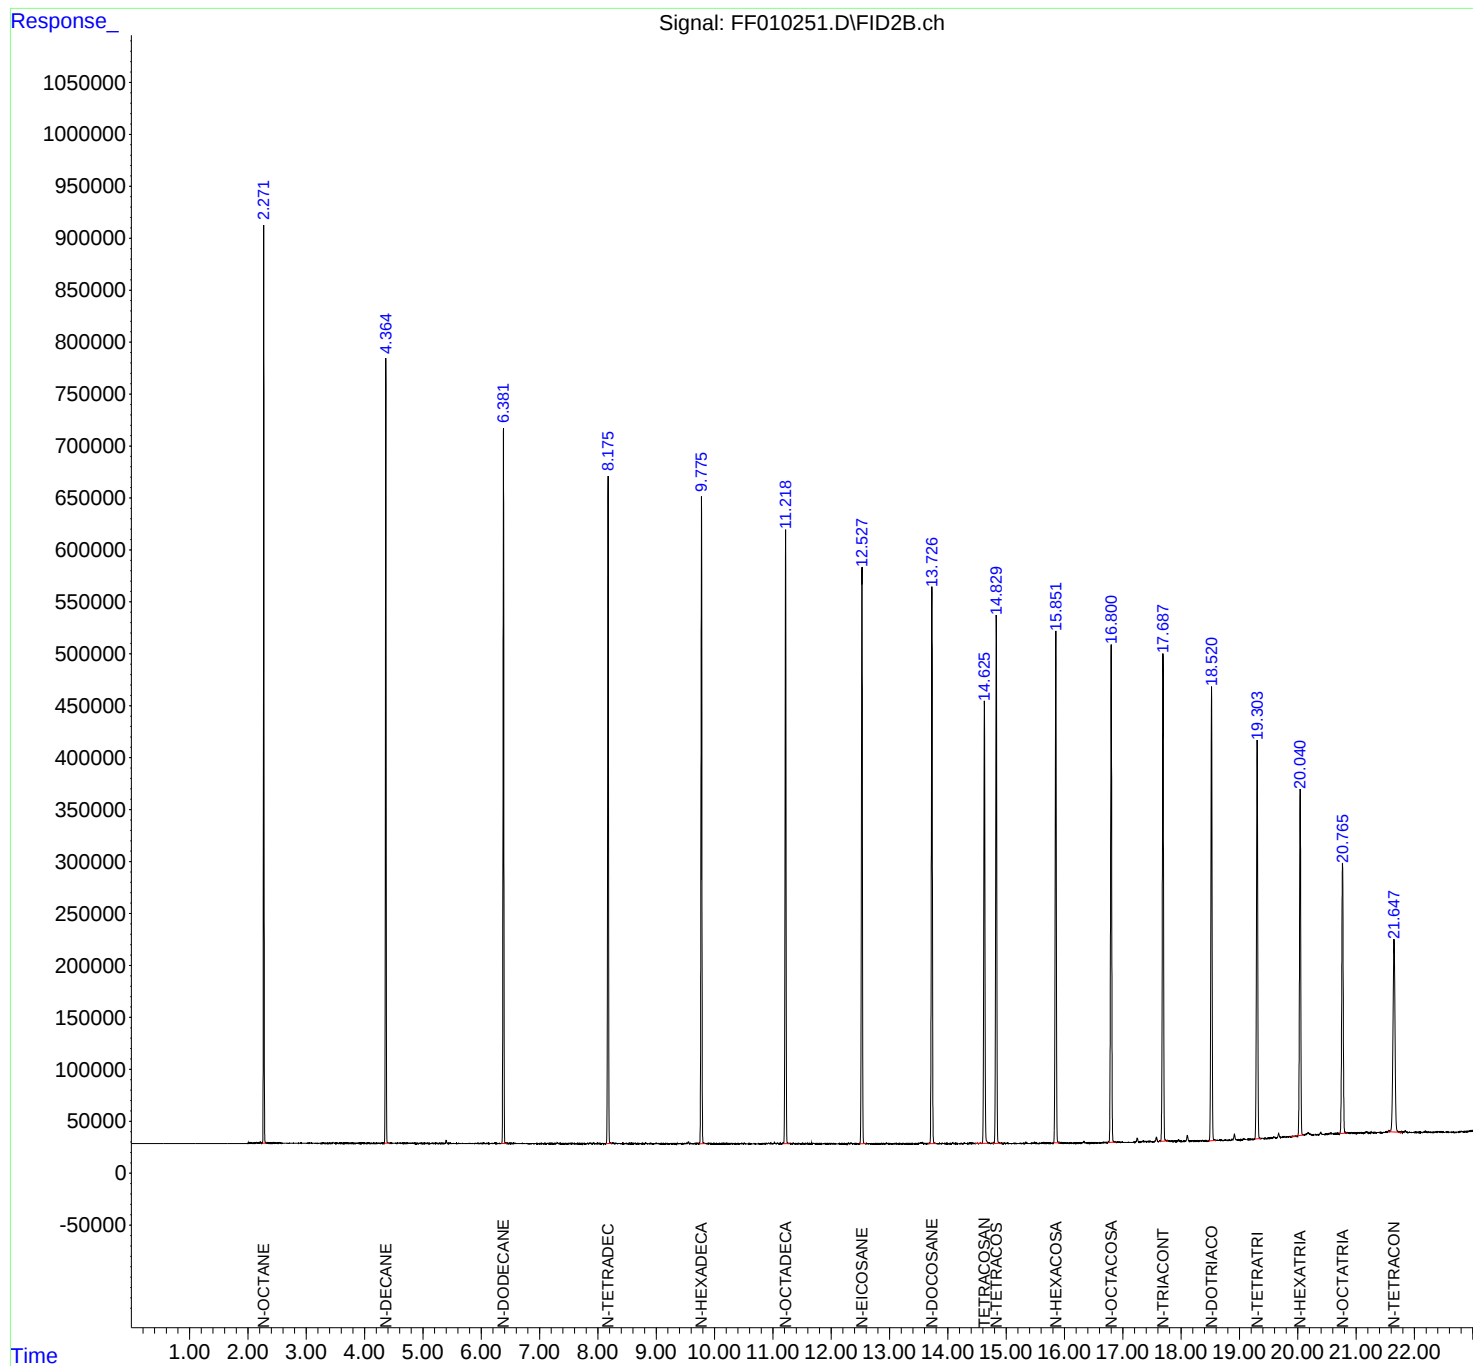


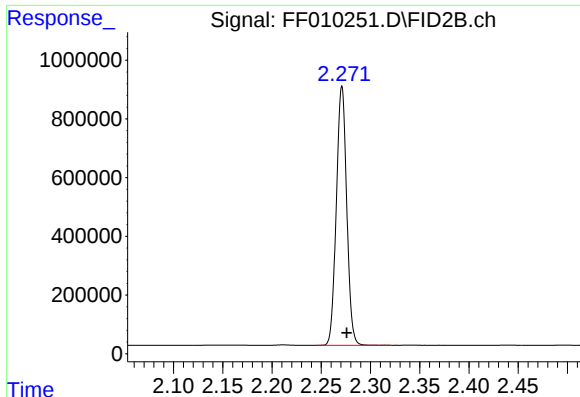

#1 N-OCTANE


R.T.: 2.271 min
Delta R.T.: -0.005 min
Response: 6473264
Conc: 49.40 ug/ml

Instrument :
FID_F
ClientSampleId :

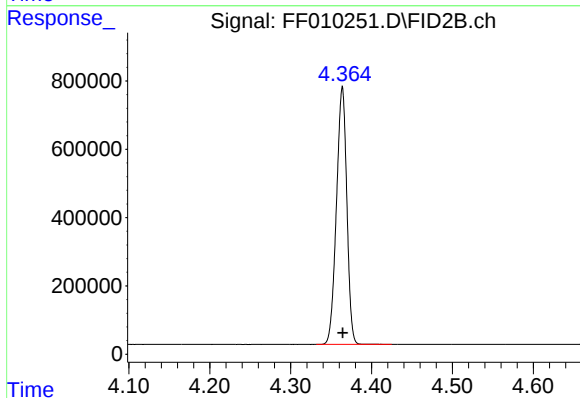


#2 N-DECANE

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 6710612
Conc: 50.48 ug/ml

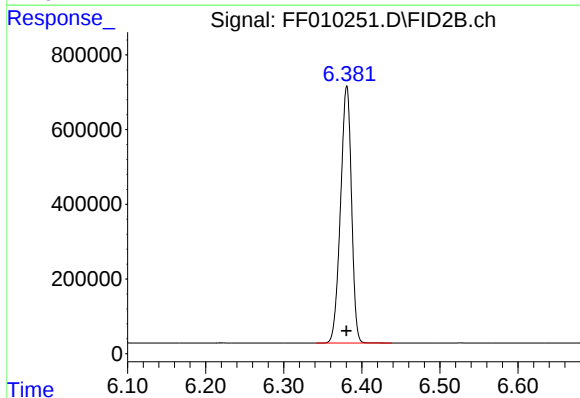


#3 N-DODECANE

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 6709517
Conc: 50.39 ug/ml

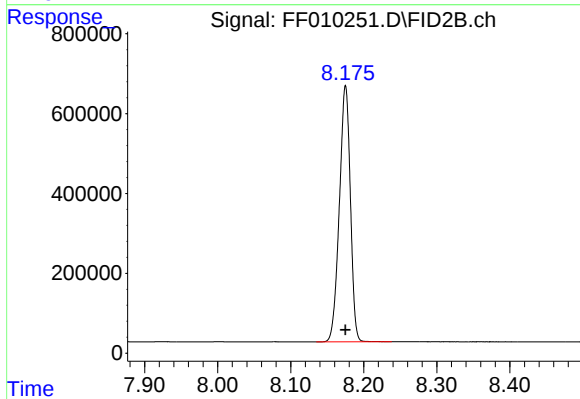

#4 N-TETRADECANE


R.T.: 8.175 min
Delta R.T.: 0.000 min
Response: 6703486
Conc: 50.56 ug/ml

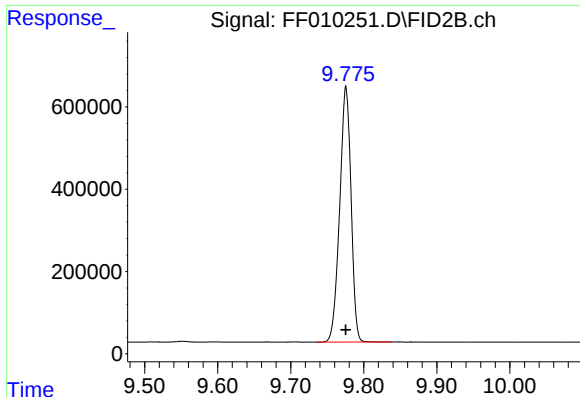

#5 N-HEXADECANE


R.T.: 9.776 min
Delta R.T.: 0.000 min
Response: 6709971
Conc: 50.54 ug/ml

Instrument :
FID_F
ClientSampleId :

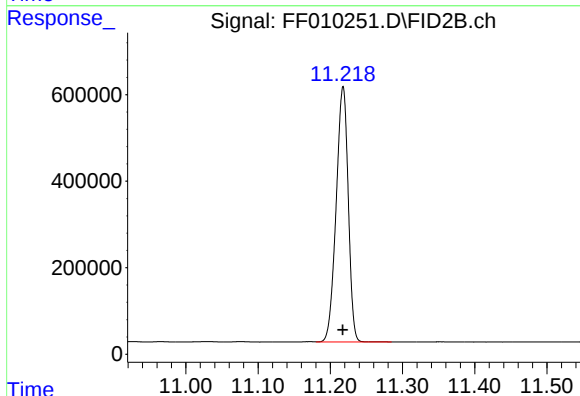


#6 N-OCTADECANE

R.T.: 11.217 min
Delta R.T.: 0.000 min
Response: 6867908
Conc: 49.95 ug/ml

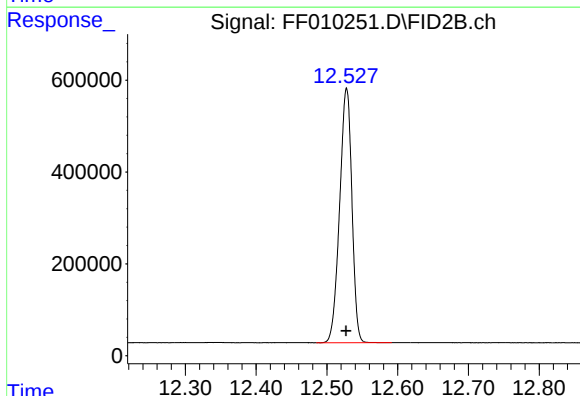


#7 N-EICOSANE

R.T.: 12.528 min
Delta R.T.: 0.000 min
Response: 6662952
Conc: 49.59 ug/ml

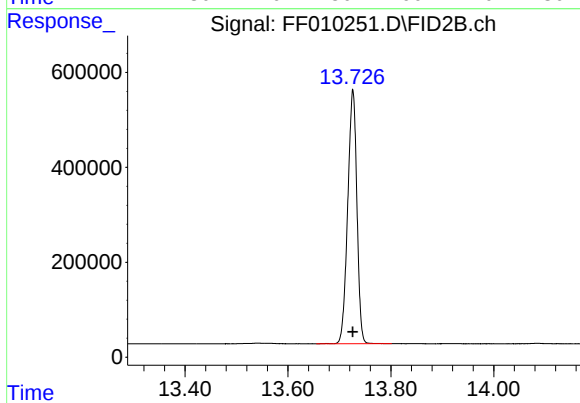

#8 N-DOCOSANE


R.T.: 13.726 min
Delta R.T.: 0.000 min
Response: 6612658
Conc: 49.42 ug/ml

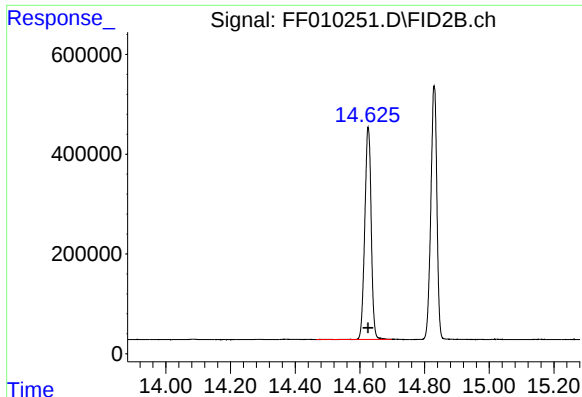

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.626 min
Delta R.T.: 0.000 min
Response: 5868904
Conc: 49.10 ug/ml

Instrument :
FID_F
ClientSampleId :

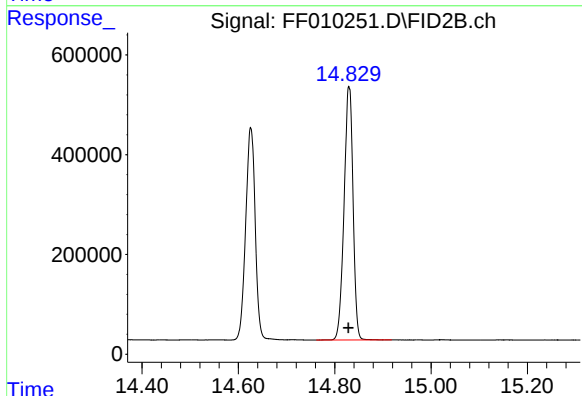


#10 N-TETRACOSANE

R.T.: 14.830 min
Delta R.T.: 0.001 min
Response: 6595253
Conc: 49.25 ug/ml

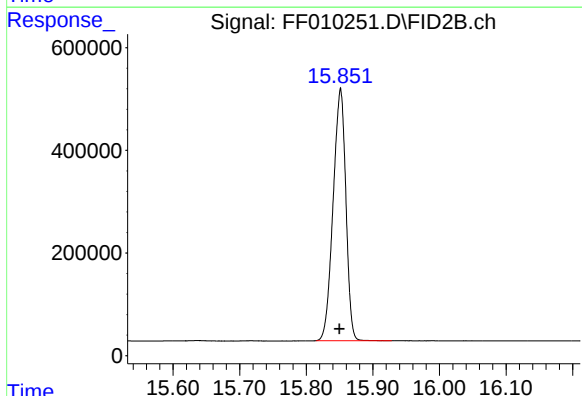


#11 N-HEXACOSANE

R.T.: 15.851 min
Delta R.T.: 0.001 min
Response: 6516354
Conc: 49.13 ug/ml

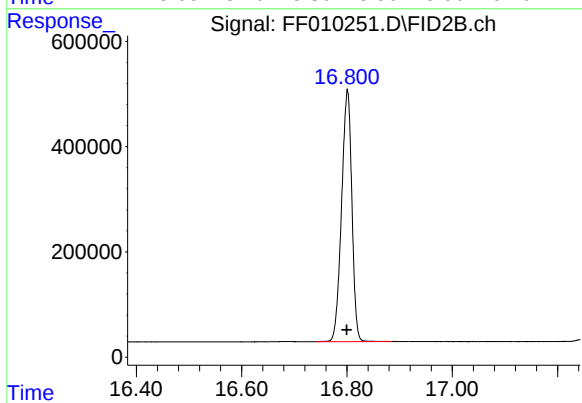

#12 N-OCTACOSANE


R.T.: 16.801 min
Delta R.T.: 0.001 min
Response: 6480674
Conc: 48.90 ug/ml

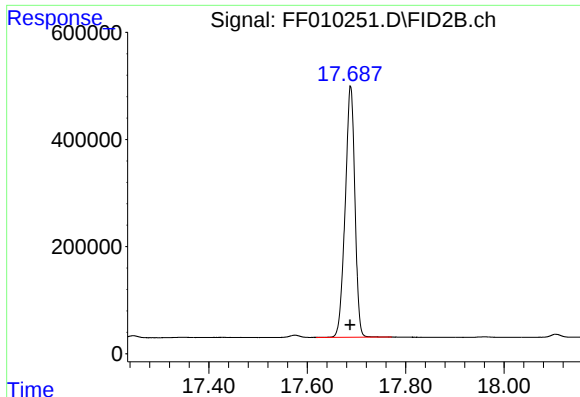

#13 N-TRIACONTANE


R.T.: 17.688 min
Delta R.T.: 0.001 min
Response: 6416488
Conc: 48.60 ug/ml

Instrument :
FID_F
ClientSampleId :

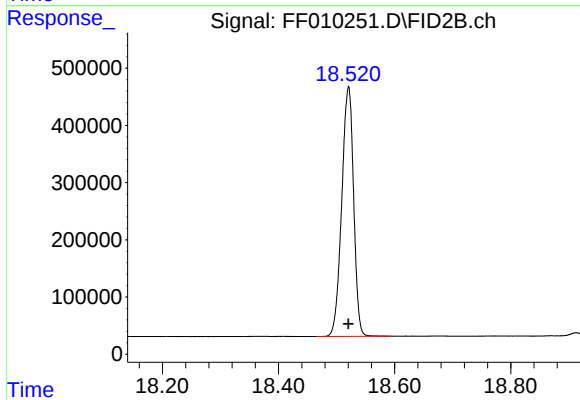


#14 N-DOTRIACONTANE

R.T.: 18.520 min
Delta R.T.: 0.000 min
Response: 6203421
Conc: 48.06 ug/ml

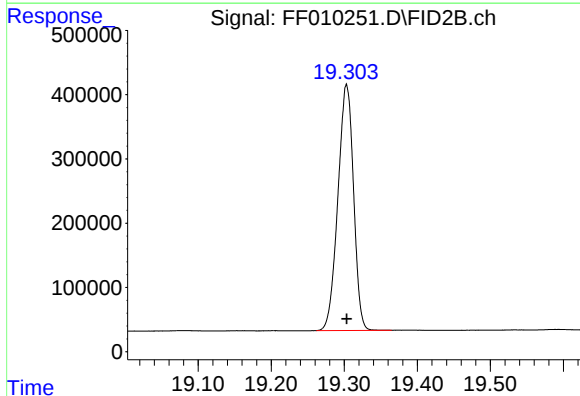


#15 N-TETRATRIACONTANE

R.T.: 19.303 min
Delta R.T.: 0.000 min
Response: 5692902
Conc: 48.91 ug/ml

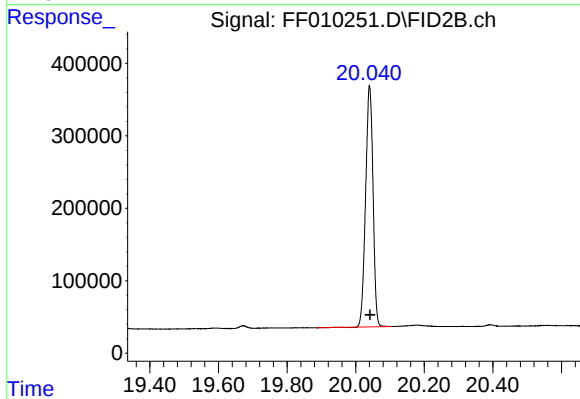

#16 N-HEXATRIACONTANE


R.T.: 20.041 min
Delta R.T.: -0.002 min
Response: 4970196
Conc: 47.65 ug/ml

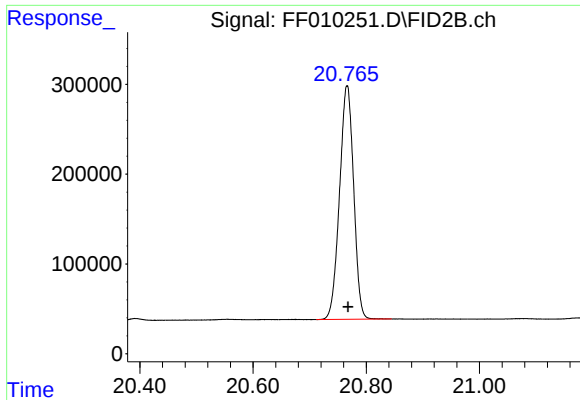

#17 N-OCTATRIACONTANE

R.T.: 20.766 min
Delta R.T.: -0.002 min
Response: 4502686
Conc: 50.40 ug/ml

Instrument :
FID_F
ClientSampleId :

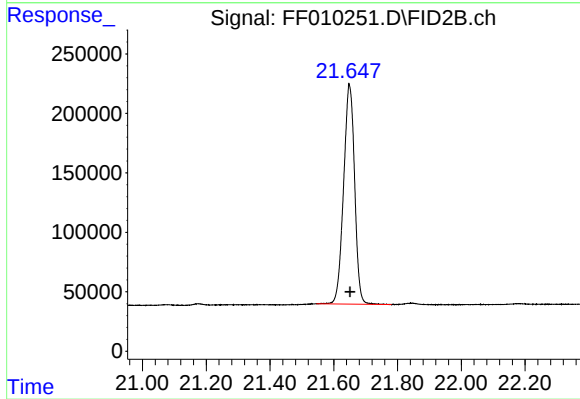

#18 N-TETRACONTANE

R.T.: 21.649 min
Delta R.T.: -0.002 min
Response: 4431925
Conc: 50.59 ug/ml