

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040422\
Data File : FF010254.D
Signal(s) : FID2B.ch
Acq On : 04 Apr 2022 15:16
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 05 01:12:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.380	3802206	28.556 ug/ml
12)	N-OCTACOSANE	16.799	3937363	29.707 ug/ml
13)	N-TRIACONTANE	17.684	160837	1.218 ug/ml
14)	N-DOTRIACONTANE	18.516	200740	1.555 ug/ml
15)	N-TETRATRIACONTANE	19.298	151243	1.299 ug/ml
16)	N-HEXATRIACONTANE	20.038	195706	1.876 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040422\
Data File : FF010254.D
Signal(s) : FID2B.ch
Acq On : 04 Apr 2022 15:16
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 05 01:12:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

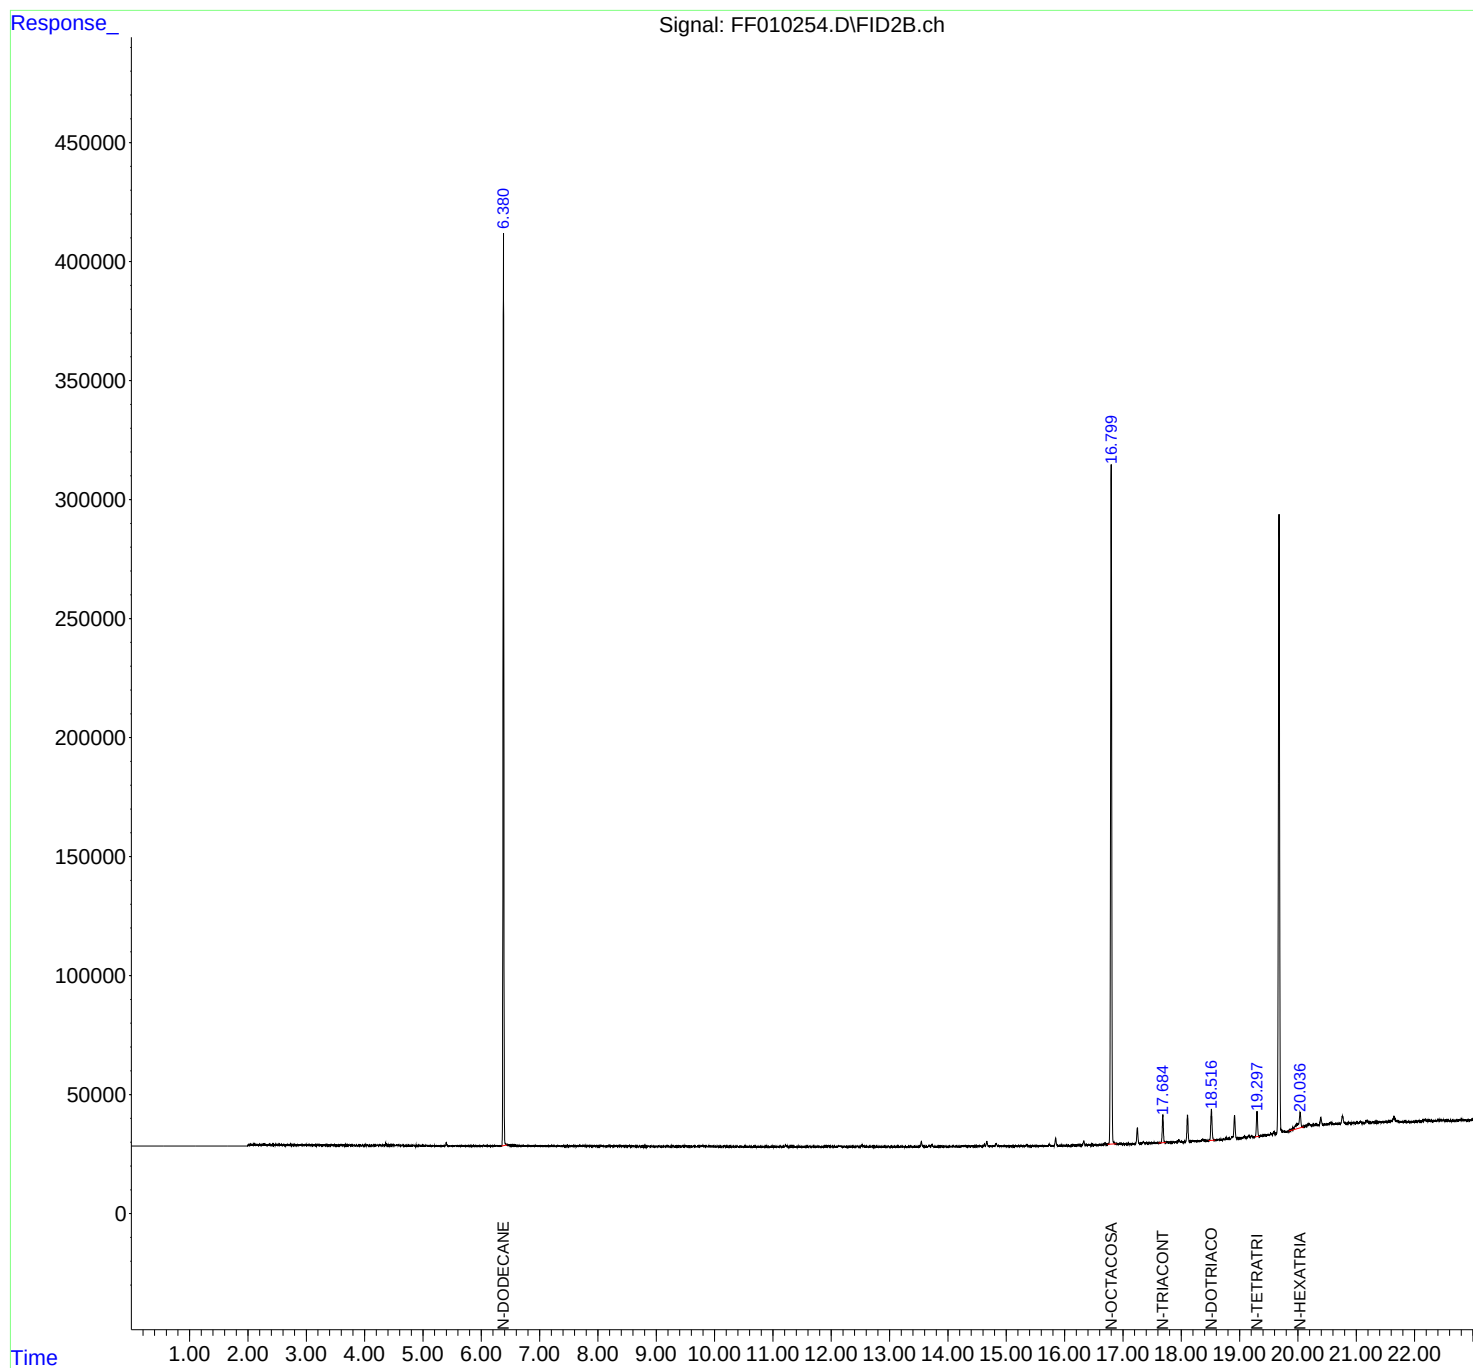


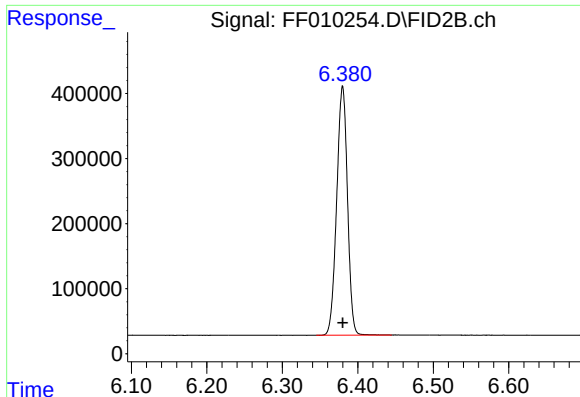

#3 N-DODECANE


R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 3802206
Conc: 28.56 ug/ml

Instrument :
FID_F
ClientSampleId :

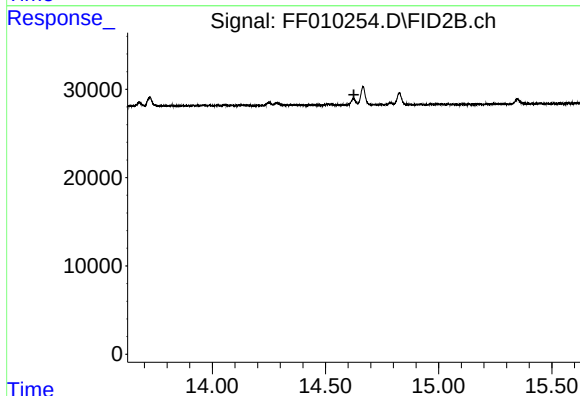


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.625 min
Response: 0
Conc: N.D.

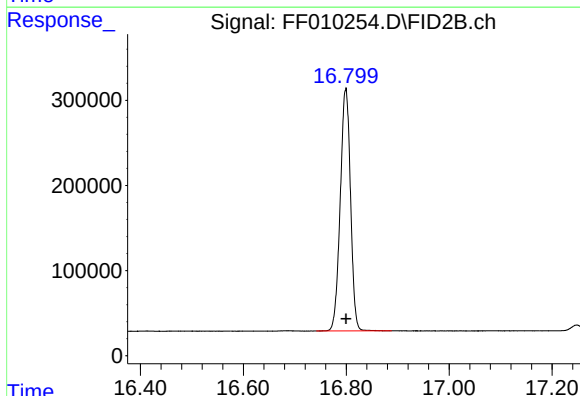


#12 N-OCTACOSANE

R.T.: 16.799 min
Delta R.T.: 0.000 min
Response: 3937363
Conc: 29.71 ug/ml

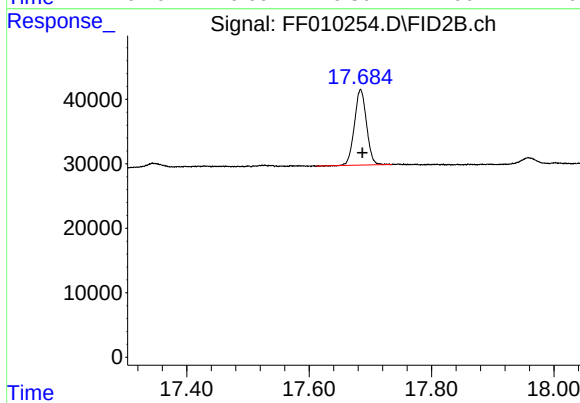

#13 N-TRIACONTANE


R.T.: 17.684 min
Delta R.T.: -0.003 min
Response: 160837
Conc: 1.22 ug/ml

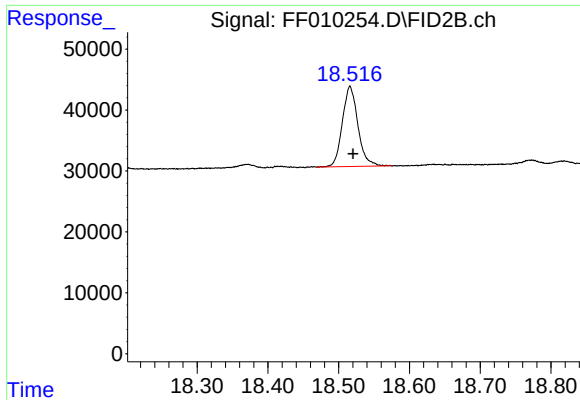

#14 N-DOTRIACONTANE


R.T.: 18.516 min
Delta R.T.: -0.004 min
Response: 200740
Conc: 1.56 ug/ml

Instrument :
FID_F
ClientSampleId :

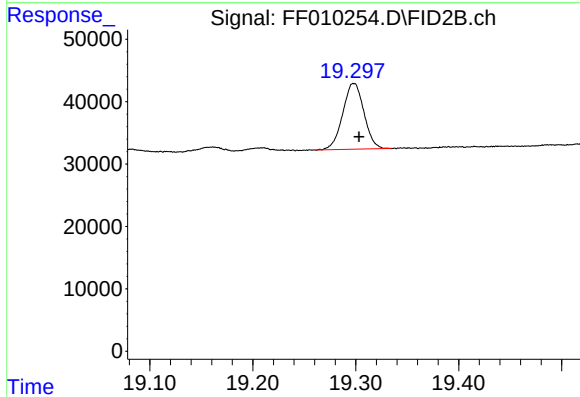

#15 N-TETRATRIACONTANE

R.T.: 19.298 min
Delta R.T.: -0.005 min
Response: 151243
Conc: 1.30 ug/ml

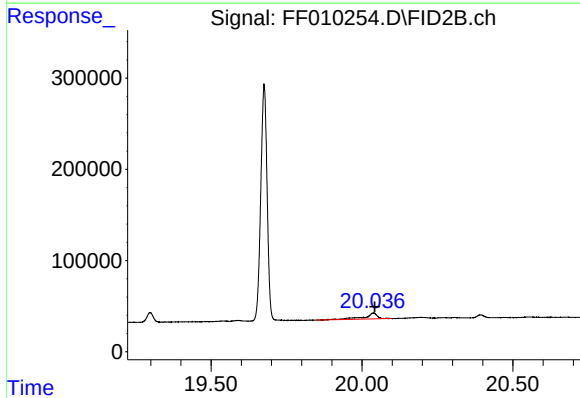

#16 N-HEXATRIACONTANE

R.T.: 20.038 min
Delta R.T.: -0.004 min
Response: 195706
Conc: 1.88 ug/ml